

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048350.D
 Acq On : 29 Apr 2022 11:04
 Operator : SY/MD
 Sample : VU0429WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV3	3334	3964	0.25%	0.032%
2	1.600	73	81	101	rBV	157270	203229	12.90%	1.657%
3	1.896	165	173	192	rVB	116756	182117	11.56%	1.484%
4	2.565	369	381	397	rBV	300553	493954	31.34%	4.026%
5	2.687	415	419	422	rBV3	440	321	0.02%	0.003%
6	2.732	430	433	435	rBV3	403	231	0.01%	0.002%
7	2.784	445	449	452	rBV4	586	603	0.04%	0.005%
8	2.874	473	477	481	rVV3	380	345	0.02%	0.003%
9	2.893	481	483	489	rVB3	304	249	0.02%	0.002%
10	2.960	499	504	505	rBV2	384	316	0.02%	0.003%
11	3.009	516	519	521	rBV2	301	183	0.01%	0.001%
12	3.044	523	530	540	rVB5	1125	2004	0.13%	0.016%
13	3.186	561	574	592	rBV2	7496	19273	1.22%	0.157%
14	3.395	636	639	642	rVB	287	208	0.01%	0.002%
15	3.414	642	645	649	rBV2	230	197	0.01%	0.002%
16	3.446	649	655	662	rVB2	267	392	0.02%	0.003%
17	3.478	662	665	670	rBV2	180	197	0.01%	0.002%
18	3.552	682	688	693	rVV2	279	326	0.02%	0.003%
19	3.700	729	734	737	rVV	210	243	0.02%	0.002%
20	3.903	794	797	800	rVB2	313	233	0.01%	0.002%
21	3.931	800	806	809	rBV2	218	258	0.02%	0.002%
22	4.128	864	867	875	rBV2	164	188	0.01%	0.002%
23	4.510	981	986	988	rBV	235	165	0.01%	0.001%
24	4.549	992	998	1000	rBV2	186	196	0.01%	0.002%
25	4.620	1006	1020	1049	rBV	183066	452827	28.74%	3.691%
26	4.861	1093	1095	1097	rBV2	322	198	0.01%	0.002%
27	5.002	1135	1139	1141	rBV	277	235	0.01%	0.002%
28	5.063	1141	1158	1180	rVV	284453	622761	39.52%	5.076%
29	5.333	1239	1242	1245	rVV3	394	320	0.02%	0.003%
30	5.433	1267	1273	1277	rBV2	299	367	0.02%	0.003%
31	5.462	1277	1282	1288	rVV2	249	419	0.03%	0.003%
32	5.726	1341	1364	1388	rBV2	583611	1575872	100.00%	12.845%
33	5.973	1436	1441	1450	rBV5	832	1293	0.08%	0.011%
34	6.044	1458	1463	1468	rBV3	669	671	0.04%	0.005%
35	6.115	1481	1485	1487	rBV3	496	394	0.03%	0.003%
36	6.173	1502	1503	1509	rVB2	247	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048350.D
 Acq On : 29 Apr 2022 11:04
 Operator : SY/MD
 Sample : VU0429WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1560	rBV	405145	771804	48.98%	6.291%
38	6.462	1588	1593	1596	rBV3	250	260	0.02%	0.002%
39	6.529	1605	1614	1623	rVV5	1734	2957	0.19%	0.024%
40	6.594	1631	1634	1636	rBV2	358	251	0.02%	0.002%
41	6.690	1647	1664	1686	rBV	373215	723446	45.91%	5.897%
42	6.796	1694	1697	1699	rBV2	587	423	0.03%	0.003%
43	7.054	1771	1777	1784	rBV3	453	745	0.05%	0.006%
44	7.176	1805	1815	1834	rVV4	3622	7699	0.49%	0.063%
45	7.301	1848	1854	1859	rBV2	203	281	0.02%	0.002%
46	7.375	1872	1877	1882	rBV2	247	385	0.02%	0.003%
47	7.449	1895	1900	1904	rBV	290	297	0.02%	0.002%
48	7.565	1923	1936	1951	rBV	198519	343875	21.82%	2.803%
49	7.690	1968	1975	1983	rVB4	1450	2514	0.16%	0.020%
50	7.726	1983	1986	1990	rVB3	317	251	0.02%	0.002%
51	7.758	1990	1996	1997	rBV	336	253	0.02%	0.002%
52	7.787	2001	2005	2008	rBV4	909	909	0.06%	0.007%
53	7.899	2025	2040	2056	rBV	710119	1239901	78.68%	10.106%
54	8.073	2089	2094	2097	rBV4	523	498	0.03%	0.004%
55	8.105	2102	2104	2107	rVB	370	209	0.01%	0.002%
56	8.124	2107	2110	2115	rVB2	268	227	0.01%	0.002%
57	8.179	2115	2127	2142	rBV	142998	234903	14.91%	1.915%
58	8.259	2150	2152	2154	rBV2	439	189	0.01%	0.002%
59	8.520	2229	2233	2237	rVB2	395	311	0.02%	0.003%
60	8.565	2241	2247	2248	rBV2	454	380	0.02%	0.003%
61	8.635	2256	2269	2309	rBV	598259	1088099	69.05%	8.869%
62	8.857	2335	2338	2341	rBV2	331	257	0.02%	0.002%
63	8.934	2359	2362	2365	rBV2	372	322	0.02%	0.003%
64	8.983	2374	2377	2379	rBV2	252	175	0.01%	0.001%
65	9.205	2442	2446	2450	rBV2	346	323	0.02%	0.003%
66	9.417	2496	2512	2541	rBV	601787	1000160	63.47%	8.152%
67	9.574	2557	2561	2567	rVB2	502	491	0.03%	0.004%
68	9.632	2573	2579	2583	rBV3	347	524	0.03%	0.004%
69	9.693	2593	2598	2600	rBV2	806	797	0.05%	0.006%
70	9.806	2628	2633	2637	rBV2	409	384	0.02%	0.003%
71	9.941	2673	2675	2681	rVB	263	158	0.01%	0.001%
72	10.060	2709	2712	2716	rBV2	167	182	0.01%	0.001%
73	10.102	2719	2725	2726	rBV3	349	335	0.02%	0.003%
74	10.491	2839	2846	2851	rBV2	379	609	0.04%	0.005%
75	10.671	2895	2902	2910	rVB	1684	2140	0.14%	0.017%
76	10.758	2916	2929	2947	rBV	655909	1053610	66.86%	8.588%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048350.D
 Acq On : 29 Apr 2022 11:04
 Operator : SY/MD
 Sample : VU0429WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.864	2959	2962	2967	rBV2	423	354	0.02%	0.003%
78	10.889	2967	2970	2973	rVV2	475	349	0.02%	0.003%
79	10.902	2973	2974	2980	rVB2	351	264	0.02%	0.002%
80	10.970	2993	2995	3001	rVB	267	220	0.01%	0.002%
81	11.002	3001	3005	3008	rBV3	488	401	0.03%	0.003%
82	11.086	3027	3031	3034	rBV3	552	424	0.03%	0.003%
83	11.465	3138	3149	3158	rBV4	1379	3046	0.19%	0.025%
84	11.812	3245	3257	3280	rBV	605469	973663	61.79%	7.936%
85	11.944	3292	3298	3301	rBV3	835	935	0.06%	0.008%
86	11.970	3304	3306	3313	rVB6	1320	1242	0.08%	0.010%
87	12.012	3316	3319	3320	rBV2	421	233	0.01%	0.002%
88	12.095	3341	3345	3347	rBV2	306	224	0.01%	0.002%
89	12.195	3361	3376	3399	rBV	740213	1221985	77.54%	9.960%
90	12.346	3420	3423	3428	rBV3	442	443	0.03%	0.004%
91	12.381	3431	3434	3436	rVB2	405	252	0.02%	0.002%
92	12.420	3441	3446	3447	rBV	379	341	0.02%	0.003%
93	12.732	3540	3543	3544	rBV	469	235	0.01%	0.002%
94	13.057	3637	3644	3651	rBV2	542	960	0.06%	0.008%
95	13.851	3884	3891	3901	rVB4	2139	3295	0.21%	0.027%
96	14.095	3958	3967	3980	rBV3	4190	7937	0.50%	0.065%
97	14.336	4032	4042	4050	rBV3	2641	4170	0.26%	0.034%
98	14.449	4075	4077	4086	rBV	388	499	0.03%	0.004%
99	15.015	4251	4253	4255	rBV	416	238	0.02%	0.002%
100	15.417	4376	4378	4380	rBV3	599	350	0.02%	0.003%




Sum of corrected areas: 12268502

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
Data File : VU048350.D
Acq On : 29 Apr 2022 11:04
Operator : SY/MD
Sample : VU0429WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

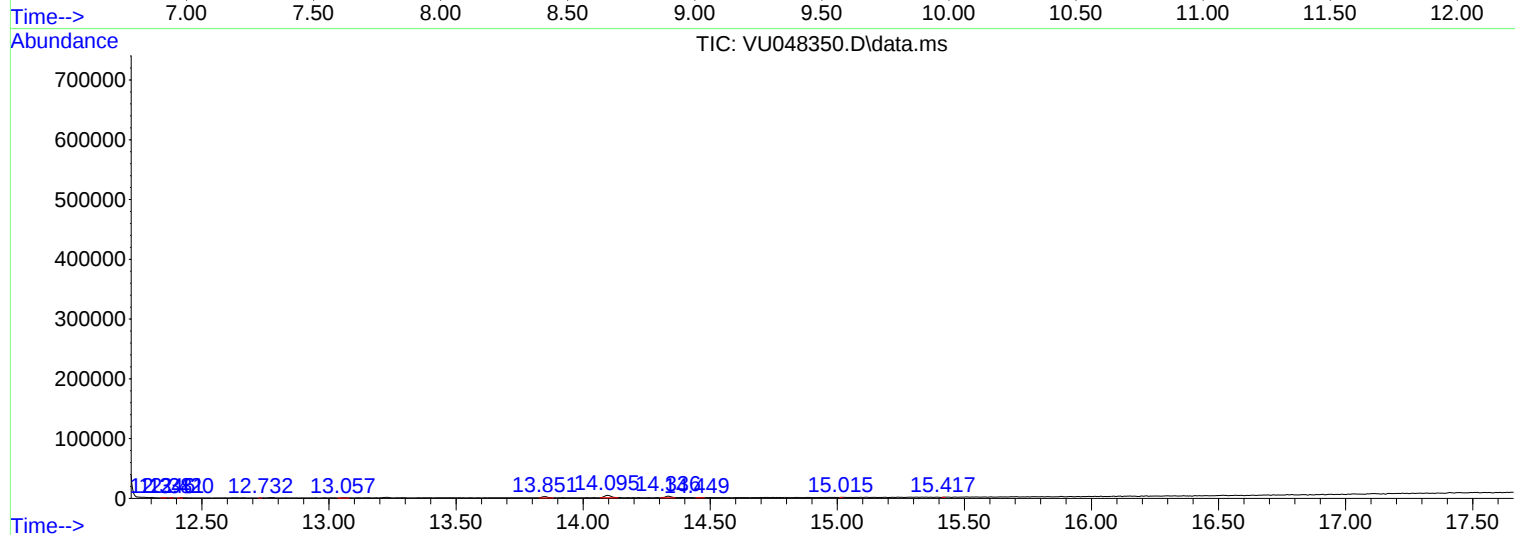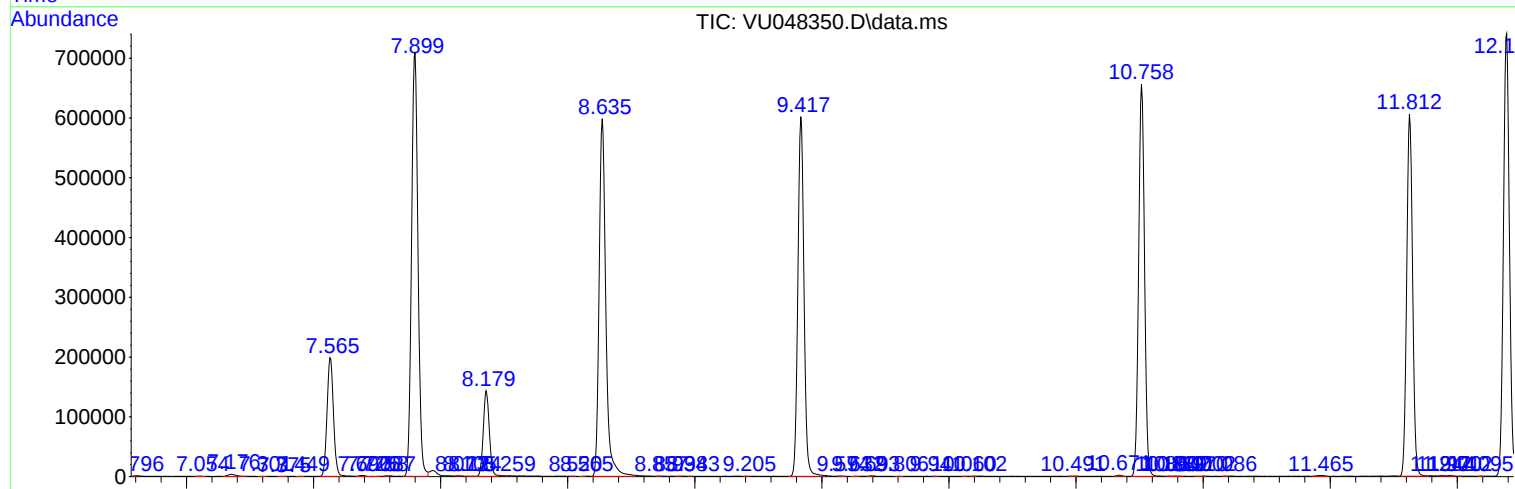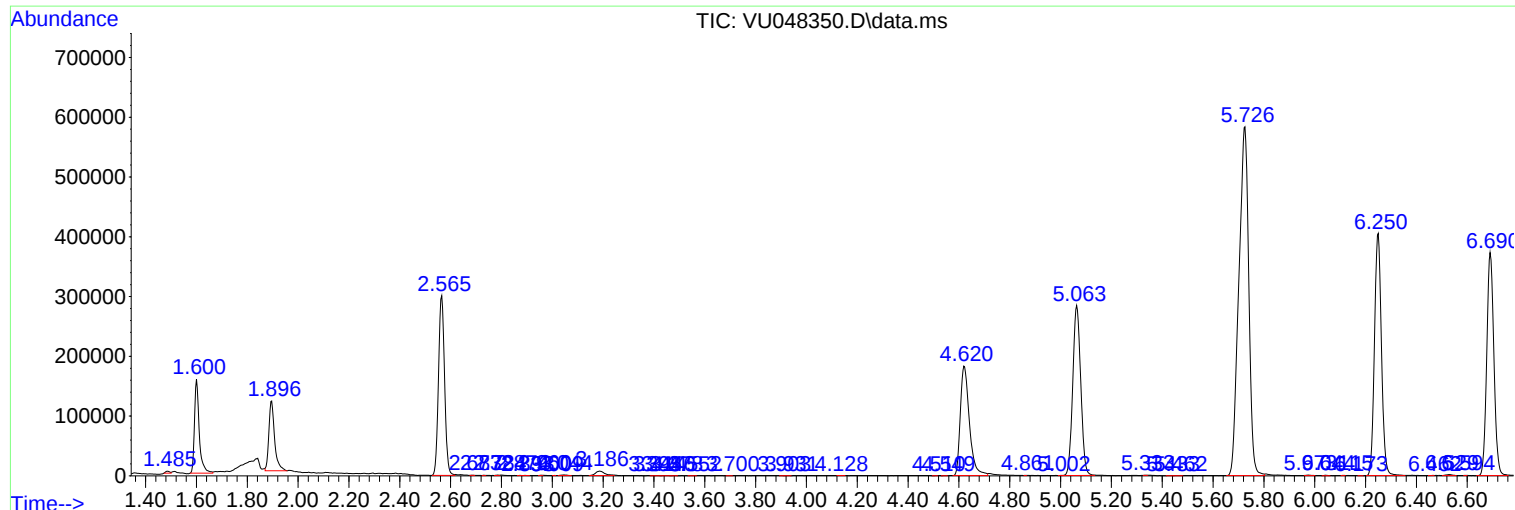

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
Data File : VU048350.D
Acq On : 29 Apr 2022 11:04
Operator : SY/MD
Sample : VU0429WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
Data File : VU048350.D
Acq On : 29 Apr 2022 11:04
Operator : SY/MD
Sample : VU0429WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------