

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048351.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2587-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rBV	153121	194778	12.49%	1.624%
2	1.896	165	173	188	rBV	114143	167219	10.72%	1.394%
3	2.501	358	361	364	rVB3	536	360	0.02%	0.003%
4	2.565	368	381	401	rBV	292258	476737	30.56%	3.976%
5	2.678	412	416	420	rBV2	391	379	0.02%	0.003%
6	2.707	420	425	428	rBV2	362	348	0.02%	0.003%
7	2.736	430	434	437	rBV3	450	360	0.02%	0.003%
8	2.900	481	485	487	rVB	251	188	0.01%	0.002%
9	2.954	499	502	504	rBV	297	188	0.01%	0.002%
10	3.047	521	531	540	rBV5	1827	3056	0.20%	0.025%
11	3.128	553	556	559	rBV2	209	175	0.01%	0.001%
12	3.186	559	574	597	rVB	13196	33280	2.13%	0.278%
13	3.269	597	600	603	rBV2	206	168	0.01%	0.001%
14	3.781	754	759	764	rBV	400	515	0.03%	0.004%
15	3.899	793	796	800	rBV2	193	211	0.01%	0.002%
16	3.957	811	814	819	rBV2	370	420	0.03%	0.004%
17	4.006	823	829	833	rBV2	197	217	0.01%	0.002%
18	4.112	859	862	865	rBV	282	210	0.01%	0.002%
19	4.247	898	904	905	rBV	254	263	0.02%	0.002%
20	4.321	923	927	933	rVB2	154	158	0.01%	0.001%
21	4.388	943	948	951	rBV	249	236	0.02%	0.002%
22	4.620	1006	1020	1061	rBV	191454	469102	30.07%	3.912%
23	4.996	1133	1137	1141	rBV2	182	198	0.01%	0.002%
24	5.063	1141	1158	1187	rVV	279942	610455	39.13%	5.091%
25	5.195	1197	1199	1202	rVB2	270	152	0.01%	0.001%
26	5.292	1222	1229	1235	rBV2	374	631	0.04%	0.005%
27	5.333	1235	1242	1244	rBV3	698	976	0.06%	0.008%
28	5.398	1257	1262	1266	rBV2	242	316	0.02%	0.003%
29	5.501	1291	1294	1297	rVB2	303	180	0.01%	0.002%
30	5.726	1338	1364	1393	rBV2	567636	1559954	100.00%	13.009%
31	5.909	1419	1421	1424	rVB2	309	147	0.01%	0.001%
32	5.973	1434	1441	1444	rVV4	742	867	0.06%	0.007%
33	6.034	1456	1460	1463	rBV2	455	431	0.03%	0.004%
34	6.112	1481	1484	1486	rBV	208	163	0.01%	0.001%
35	6.250	1511	1527	1547	rBV	389803	747180	47.90%	6.231%
36	6.526	1606	1613	1620	rBV5	1872	2846	0.18%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048351.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2587-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.587	1629	1632	1635	rBV2	448	315	0.02%	0.003%
38	6.607	1635	1638	1644	rVB3	369	319	0.02%	0.003%
39	6.690	1648	1664	1685	rBV	366574	713839	45.76%	5.953%
40	6.809	1697	1701	1706	rVV4	795	873	0.06%	0.007%
41	6.832	1706	1708	1714	rVB2	430	274	0.02%	0.002%
42	6.909	1725	1732	1735	rBV2	224	258	0.02%	0.002%
43	7.047	1770	1775	1778	rVV2	253	295	0.02%	0.002%
44	7.063	1778	1780	1788	rVB2	403	247	0.02%	0.002%
45	7.179	1804	1816	1827	rBV6	2504	5576	0.36%	0.046%
46	7.321	1858	1860	1865	rVB2	291	161	0.01%	0.001%
47	7.433	1891	1895	1898	rBV	175	138	0.01%	0.001%
48	7.565	1920	1936	1953	rBV	198597	343638	22.03%	2.866%
49	7.645	1959	1961	1963	rVB2	404	140	0.01%	0.001%
50	7.684	1968	1973	1977	rBV3	1030	1126	0.07%	0.009%
51	7.742	1988	1991	1992	rBV	274	145	0.01%	0.001%
52	7.793	1998	2007	2013	rVB4	955	1529	0.10%	0.013%
53	7.899	2026	2040	2056	rBV	693737	1209084	77.51%	10.083%
54	8.179	2115	2127	2141	rBV	140743	232348	14.89%	1.938%
55	8.555	2241	2244	2247	rBV2	259	180	0.01%	0.002%
56	8.575	2247	2250	2254	rVB5	519	350	0.02%	0.003%
57	8.636	2254	2269	2314	rBV	582521	1077722	69.09%	8.987%
58	8.838	2329	2332	2337	rBV4	212	213	0.01%	0.002%
59	8.902	2349	2352	2355	rBV2	298	243	0.02%	0.002%
60	8.944	2363	2365	2370	rBV3	579	527	0.03%	0.004%
61	9.015	2384	2387	2390	rVB	341	195	0.01%	0.002%
62	9.034	2390	2393	2396	rBV3	307	258	0.02%	0.002%
63	9.150	2424	2429	2430	rBV2	365	309	0.02%	0.003%
64	9.185	2437	2440	2444	rBV2	181	151	0.01%	0.001%
65	9.417	2498	2512	2532	rBV	586303	980304	62.84%	8.175%
66	9.645	2579	2583	2588	rVB3	541	451	0.03%	0.004%
67	9.697	2592	2599	2607	rVV3	822	1098	0.07%	0.009%
68	9.780	2619	2625	2627	rBV2	200	205	0.01%	0.002%
69	9.893	2658	2660	2665	rVB	331	203	0.01%	0.002%
70	10.343	2798	2800	2805	rVB2	215	187	0.01%	0.002%
71	10.382	2805	2812	2820	rBV2	323	626	0.04%	0.005%
72	10.443	2827	2831	2835	rBV2	214	297	0.02%	0.002%
73	10.484	2840	2844	2848	rBV2	266	297	0.02%	0.002%
74	10.619	2883	2886	2892	rVB	309	242	0.02%	0.002%
75	10.671	2897	2902	2914	rVB3	2125	2379	0.15%	0.020%
76	10.758	2915	2929	2946	rBV	636276	1029611	66.00%	8.586%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048351.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2587-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.912	2974	2977	2980	rVB3	206	146	0.01%	0.001%
78	11.118	3037	3041	3048	rVB6	743	840	0.05%	0.007%
79	11.150	3048	3051	3053	rBV	300	147	0.01%	0.001%
80	11.324	3101	3105	3108	rBV	196	176	0.01%	0.001%
81	11.378	3117	3122	3130	rBV2	233	361	0.02%	0.003%
82	11.414	3130	3133	3138	rBV3	577	387	0.02%	0.003%
83	11.459	3139	3147	3160	rVV9	1544	2792	0.18%	0.023%
84	11.578	3182	3184	3190	rVB3	377	193	0.01%	0.002%
85	11.639	3199	3203	3204	rBV	269	137	0.01%	0.001%
86	11.668	3210	3212	3216	rVB2	282	183	0.01%	0.002%
87	11.697	3216	3221	3225	rBV3	565	612	0.04%	0.005%
88	11.745	3231	3236	3237	rBV3	450	363	0.02%	0.003%
89	11.812	3244	3257	3280	rBV	580613	926410	59.39%	7.725%
90	11.973	3304	3307	3313	rVB3	1402	1365	0.09%	0.011%
91	12.079	3337	3340	3341	rBV3	244	137	0.01%	0.001%
92	12.121	3350	3353	3355	rBV2	228	144	0.01%	0.001%
93	12.195	3362	3376	3397	rBV	716397	1169610	74.98%	9.754%
94	12.513	3472	3475	3477	rBV	270	164	0.01%	0.001%
95	12.562	3486	3490	3493	rBV2	487	308	0.02%	0.003%
96	12.745	3544	3547	3550	rVB2	394	216	0.01%	0.002%
97	12.774	3550	3556	3560	rBV	594	861	0.06%	0.007%
98	13.844	3884	3889	3890	rBV	706	612	0.04%	0.005%
99	14.095	3958	3967	3978	rBV5	2108	4070	0.26%	0.034%
100	14.336	4036	4042	4049	rBV3	1404	1972	0.13%	0.016%




Sum of corrected areas: 11991623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
Data File : VU048351.D
Acq On : 29 Apr 2022 11:28
Operator : SY/MD
Sample : N2587-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

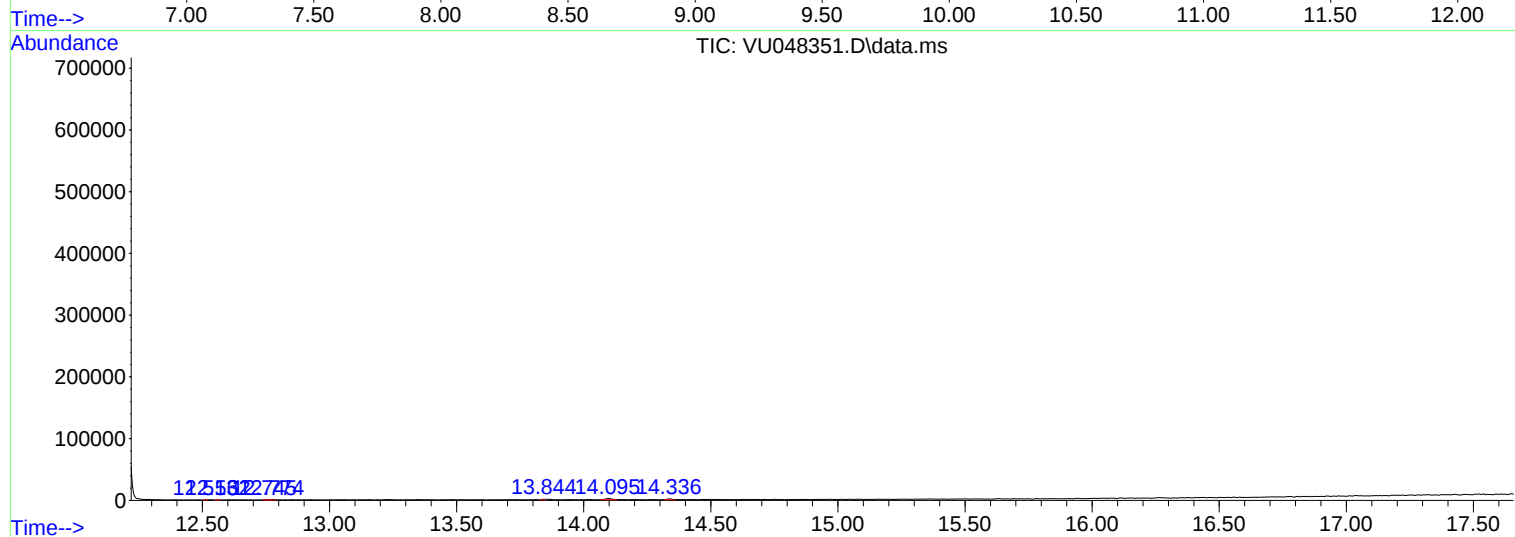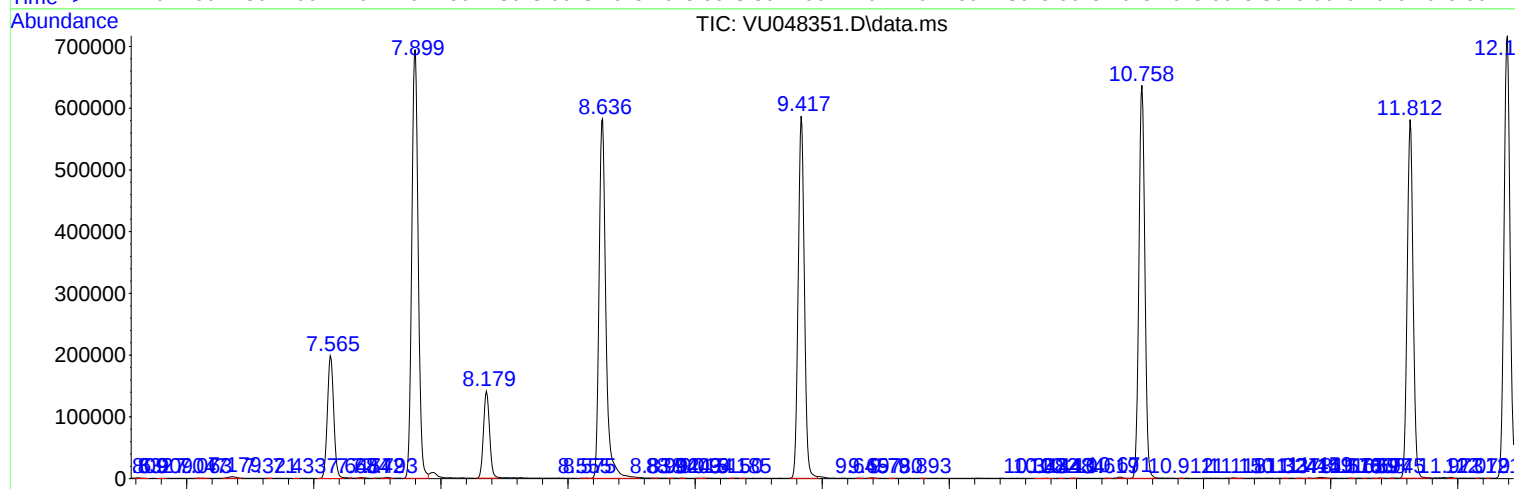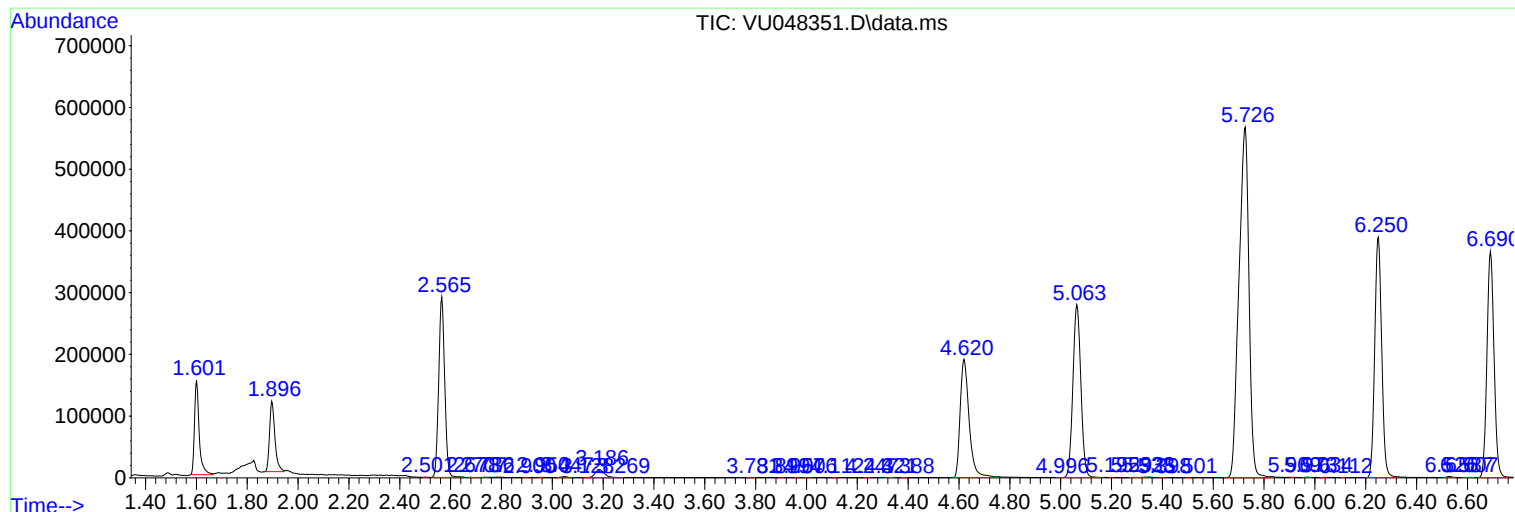

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
Data File : VU048351.D
Acq On : 29 Apr 2022 11:28
Operator : SY/MD
Sample : N2587-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
Data File : VU048351.D
Acq On : 29 Apr 2022 11:28
Operator : SY/MD
Sample : N2587-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------