


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042922\
 Data File : VU048347.D
 Acq On : 29 Apr 2022 08:43
 Operator : SY/MD
 Sample : BFB076
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB076

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Thu May 05 02:16:45 2022

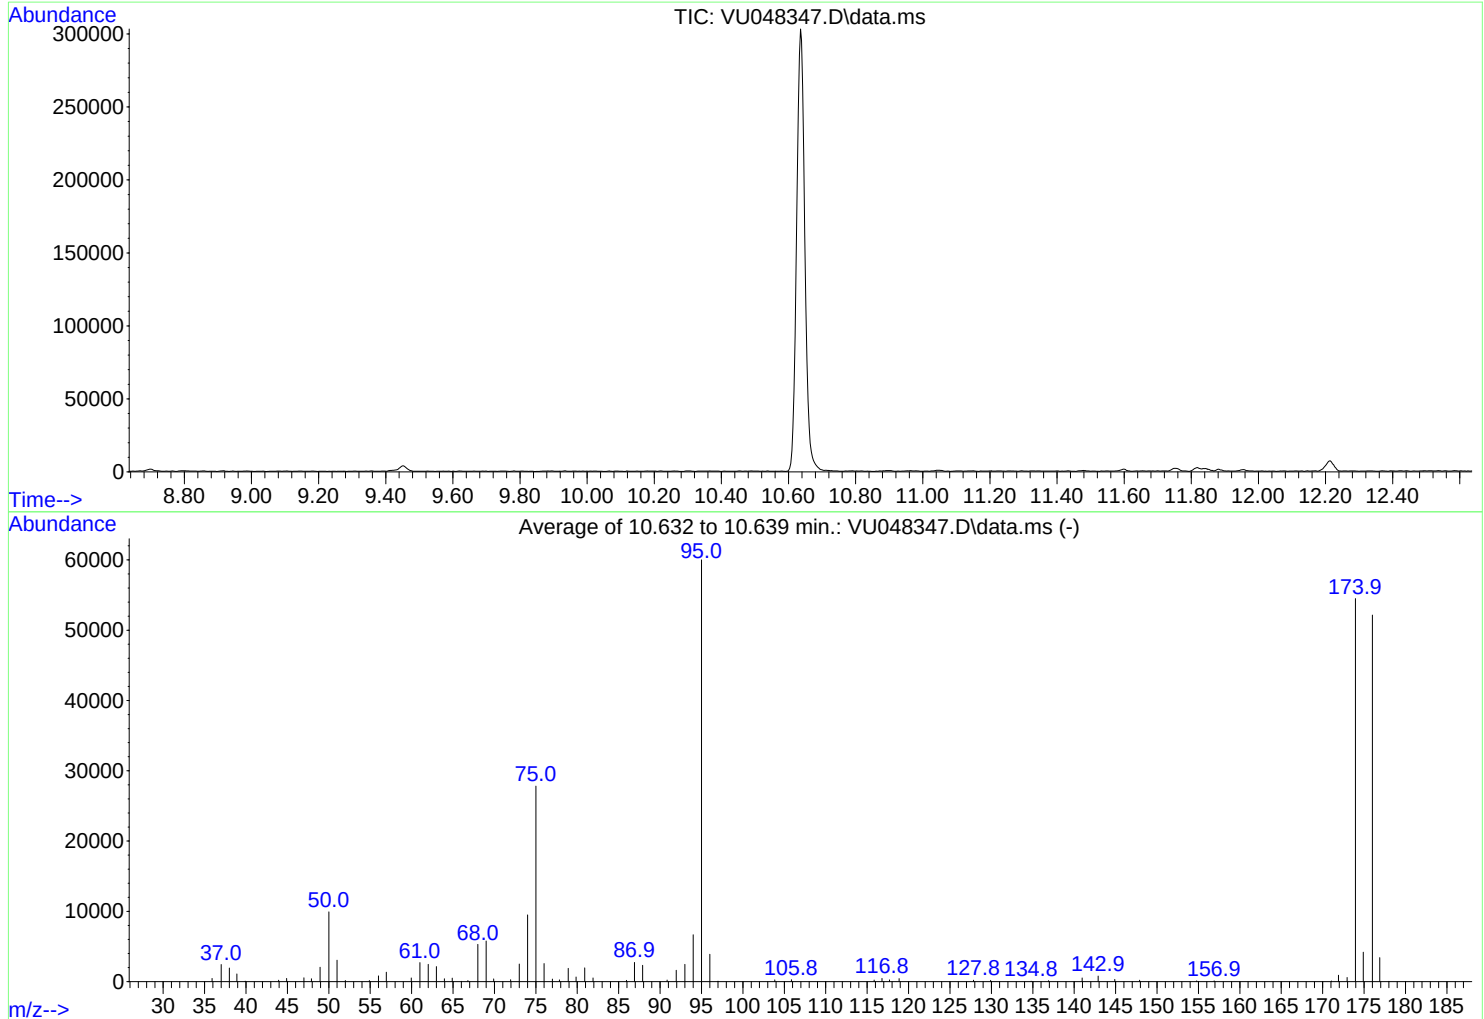

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	9936	PASS
75	95	30	80	46.4	27816	PASS
95	95	100	100	100.0	60011	PASS
96	95	5	9	6.5	3904	PASS
173	174	0.00	2	1.1	586	PASS
174	95	50	120	90.8	54496	PASS
175	174	5	9	7.7	4195	PASS
176	174	95	101	95.7	52157	PASS
177	176	5	9	6.5	3404	PASS

m/z	Abundance
39.90	101.0
44.00	307.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	494.0
37.00	2432.0
38.00	1943.0
38.90	1171.0
40.00	179.0
44.00	470.0
44.90	453.0
47.00	524.0
48.00	430.0
48.90	2016.0
50.00	9834.0
51.00	2942.0
52.00	160.0
54.90	158.0
56.00	773.0
56.90	1302.0
59.90	500.0
61.00	2705.0
62.00	2465.0
63.00	2060.0
63.90	432.0
64.90	484.0
66.80	139.0
68.00	5367.0
69.00	5765.0
69.90	391.0
72.00	264.0
73.00	2540.0
74.00	9174.0
75.00	27176.0
76.00	2671.0
77.00	331.0
77.80	251.0
78.90	1884.0
79.80	644.0
80.90	1902.0
81.90	532.0
85.90	177.0
86.90	2772.0
87.90	2159.0
90.80	229.0
91.90	1549.0
93.00	2390.0
94.00	6605.0
95.00	58360.0
96.00	3829.0
97.00	132.0
103.80	239.0
105.90	269.0
115.80	224.0
116.80	458.0
117.70	274.0
118.80	389.0
127.90	228.0
129.90	185.0
136.90	109.0
140.90	507.0
142.90	793.0
144.90	322.0
147.90	158.0
154.80	182.0
156.90	118.0
171.90	843.0
172.90	561.0
173.90	51864.0
174.90	4134.0
176.00	49584.0
176.90	3148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	467.0
37.00	2533.0
38.00	1996.0
38.90	1142.0
40.00	190.0
43.90	519.0
44.90	463.0
47.00	579.0
47.90	411.0
49.00	2045.0
50.00	10215.0
51.00	3161.0
52.00	165.0
54.90	181.0
56.00	872.0
57.00	1392.0
59.90	518.0
61.00	2768.0
62.00	2496.0
63.00	2204.0
63.90	424.0
64.90	506.0
66.80	163.0
68.00	5459.0
69.00	5956.0
69.90	401.0
71.90	282.0
73.00	2552.0
74.00	9810.0
75.00	28632.0
76.00	2654.0
77.00	380.0
77.90	232.0
78.90	1942.0
79.80	672.0
80.90	2031.0
81.90	525.0
85.90	199.0
86.90	2839.0
87.90	2376.0
90.90	225.0
92.00	1679.0
93.00	2523.0
94.00	6925.0
95.00	61640.0
96.00	4008.0
97.00	109.0
103.90	258.0
105.90	276.0
115.90	235.0
116.80	465.0
117.70	262.0
118.80	454.0
127.90	205.0
129.90	185.0
134.80	119.0
136.90	155.0
141.00	540.0
142.90	815.0
144.90	334.0
147.90	213.0
154.80	135.0
156.90	125.0
171.00	134.0
171.90	950.0
172.90	600.0
173.90	55992.0
174.90	4336.0
176.00	53616.0
176.90	3487.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	425.0
37.00	2370.0
38.00	1855.0
38.90	968.0
39.90	168.0
43.90	561.0
44.90	432.0
47.00	575.0
47.80	389.0
49.00	2065.0
50.00	9760.0
51.00	3079.0
52.00	148.0
54.90	167.0
56.00	829.0
57.00	1354.0
60.00	525.0
61.00	2638.0
62.00	2418.0
63.00	2178.0
64.00	349.0
64.90	498.0
66.00	108.0
66.80	148.0
68.00	5076.0
69.00	5596.0
69.90	397.0
71.90	269.0
73.00	2399.0
74.00	9507.0
75.00	27640.0
76.00	2412.0
77.00	378.0
77.90	237.0
78.90	1859.0
79.90	675.0
80.90	1968.0
81.90	485.0
86.00	169.0
86.90	2608.0
87.90	2420.0
90.90	218.0
92.00	1626.0
93.00	2491.0
94.00	6498.0
95.00	60032.0
96.00	3876.0
103.90	271.0
105.80	265.0
115.90	212.0
116.80	450.0
117.70	214.0
118.90	433.0
127.80	188.0
129.90	189.0
134.80	117.0
136.90	168.0
140.90	536.0
142.90	780.0
144.90	325.0
147.90	224.0
156.90	119.0
171.10	137.0
171.90	958.0
173.00	597.0
174.00	55632.0
174.90	4115.0
176.00	53272.0
176.90	3577.0
178.00	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076