

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042924\
 Data File : VU058817.D
 Acq On : 29 Apr 2024 14:37
 Operator : MD/SY
 Sample : P2305-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Apr 30 06:12:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 30 06:10:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	63318	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	61958	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	28574	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	17959	3.606	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	72.200%	
7) Chloroethane-d5	1.904	69	14045	3.742	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	74.800%	
11) 1,1-Dichloroethene-d2	2.557	65	10732	4.280	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	85.600%	
20) 2-Butanone-d5	4.612	46	37064	42.357	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.720%	
24) Chloroform-d	5.049	84	51722	5.080	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4	5.692	65	27046	5.480	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.600%	
32) Benzene-d6	5.718	84	89779	4.552	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	6.682	67	25291	4.300	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.000%	
41) Toluene-d8	7.891	98	78467	4.445	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	8.177	79	10096	4.714	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.200%	
46) 2-Hexanone-d5	8.627	63	28761	45.321	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.640%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84	16261	4.539	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152	27523	5.527	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.600%	
Target Compounds						Qvalue
16) Methylene chloride	3.033	84	4153	0.837	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042924\
Data File : VU058817.D
Acq On : 29 Apr 2024 14:37
Operator : MD/SY
Sample : P2305-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Apr 30 06:12:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 30 06:10:03 2024
Response via : Initial Calibration

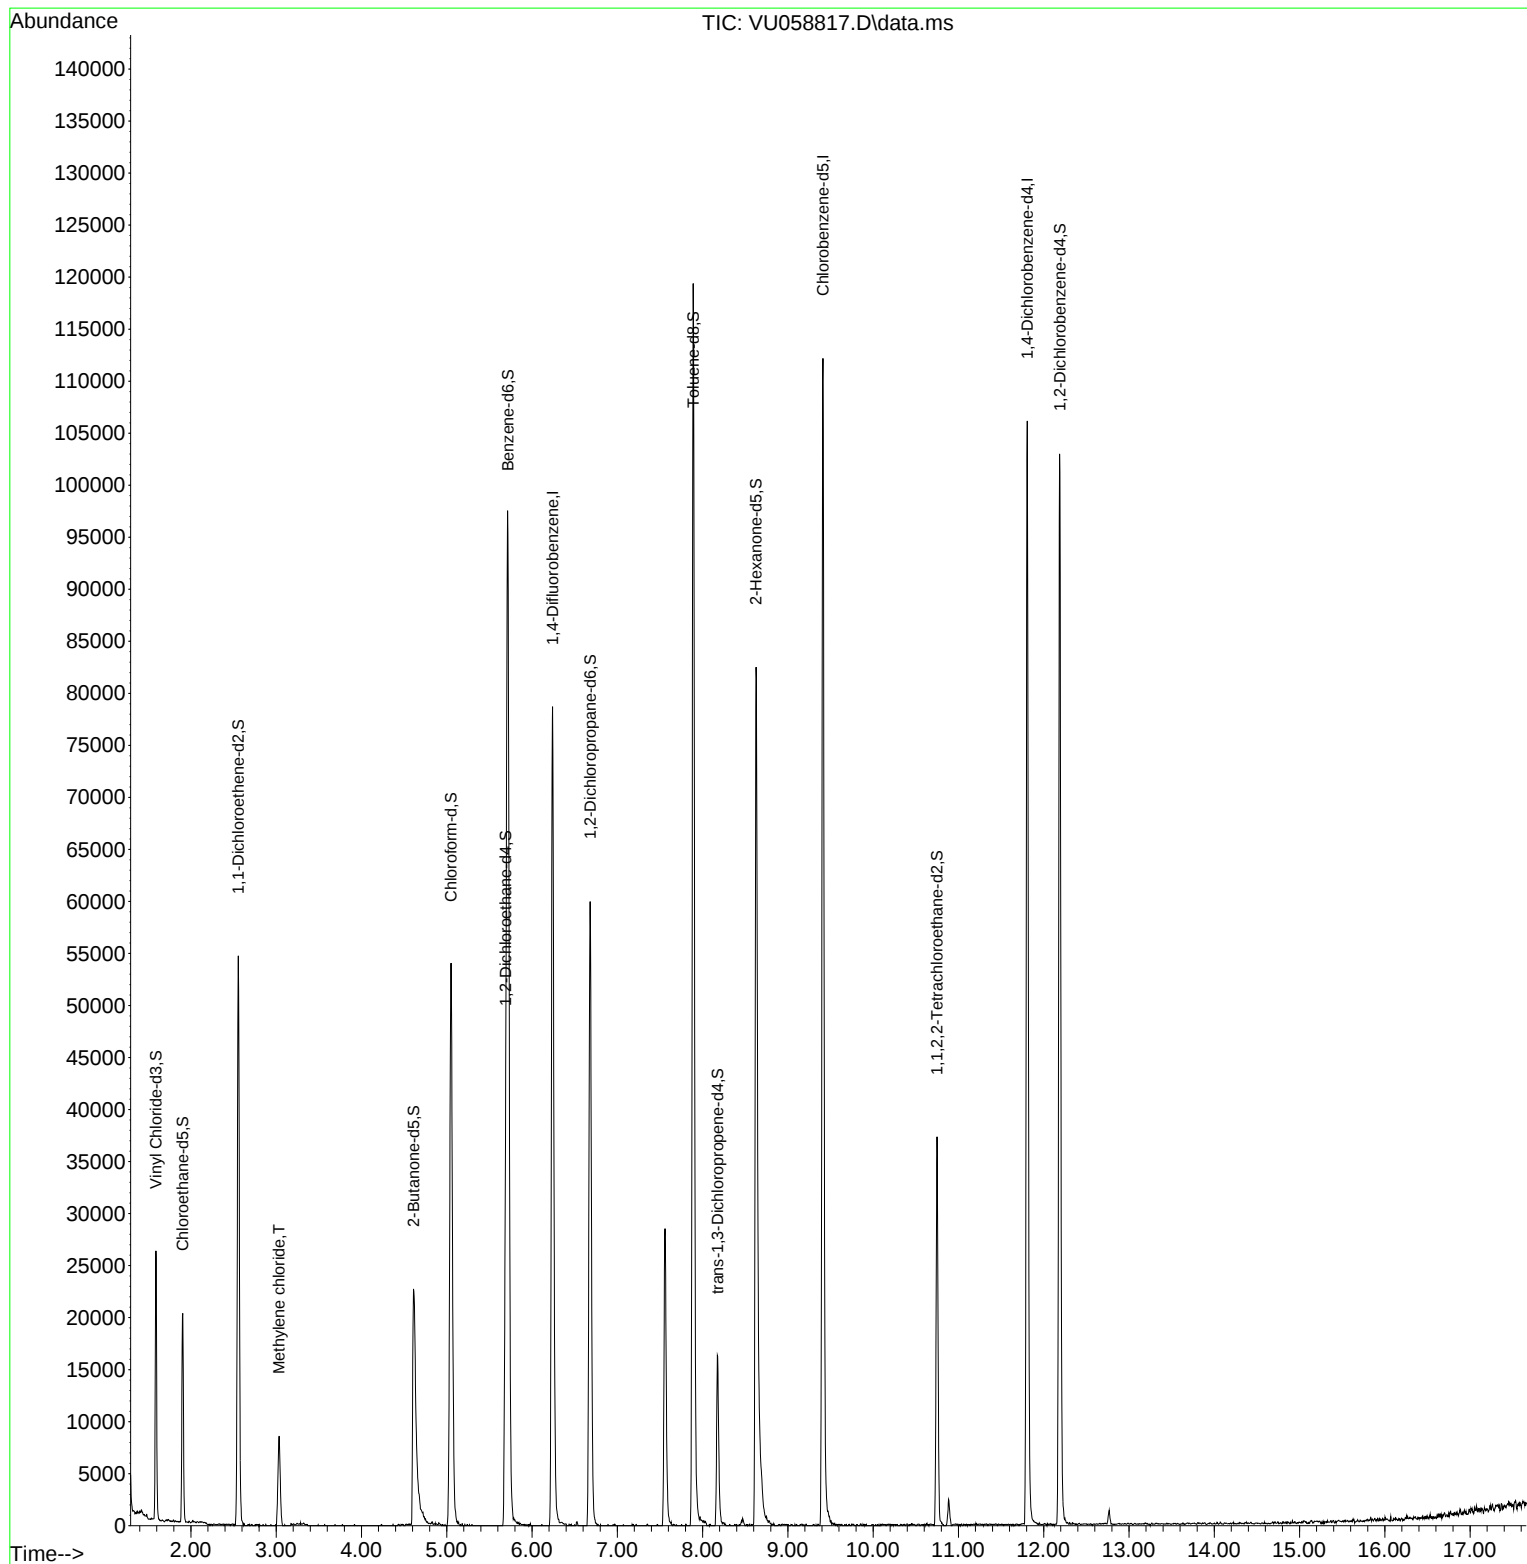

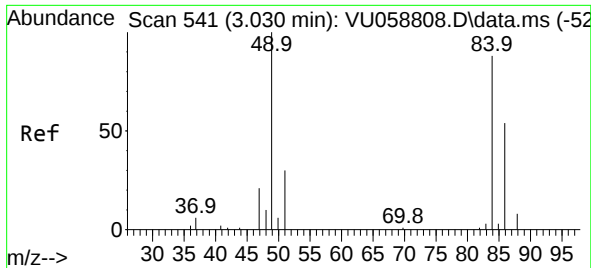

#16
Methylene chloride
Concen: 0.837 ug/L
RT: 3.033 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU058817.D
Acq: 29 Apr 2024 14:37

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

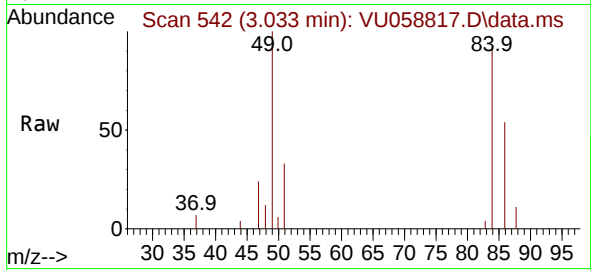

Tgt Ion: 84 Resp: 4153
Ion Ratio Lower Upper
84 100
86 58.3 45.0 83.6
49 108.3 91.6 170.2

