


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042924\
Data File : VU058807.D
Acq On : 29 Apr 2024 09:05
Operator : MD/SY
Sample : BFB150
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB150

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 30 06:10:03 2024

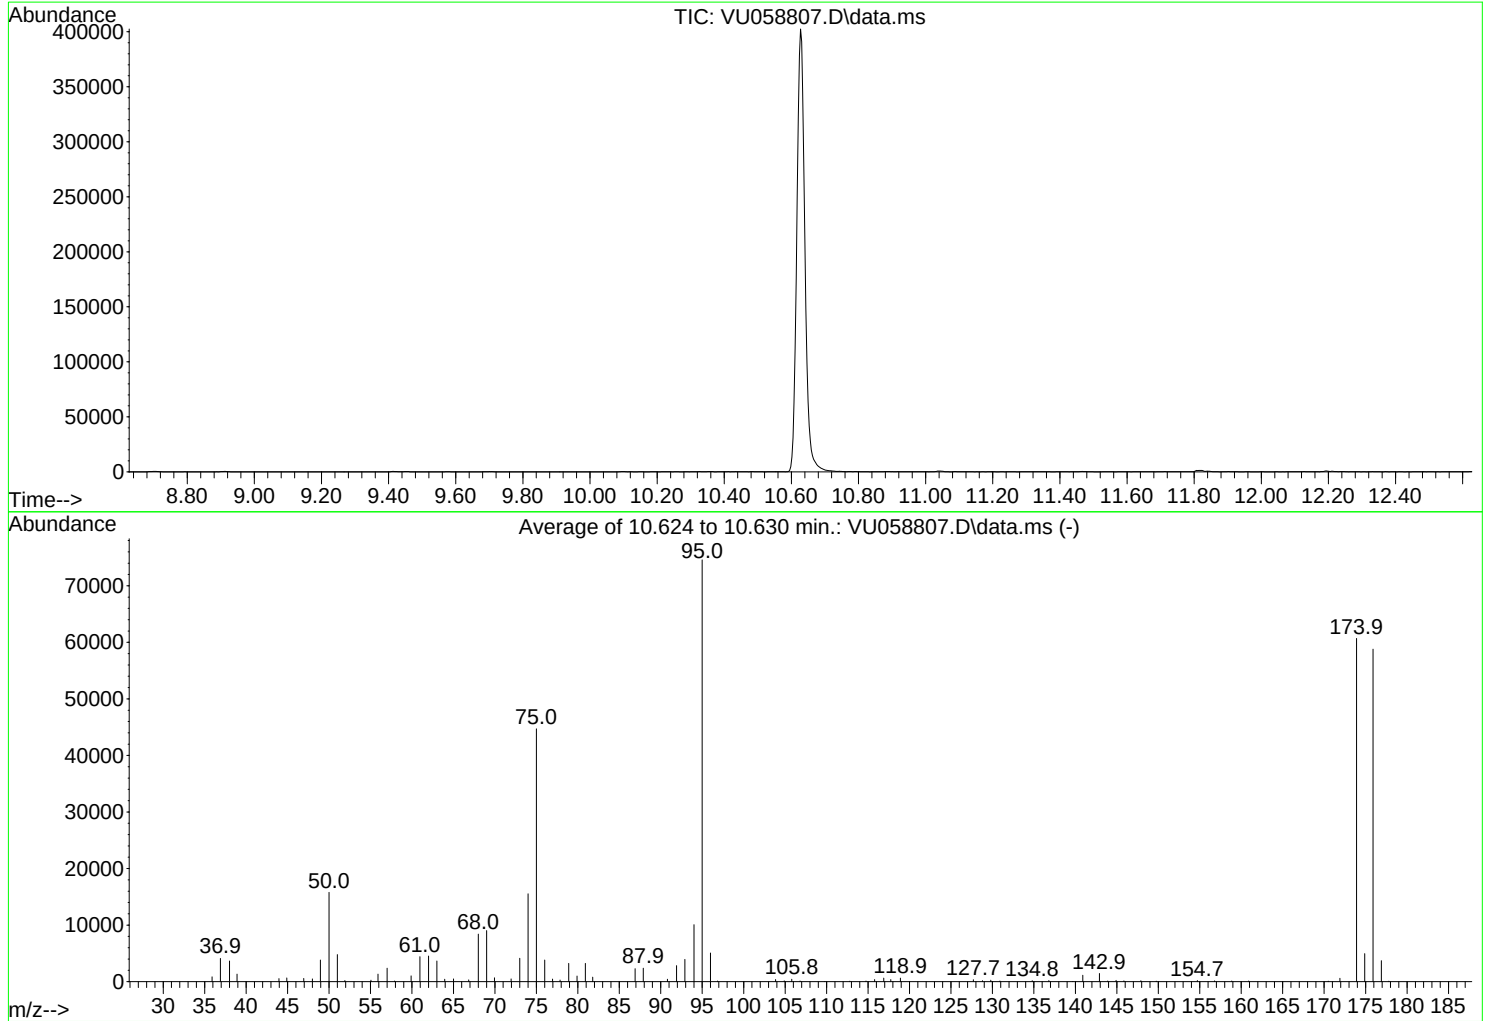

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	15783	PASS
75	95	30	80	59.9	44707	PASS
95	95	100	100	100.0	74587	PASS
96	95	5	9	6.8	5063	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.4	60677	PASS
175	174	5	9	8.2	4961	PASS
176	174	95	101	96.9	58797	PASS
177	176	5	9	6.3	3696	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB150

m/z	Abundance
35.90	866.0
36.90	4114.0
38.00	3513.0
38.90	1289.0
43.90	569.0
44.90	574.0
47.00	532.0
48.00	478.0
49.00	3812.0
50.00	15090.0
51.00	4749.0
51.90	233.0
55.10	265.0
55.90	1389.0
57.00	2277.0
57.90	123.0
59.90	1062.0
60.90	4202.0
62.00	4389.0
63.00	3477.0
63.90	428.0
65.00	519.0
66.80	313.0
68.00	7969.0
69.00	8824.0
69.90	677.0
71.90	446.0
73.00	4145.0
74.00	15243.0
75.00	43464.0
76.00	3734.0
77.00	404.0
77.80	240.0
78.90	3074.0
79.90	921.0
80.90	3162.0
81.80	717.0
86.90	2115.0
87.90	2344.0
90.80	401.0
91.90	2890.0
92.90	3815.0
94.00	9675.0
95.00	73040.0
96.00	5008.0
96.80	110.0
103.80	353.0
104.90	143.0
105.80	422.0
106.80	114.0
109.80	104.0
112.80	128.0
114.80	125.0
115.80	382.0
116.90	679.0
117.80	358.0
118.90	602.0
127.60	305.0
128.80	196.0
129.80	257.0
130.90	133.0
134.80	160.0
136.80	208.0
140.90	1115.0
142.90	1433.0
144.00	120.0
144.90	213.0
145.80	143.0
147.90	158.0
154.70	177.0
156.80	158.0
158.90	117.0
160.90	102.0
171.90	578.0
173.90	58080.0
174.90	4831.0
175.90	56016.0
176.90	3710.0
177.80	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150

m/z	Abundance
35.90	866.0
36.90	4200.0
38.00	3763.0
38.90	1373.0
44.00	554.0
44.90	709.0
47.00	593.0
48.00	512.0
49.00	3970.0
50.00	16361.0
51.00	4997.0
51.90	204.0
55.00	252.0
55.90	1383.0
57.00	2449.0
57.90	136.0
59.90	1055.0
61.00	4567.0
62.00	4640.0
63.00	3743.0
64.00	422.0
65.00	488.0
66.90	306.0
68.00	8671.0
69.00	9244.0
69.90	708.0
71.90	505.0
73.00	4259.0
74.00	15958.0
75.00	46096.0
76.00	3932.0
76.90	477.0
77.90	286.0
78.90	3256.0
79.90	1034.0
80.90	3339.0
81.80	844.0
86.90	2349.0
87.90	2461.0
90.80	432.0
91.90	2926.0
92.90	4120.0
94.00	10452.0
95.00	76656.0
96.00	5238.0
96.90	114.0
103.80	348.0
104.90	141.0
105.80	448.0
106.80	113.0
112.80	109.0
114.70	118.0
115.80	372.0
116.90	622.0
117.80	376.0
118.90	660.0
127.70	359.0
128.80	156.0
129.80	275.0
130.90	128.0
134.80	186.0
136.80	214.0
140.90	1162.0
142.90	1465.0
143.90	122.0
144.90	244.0
145.90	152.0
147.90	167.0
149.70	131.0
154.70	203.0
156.80	136.0
158.90	121.0
160.90	114.0
170.50	123.0
171.90	637.0
173.90	62568.0
174.90	5143.0
175.90	60520.0
176.90	3794.0
177.80	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150

m/z	Abundance
35.90	810.0
36.90	4005.0
38.00	3655.0
38.90	1319.0
44.00	513.0
44.90	704.0
46.90	620.0
48.00	496.0
48.90	3687.0
50.00	15898.0
51.00	4621.0
51.90	178.0
55.00	239.0
55.90	1231.0
57.00	2379.0
57.90	121.0
59.90	917.0
61.00	4470.0
62.00	4543.0
63.00	3737.0
64.00	426.0
65.00	411.0
66.90	317.0
68.00	8569.0
69.00	8996.0
70.00	665.0
72.00	520.0
73.00	4037.0
74.00	15446.0
75.00	44560.0
76.00	3788.0
76.90	515.0
77.90	317.0
78.90	3333.0
79.90	1036.0
80.90	3199.0
81.80	837.0
86.90	2409.0
87.90	2363.0
90.80	425.0
91.90	2722.0
92.90	3848.0
94.00	10128.0
95.00	74064.0
96.00	4942.0
96.90	127.0
103.90	372.0
104.90	121.0
105.80	417.0
106.80	104.0
114.70	105.0
115.80	343.0
116.90	582.0
117.70	380.0
118.90	642.0
127.80	383.0
128.80	161.0
129.80	280.0
130.90	121.0
134.80	205.0
136.80	207.0
139.70	108.0
140.90	1103.0
142.90	1419.0
143.80	114.0
144.90	260.0
145.90	111.0
147.90	156.0
149.80	147.0
154.70	202.0
156.80	111.0
158.80	106.0
160.90	105.0
170.50	131.0
171.90	564.0
173.90	61384.0
174.90	4910.0
175.90	59856.0
176.90	3583.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150