

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU043018\
 Data File : VU023534.D
 Acq On : 30 Apr 2018 18:18
 Operator : MD/SY
 Sample : VU0430WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0430WBL01

Quant Time: May 01 05:27:42 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\524U043018DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue May 01 05:06:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.74	96	50168	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	13392	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	
68) 1,2-Dichlorobenzene-d4	11.87	152	13174	0.83	ug/l	0.00
Spiked Amount 1.000			Recovery	=	83.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU043018\
Data File : VU023534.D
Acq On : 30 Apr 2018 18:18
Operator : MD/SY
Sample : VU0430WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0430WBL01

Quant Time: May 01 05:27:42 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\524U043018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue May 01 05:06:52 2018
Response via : Initial Calibration

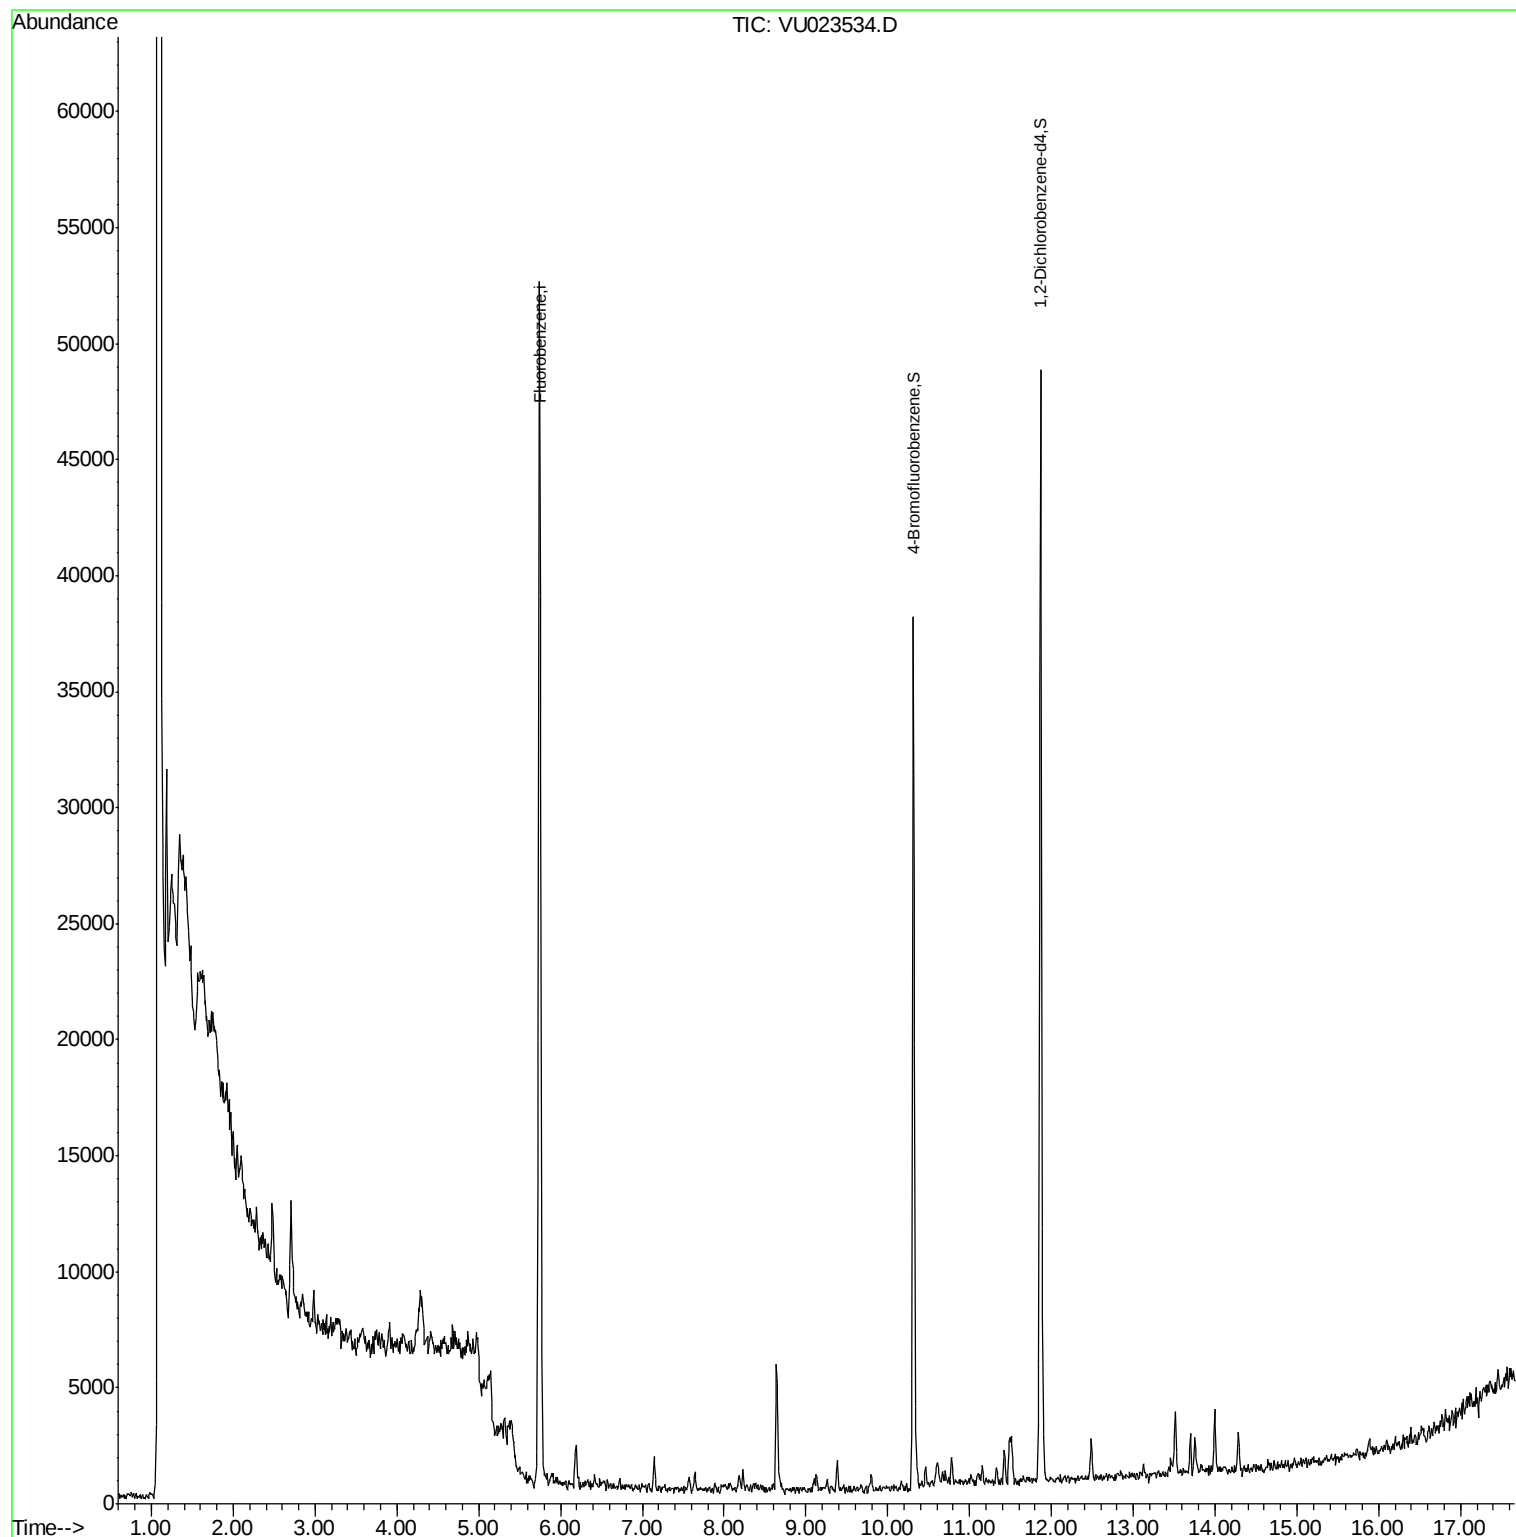

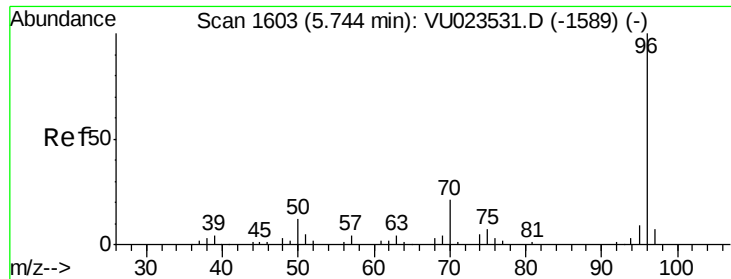

#1

Fluorobenzene

Concen: 1.00 ug/l

RT: 5.74 min Scan# 1603

Delta R.T. -0.00 min

Lab File: VU023534.D

Acq: 30 Apr 2018 18:18

Instrument :

MSVOA_U

ClientSampleId :

VU0430WBL01

Tot Ion: 96 Resp: 50168


Ion Ratio Lower Upper

96 100

70 19.9 16.2 24.4

95 8.8 6.9 10.3

97 6.9 0.0 0.0#



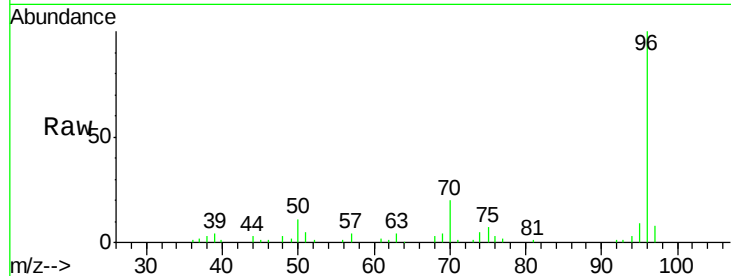


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

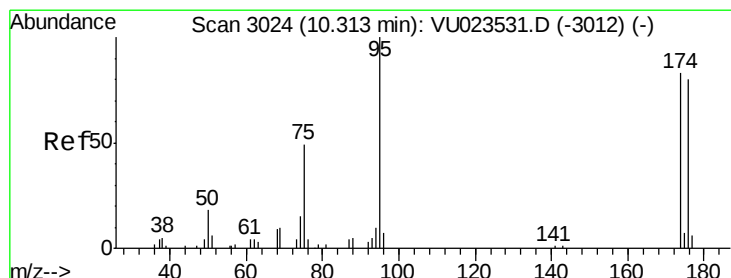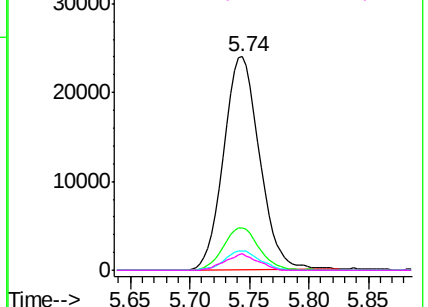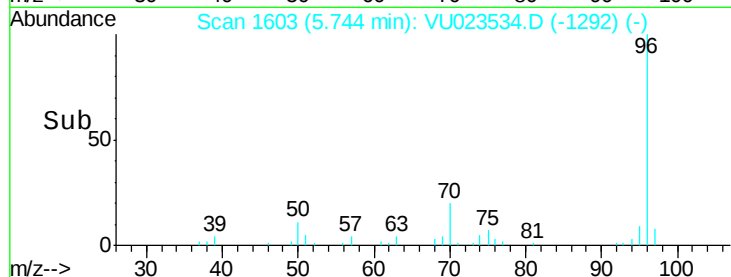

#57

4-Bromofluorobenzene

Concen: Below ug/l

RT: 10.31 min Scan# 3024

Delta R.T. -0.00 min

Lab File: VU023534.D

Acq: 30 Apr 2018 18:18


Tgt Ion: 95 Resp: 13392

Ion Ratio Lower Upper

95 100

174 84.8 65.6 98.4



176 77.0 62.0 93.0



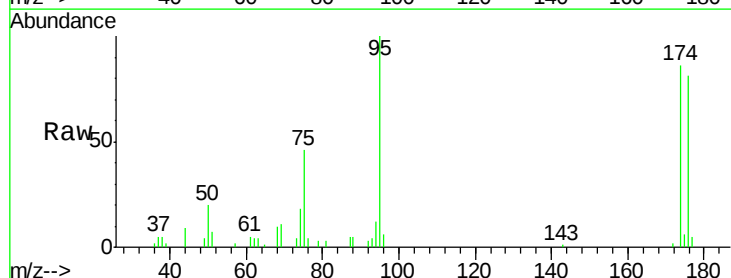


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

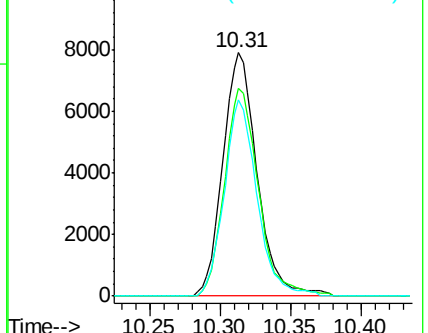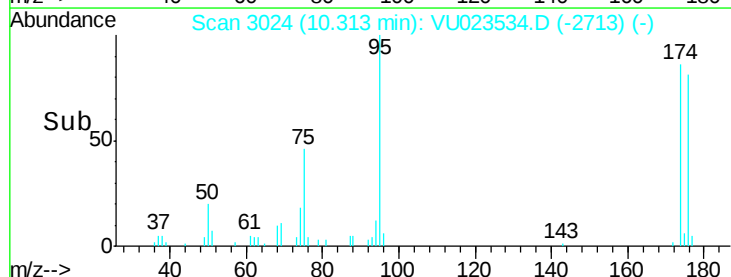

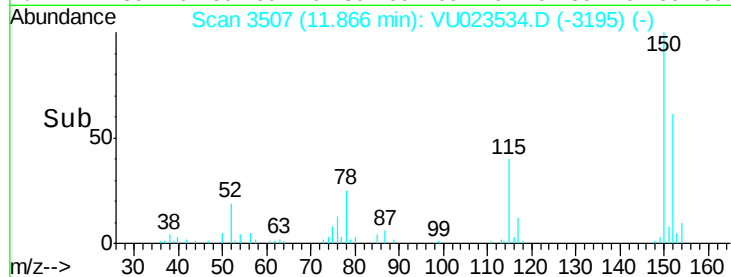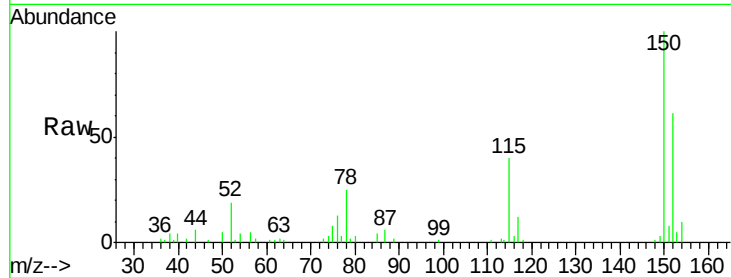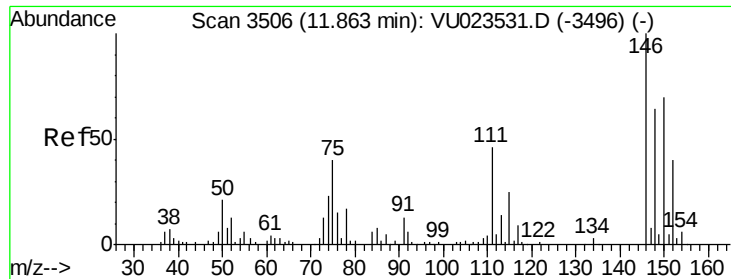

#68

1,2-Dichlorobenzene-d4

Concen: N.D. ug/l

RT: 11.87 min Scan# 3507

Delta R.T. 0.00 min

Lab File: VU023534.D

Acq: 30 Apr 2018 18:18

Instrument :

MSVOA_U

ClientSampleId :

VU0430WBL01

Tot Ion:152 Resp: 13174

Ion Ratio Lower Upper

152 100

115 65.6 0.0 118.8

150 158.8 0.0 0.0#

