


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU043018\
Data File : VU023526.D
Acq On : 30 Apr 2018 14:07
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_U\METHOD\524U043018DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu May 03 10:23:54 2018

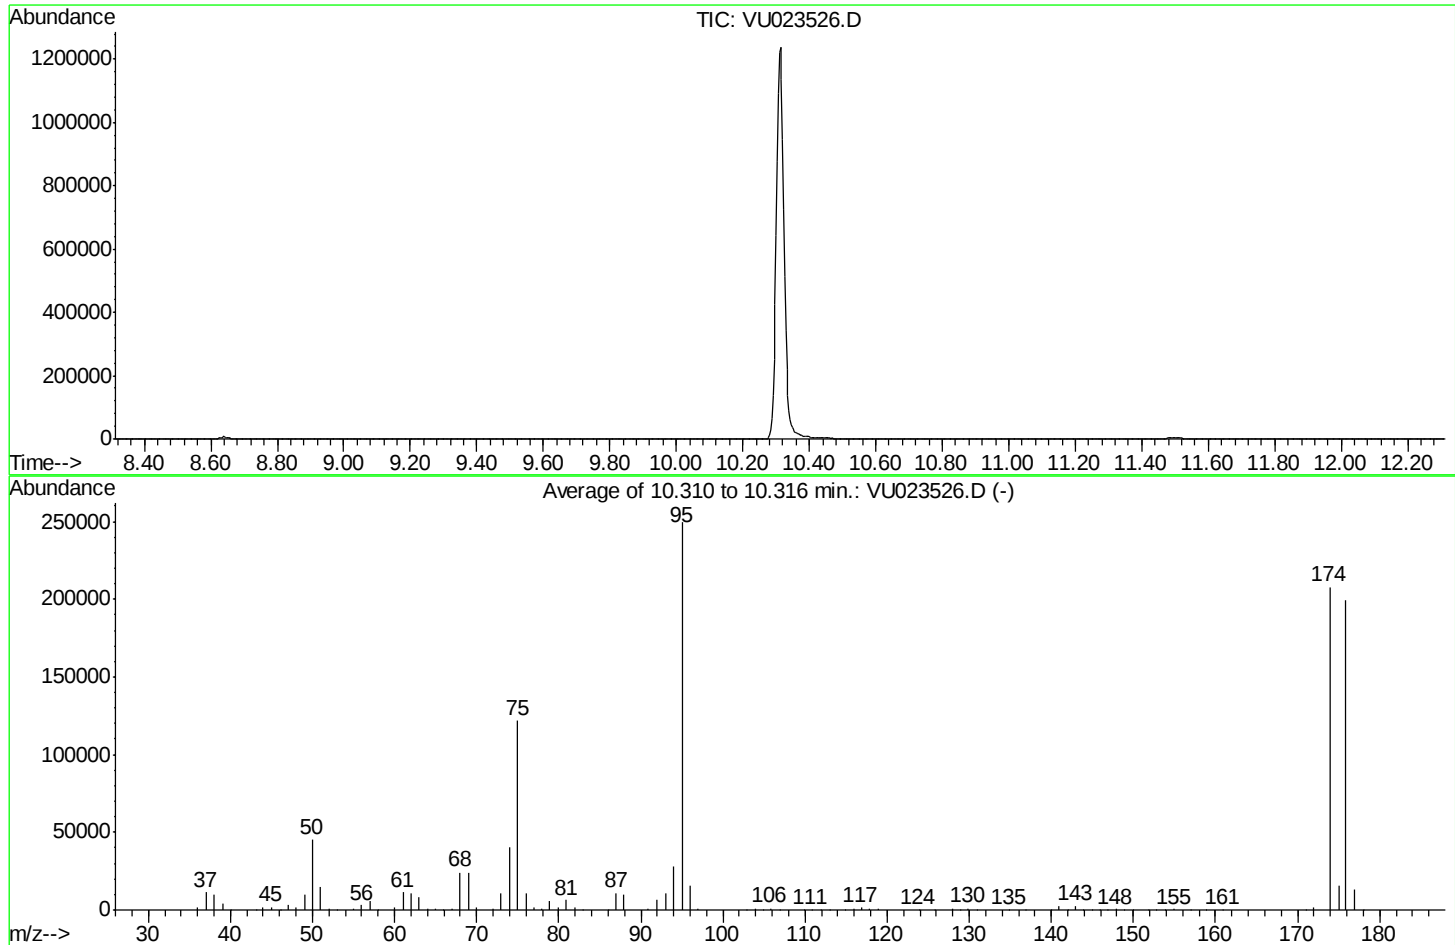

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3009

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	45112	PASS
75	95	30	60	48.7	121538	PASS
95	95	100	100	100.0	249472	PASS
96	95	5	9	6.4	16064	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.4	207978	PASS
175	174	5	9	7.5	15571	PASS
176	174	95	101	96.0	199722	PASS
177	176	5	9	6.4	12830	PASS