
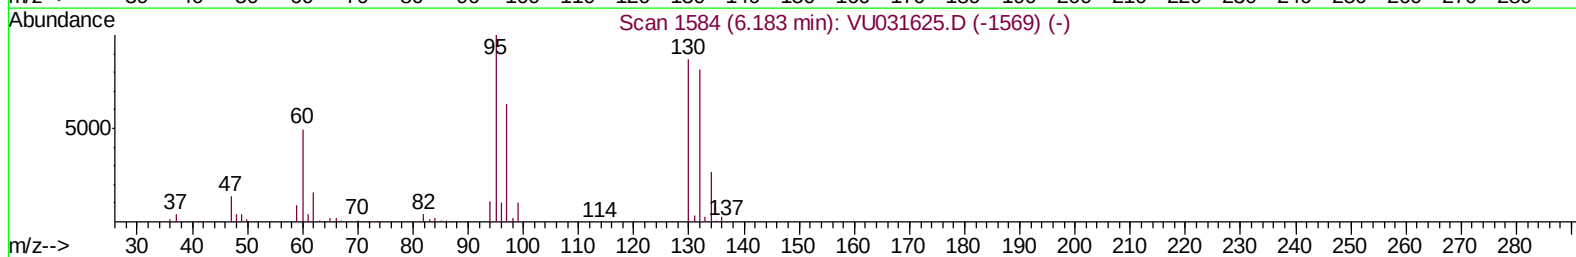
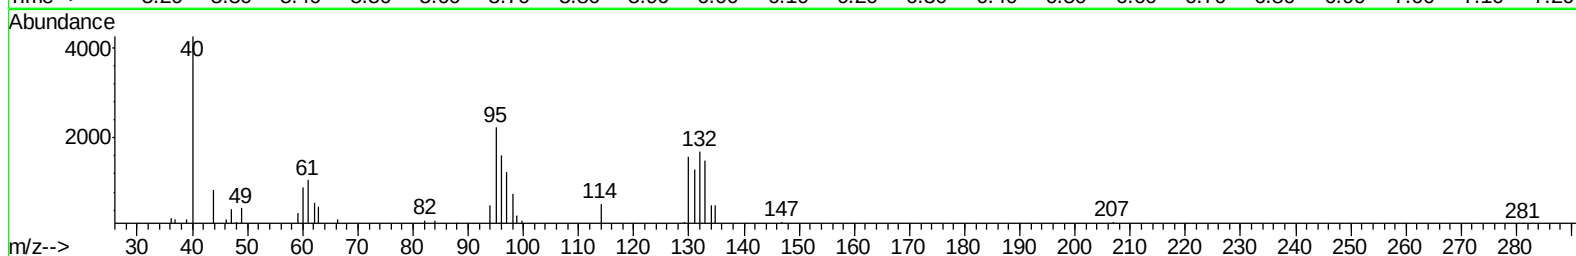


Data File : VU031626.D
Acq On : 30 Apr 2019 12:09
Operator : JC/SP
Sample : VU0430WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 01 01:41:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

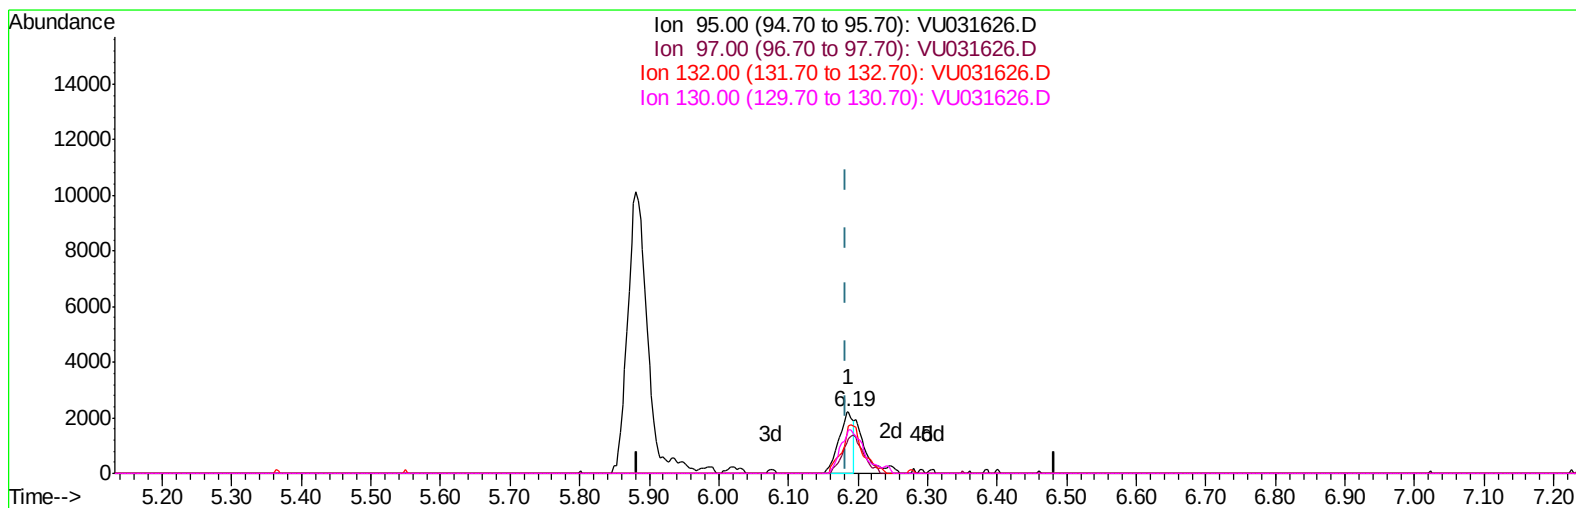

TIC: VU031626.D

(34) Trichloroethene (T)

6.186min (+0.003) 0.57ug/L

response 3115

Ion	Exp%	Act%
95.00	100	100
97.00	64.00	55.61
132.00	90.10	75.67
130.00	95.00	70.78