
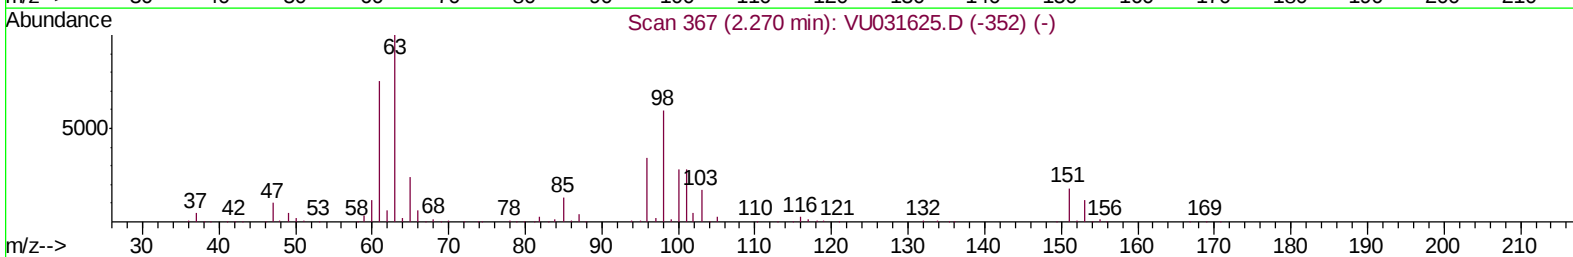
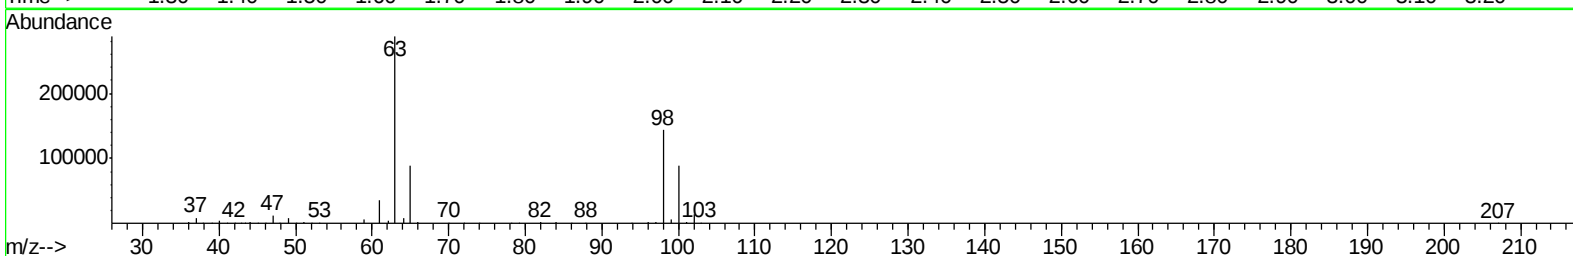


Data File : VU031632.D
Acq On : 30 Apr 2019 14:32
Operator : JC/SP
Sample : K2592-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 01 01:42:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

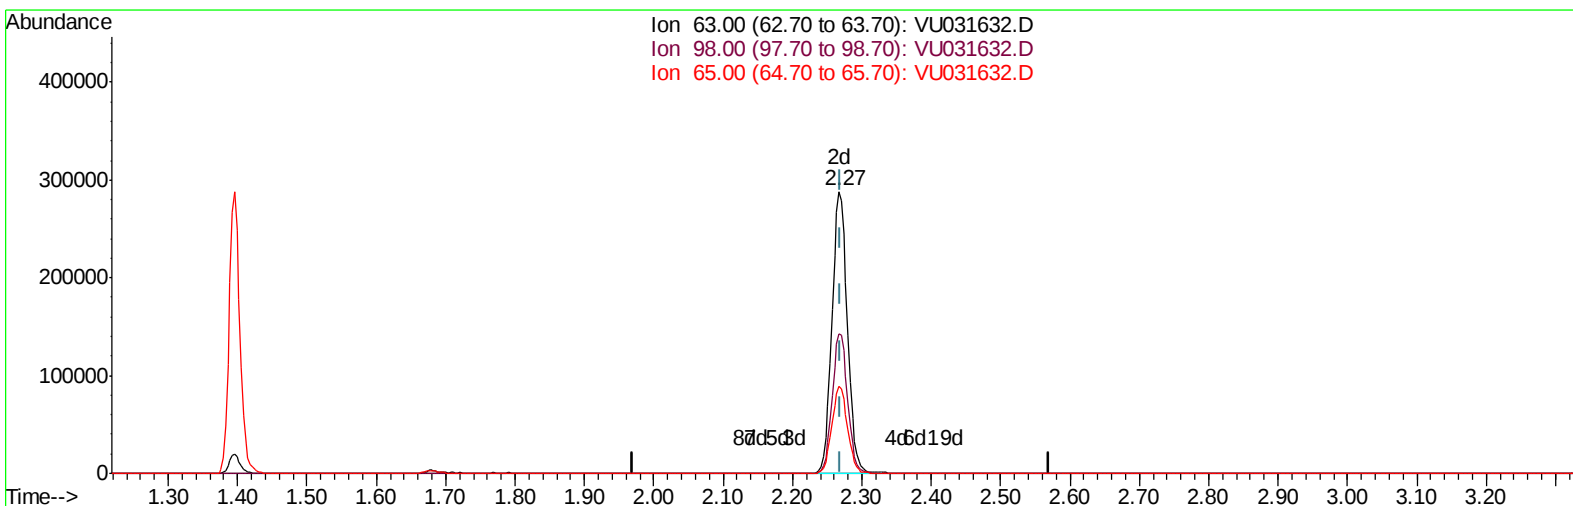

TIC: VU031632.D

(11) 1,1-Dichloroethene-d2 (S)

2.267min (-0.003) 43.05ug/L m

response 441640

Ion	Exp%	Act%
63.00	100	100
98.00	66.60	0.03#
65.00	23.40	0.01#
0.00	0.00	0.00