
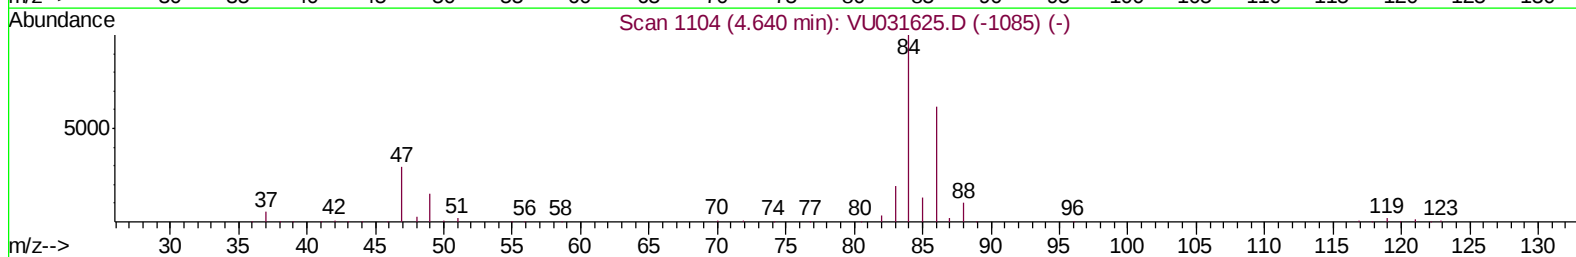
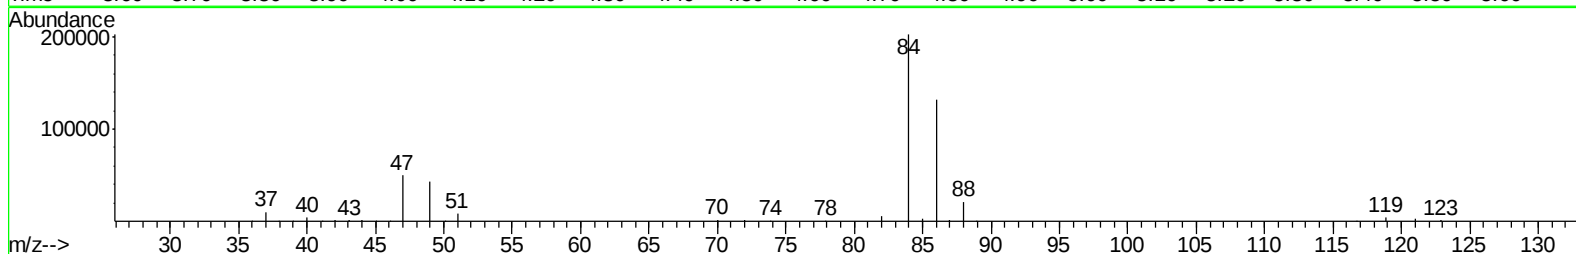


Data File : VU031632.D
Acq On : 30 Apr 2019 14:32
Operator : JC/SP
Sample : K2592-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 01 01:42:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

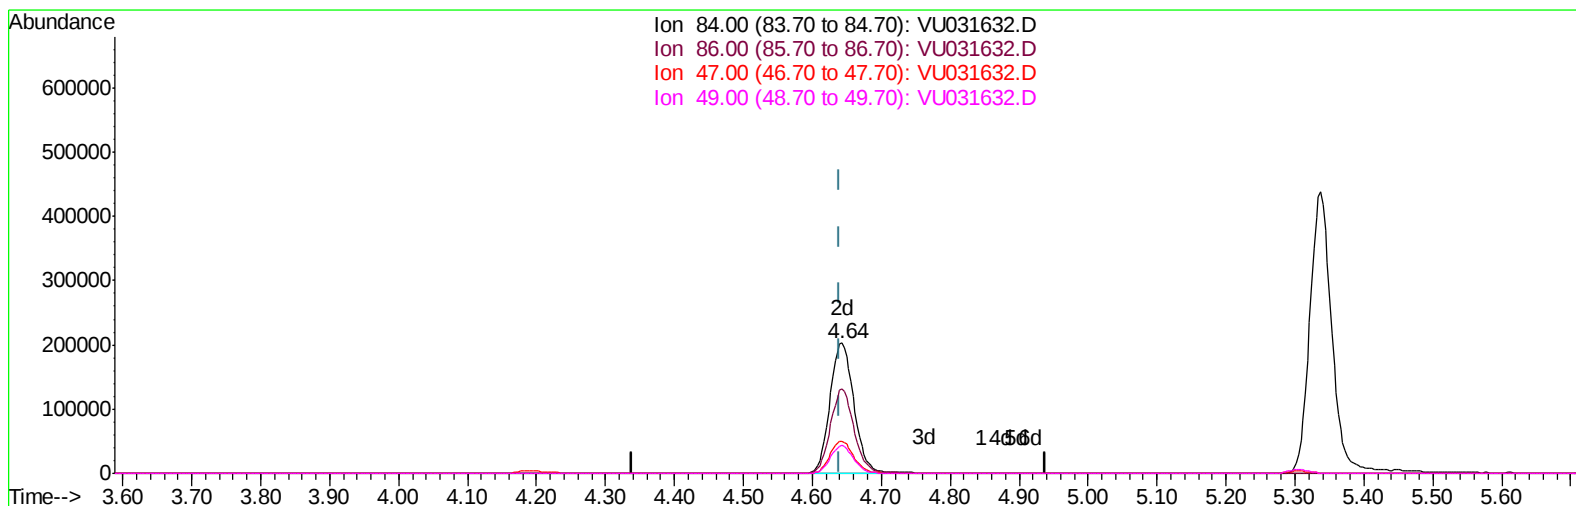

TIC: VU031632.D

(24) Chloroform-d (S)

4.643min (+0.003) 51.53ug/L m

response 486116

Ion	Exp%	Act%
84.00	100	100
86.00	62.50	0.02#
47.00	45.70	0.02#
49.00	27.20	0.01#