
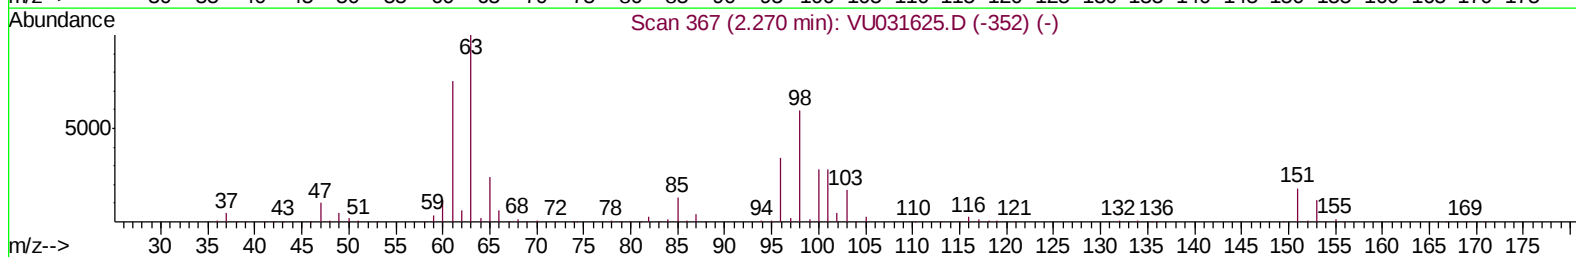
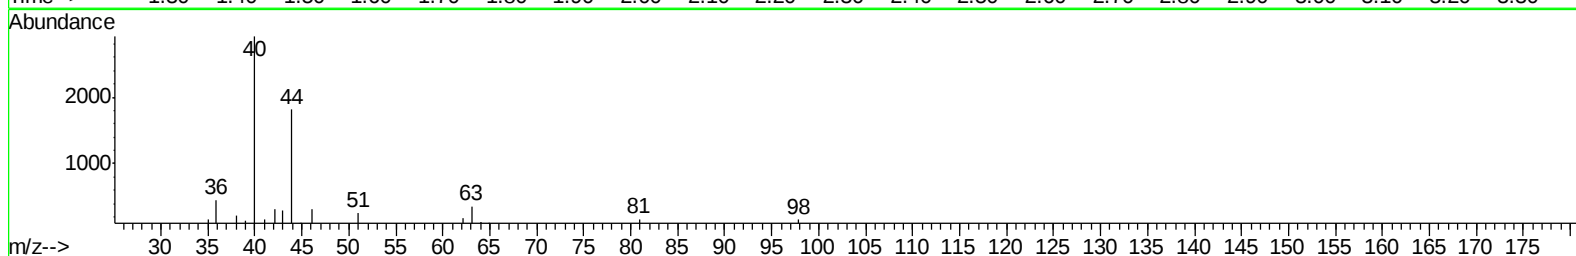


Data File : VU031637.D
Acq On : 30 Apr 2019 16:29
Operator : JC/SP
Sample : K2593-05DL 2500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 01 01:43:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

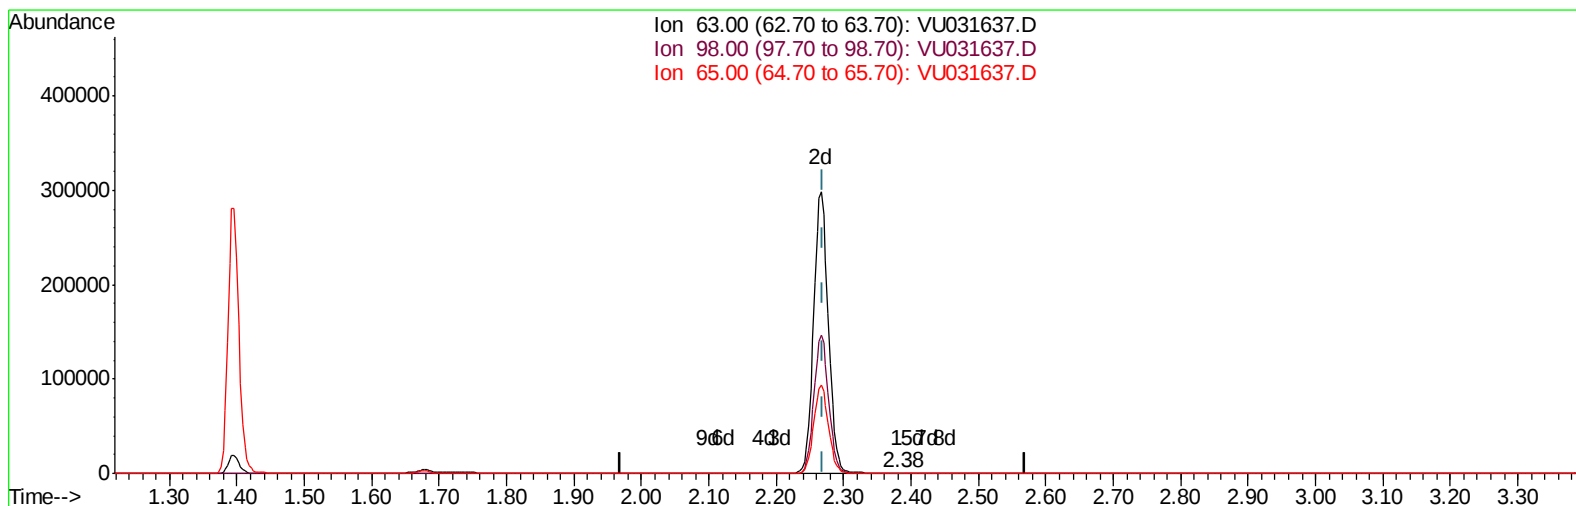

TIC: VU031637.D

(11) 1,1-Dichloroethene-d2 (S)

2.379min (+0.109) 0.02ug/L

response 265

Ion	Exp%	Act%
63.00	100	100
98.00	66.60	61.51
65.00	23.40	19.25
0.00	0.00	0.00