
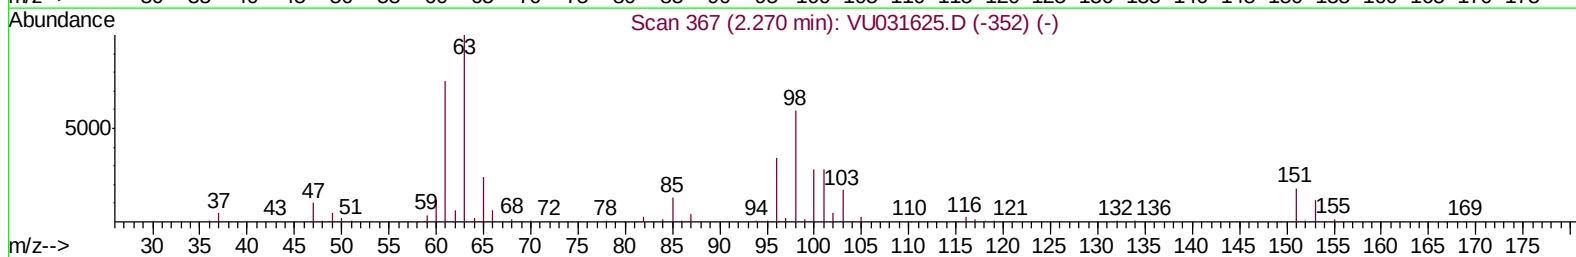
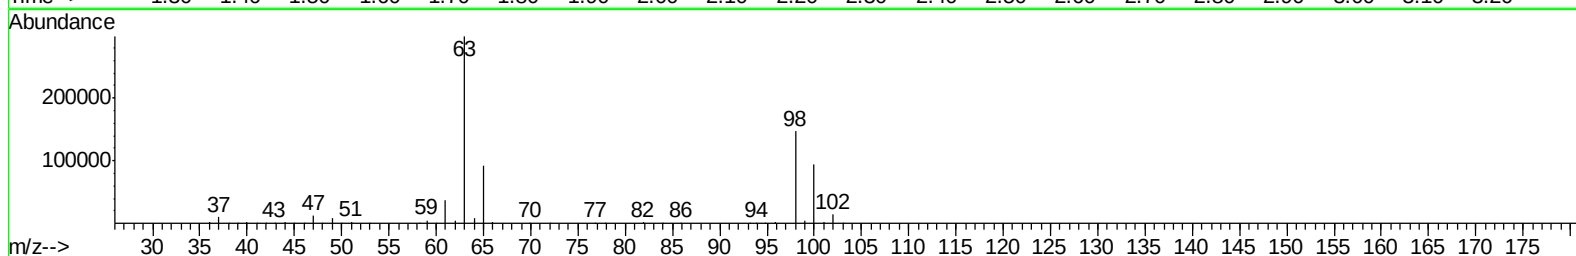


Data File : VU031637.D  
Acq On : 30 Apr 2019 16:29  
Operator : JC/SP  
Sample : K2593-05DL 2500X  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 01 01:43:20 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM042719WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed May 01 01:38:49 2019  
Response via : Initial Calibration

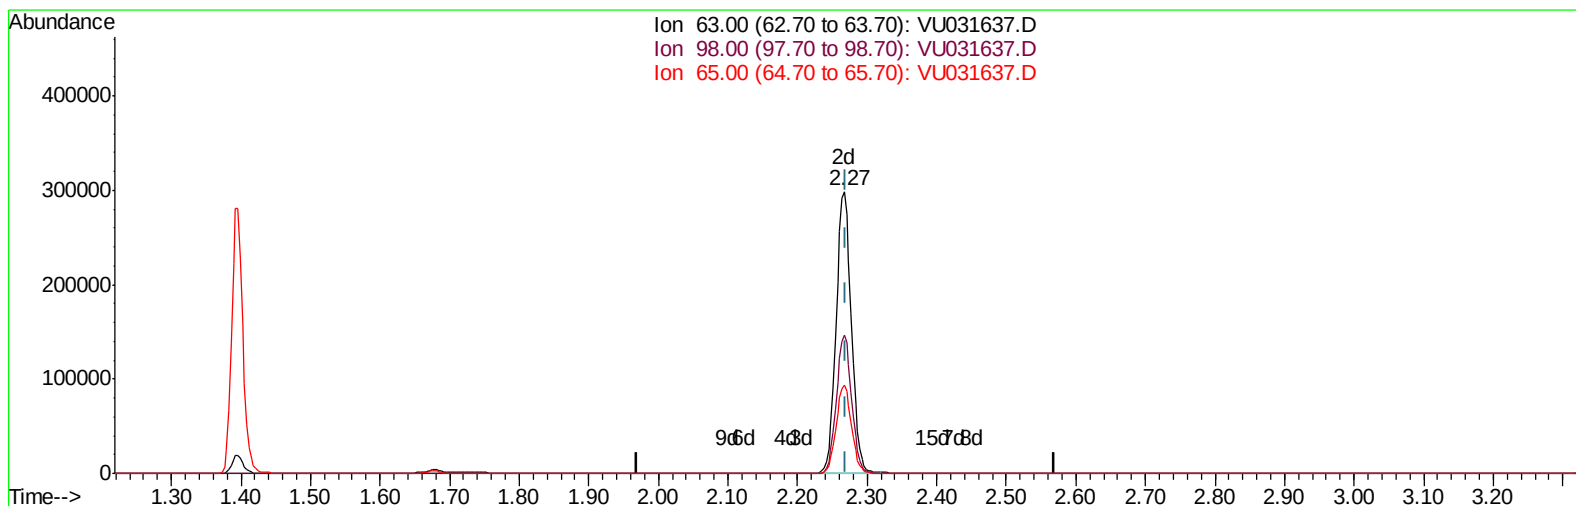

TIC: VU031637.D

(11) 1,1-Dichloroethene-d2 (S)

2.267min (-0.003) 39.99ug/L m

response 452054

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 63.00 | 100   | 100   |
| 98.00 | 66.60 | 0.04# |
| 65.00 | 23.40 | 0.01# |
| 0.00  | 0.00  | 0.00  |