
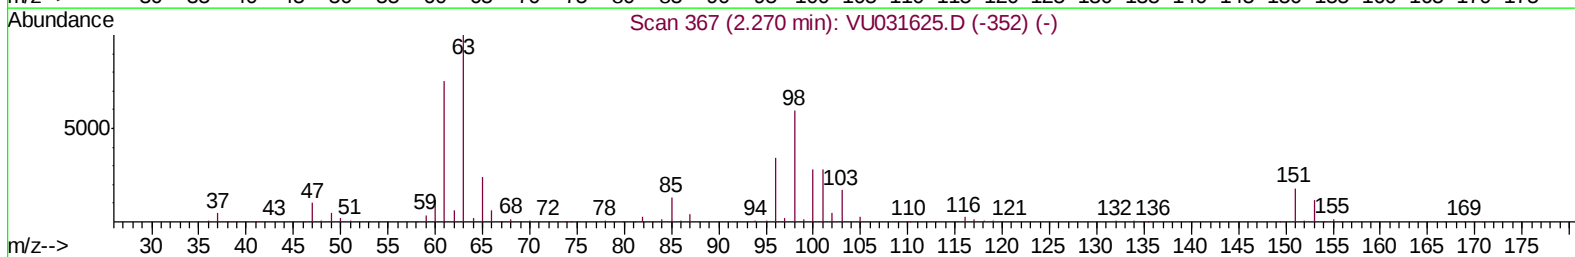
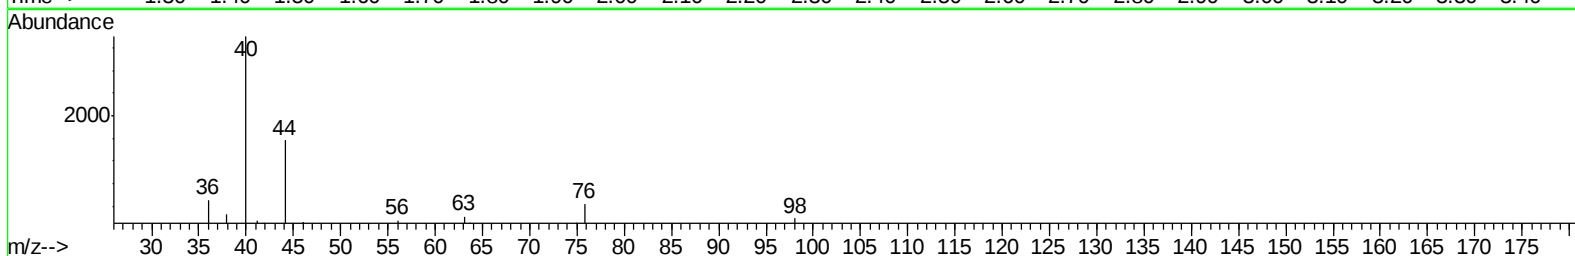


Data File : VU031640.D
Acq On : 30 Apr 2019 17:39
Operator : JC/SP
Sample : K2593-09DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 01 01:43:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

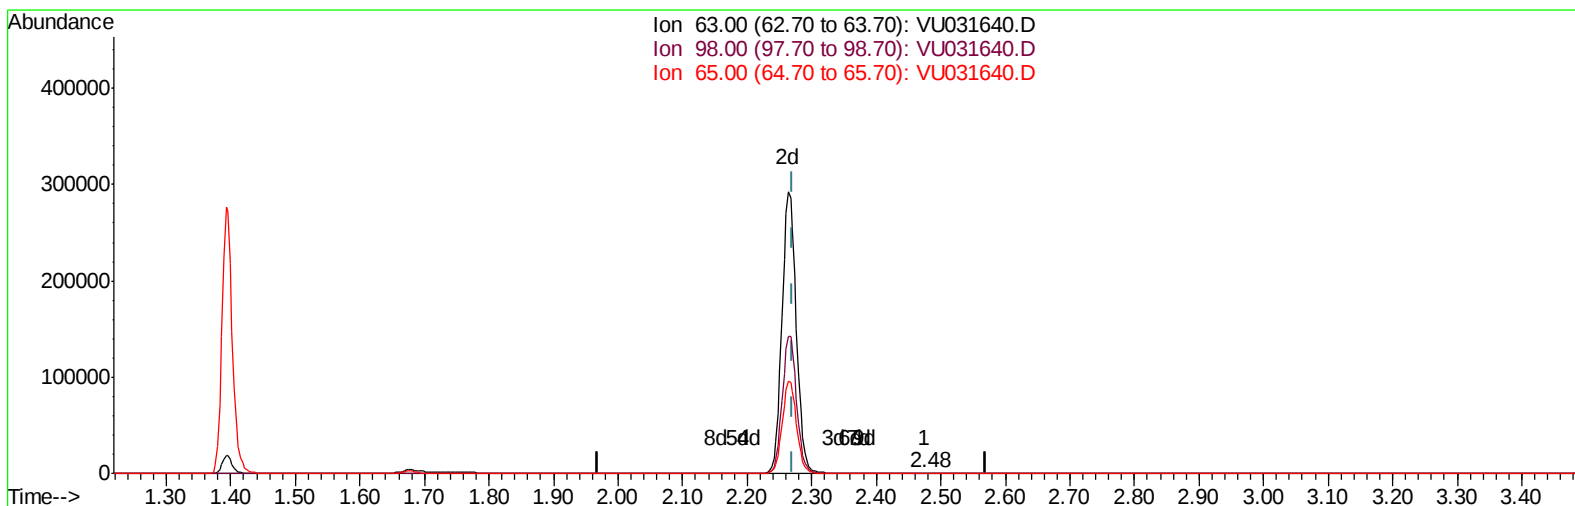

TIC: VU031640.D

(11) 1,1-Dichloroethene-d2 (S)

2.476min (+0.206) 0.01ug/L

response 157

Ion	Exp%	Act%
63.00	100	100
98.00	66.60	61.15
65.00	23.40	26.11
0.00	0.00	0.00