
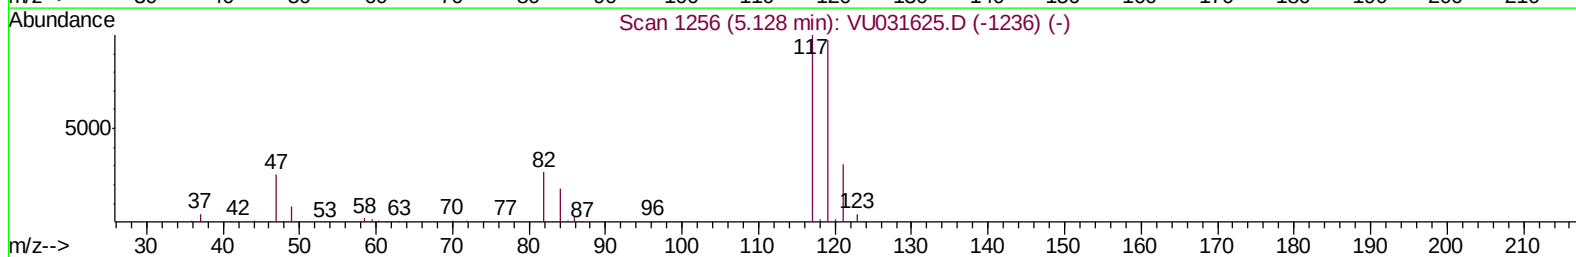
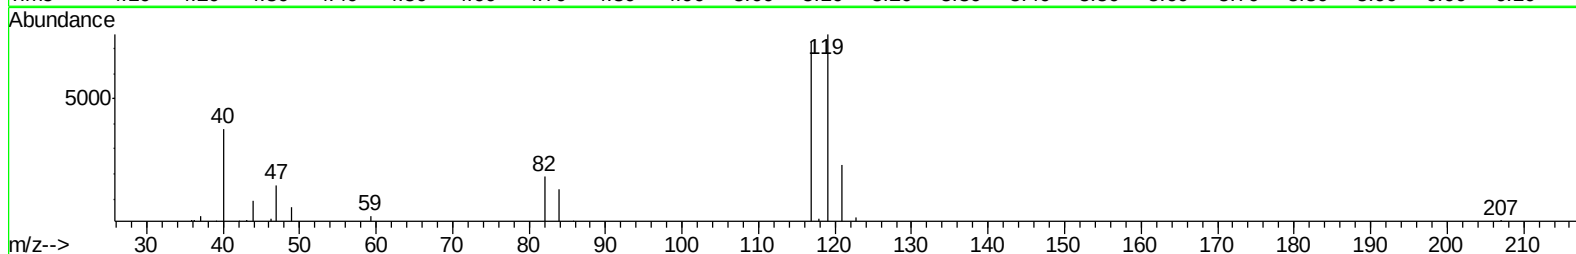


Data File : VU031643.D
Acq On : 30 Apr 2019 18:49
Operator : JC/SP
Sample : K2590-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 01 01:44:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

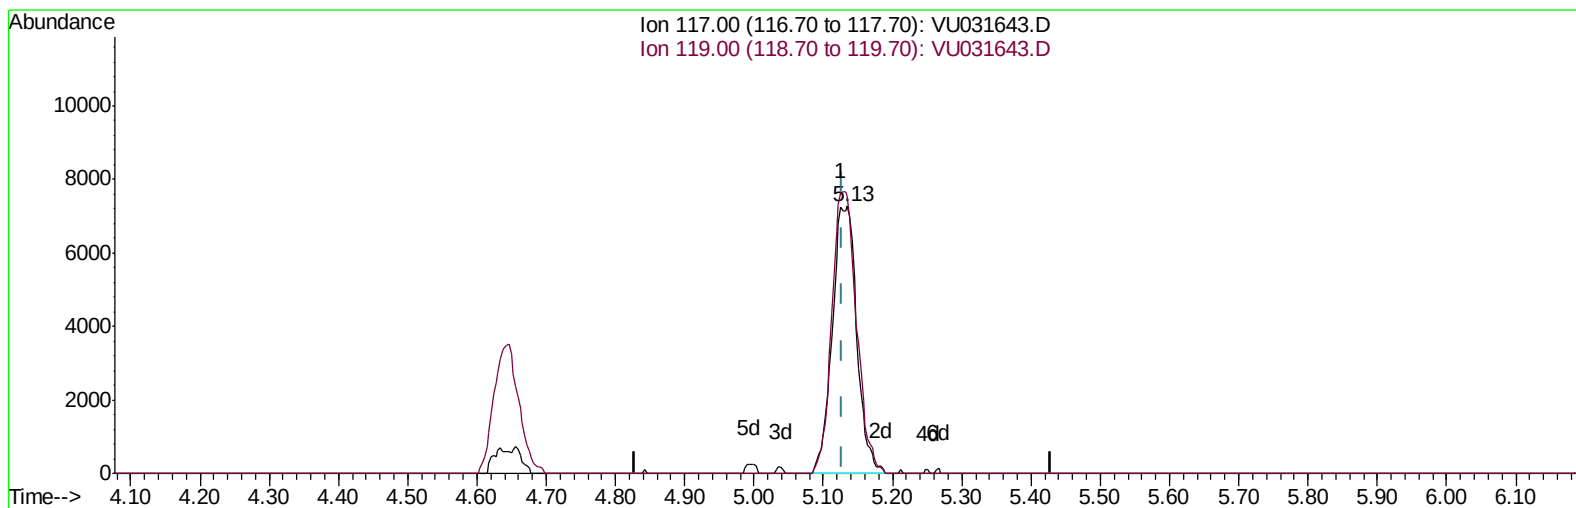

TIC: VU031643.D

(31) Carbon tetrachloride (T)

5.135min (+0.006) 2.44ug/L m

response 17785

Ion	Exp%	Act%
117.00	100	100
119.00	95.70	106.58
0.00	0.00	0.00
0.00	0.00	0.00