
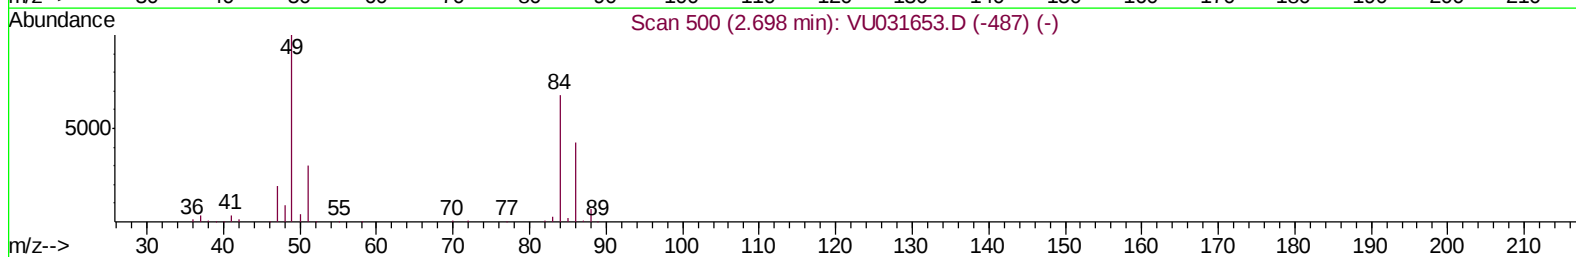
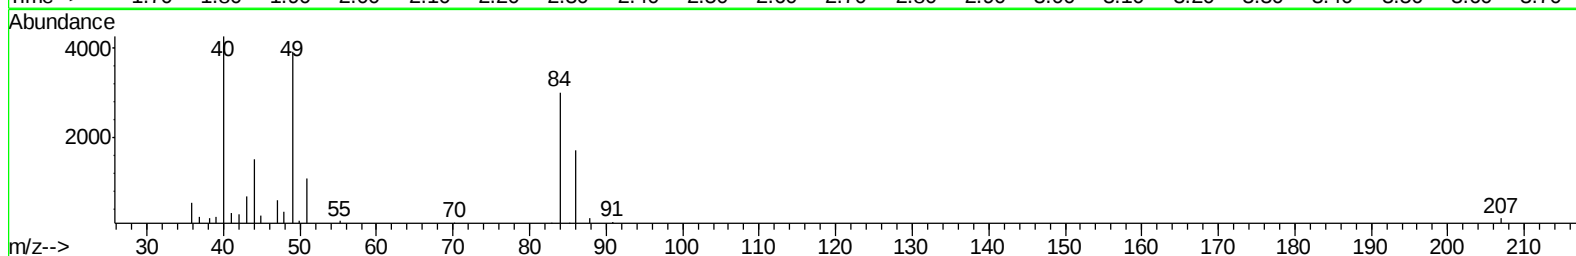


Data File : VU031656.D
Acq On : 01 May 2019 00:39
Operator : JC/SP
Sample : K2604-05
Misc : 5.08g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 35 Sample Multiplier: 1

Quant Time: May 01 04:45:48 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 04:42:38 2019
Response via : Initial Calibration

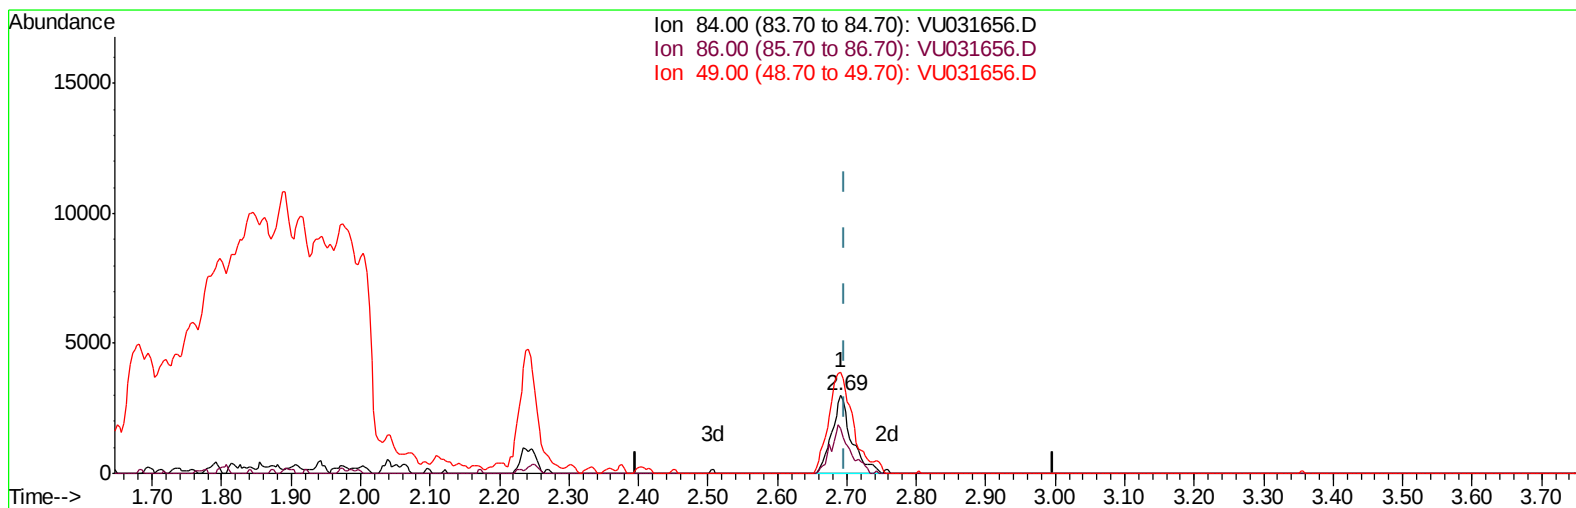

TIC: VU031656.D

(16) Methylene chloride (T)

2.691min (-0.006) 0.76ug/L m

response 5904

Ion	Exp%	Act%
84.00	100	100
86.00	63.90	57.45
49.00	137.90	130.22
0.00	0.00	0.00