

Data File : VU031646.D
Acq On : 30 Apr 2019 19:59
Operator : JC/SP
Sample : K2593-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X79

Quant Time: May 01 01:44:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	671844	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	660025	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	231970	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	304352	54.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	108.26%
7) Chloroethane-d5	1.68	69	225102	51.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.60%
11) 1,1-Dichloroethene-d2	2.27	63	452585	40.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.84%
21) 2-Butanone-d5	4.19	46	489103	96.01	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.01%
24) Chloroform-d	4.64	84	513786	49.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.78%
26) 1,2-Dichloroethane-d4	5.31	65	358958	53.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.70%
32) Benzene-d6	5.34	84	982668	48.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.96%
36) 1,2-Dichloropropane-d6	6.33	67	359128	50.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.72%
41) Toluene-d8	7.56	98	795683	45.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.14%
43) trans-1,3-Dichloropropene-	7.85	79	133897	43.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.48%
47) 2-Hexanone-d5	8.31	63	264245	85.62	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.62%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	430785	45.02	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.04%
64) 1,2-Dichlorobenzene-d4	11.86	152	228471	46.83	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.66%

Target Compounds


						Qvalue
9) Trichlorofluoromethane	1.88	101	53708	5.638	ug/L	100
10) 1,1,2-Trichloro-1,2,2-trif	2.26	101	3820	0.709	ug/L #	23
12) 1,1-Dichloroethene	2.27	96	3638	0.694	ug/L #	1
34) Trichloroethene	6.18	95	3973553	675.513	ug/L	93
42) Toluene	7.64	91	13439	0.556	ug/L	94
46) Tetrachloroethene	8.22	164	40066	9.991	ug/L	92
48) 2-Hexanone	8.37	43	20358	2.375	ug/L #	71
59) 1,2,3-Trichloropropane	11.48	75	32721	4.006	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU031646.D
Acq On : 30 Apr 2019 19:59
Operator : JC/SP
Sample : K2593-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X79

Quant Time: May 01 01:44:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 01:38:49 2019
Response via : Initial Calibration

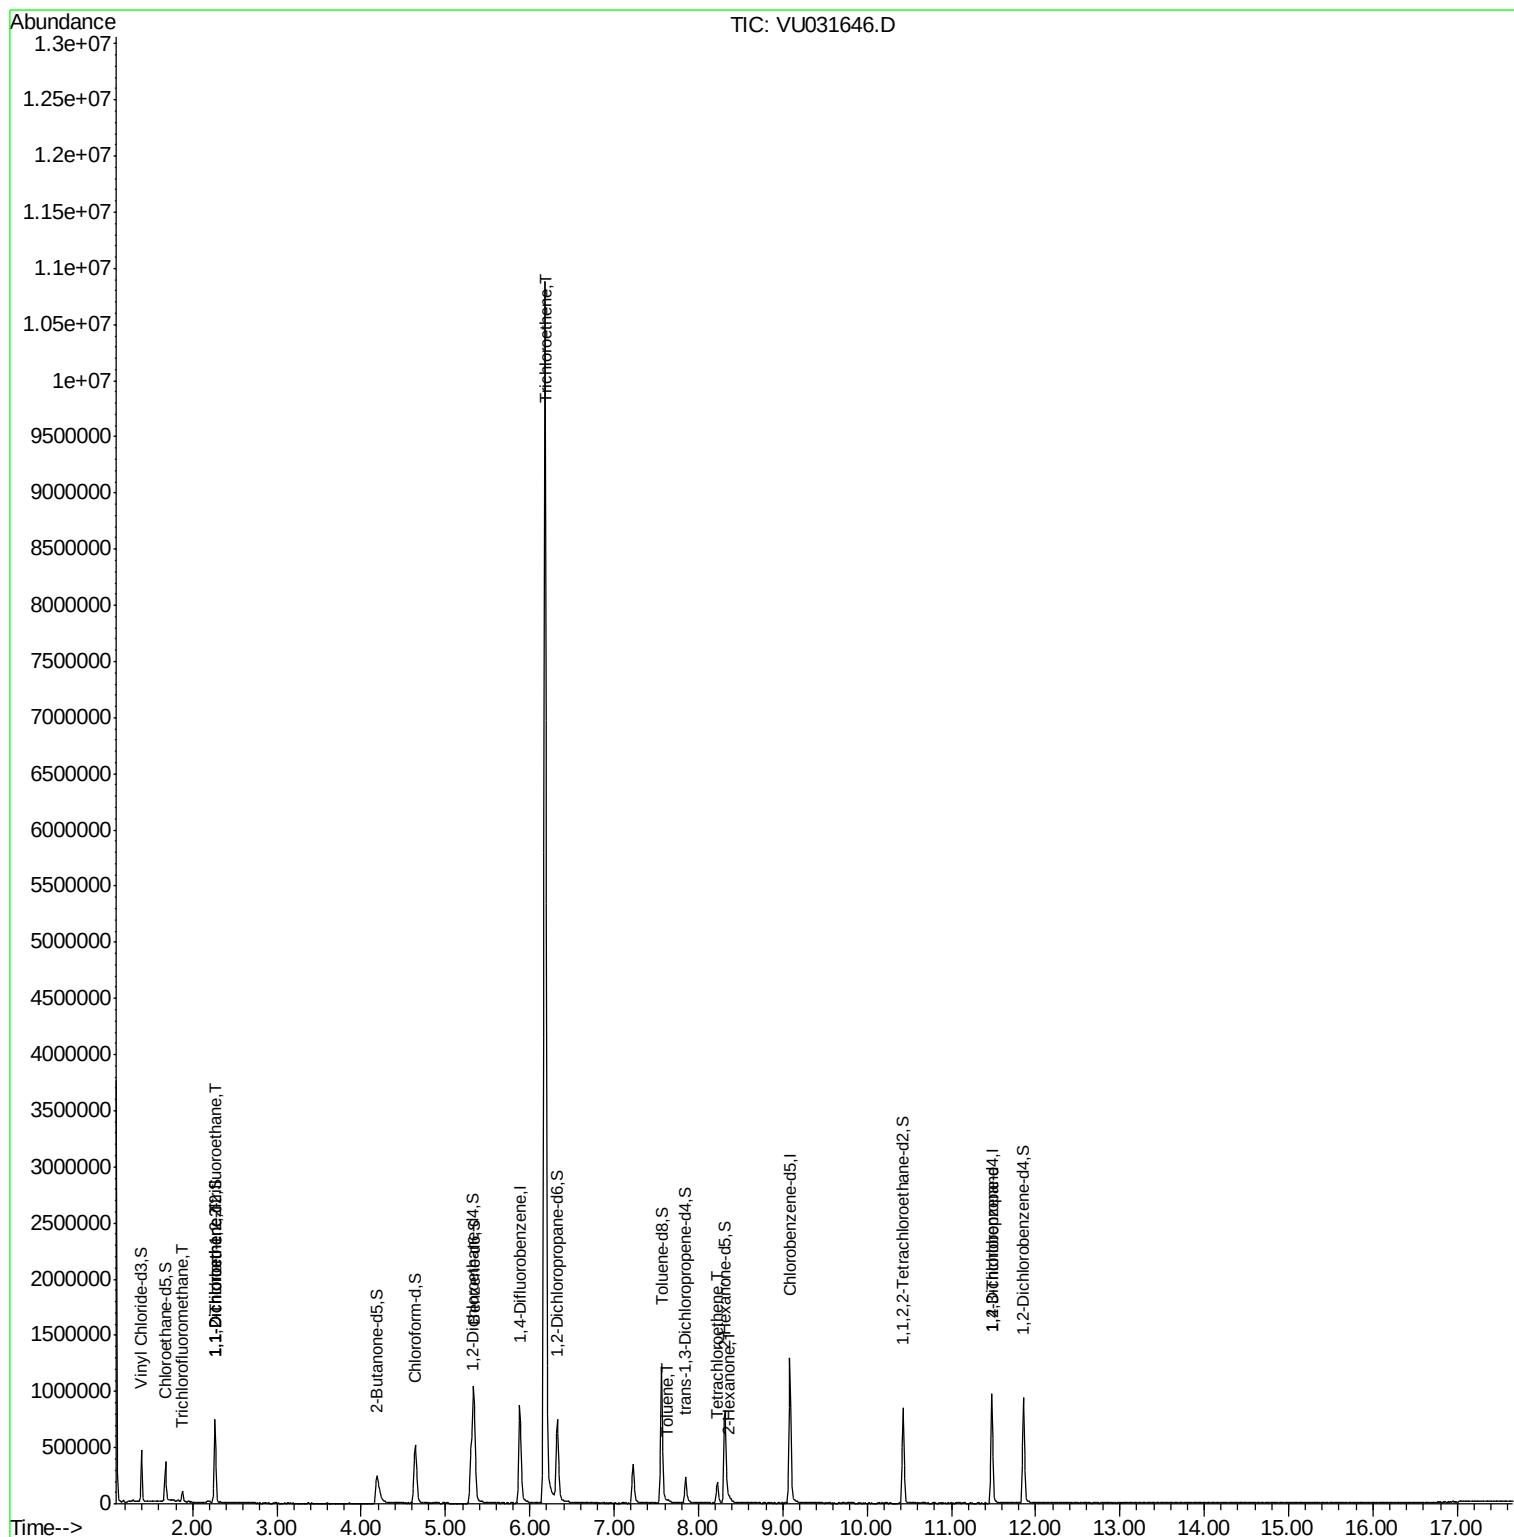




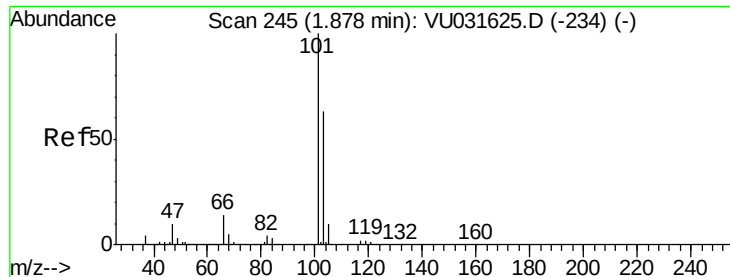


#9

Trichlorofluoromethane
 Concen: 5.638 ug/L
 RT: 1.88 min Scan# 245
 Delta R.T. -0.00 min
 Lab File: VU031646.D
 Acq: 30 Apr 2019 19:59

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X79




Tgt Ion:101 Resp: 53708
 Ion Ratio Lower Upper
 101 100
 103 63.8 50.8 76.2

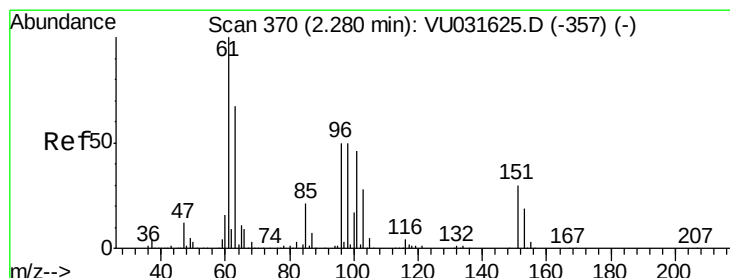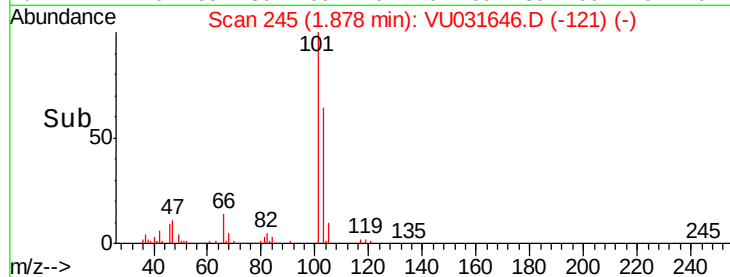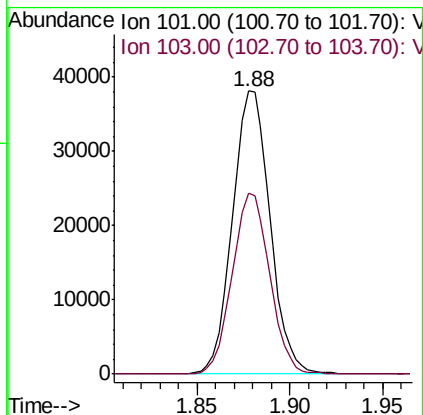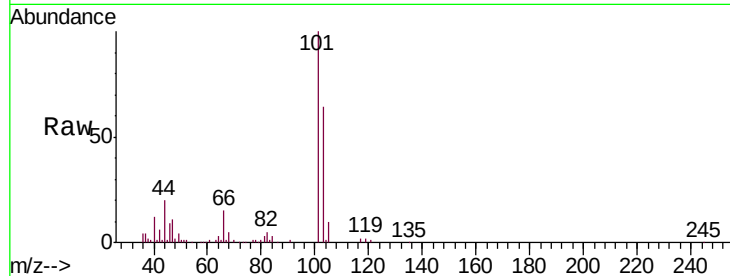


#10

1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.709 ug/L
 RT: 2.26 min Scan# 365
 Delta R.T. -0.02 min
 Lab File: VU031646.D
 Acq: 30 Apr 2019 19:59

Tgt Ion:101 Resp: 3820
 Ion Ratio Lower Upper
 101 100
 85 2.5 36.1 54.1#
 151 0.0 56.1 84.1#


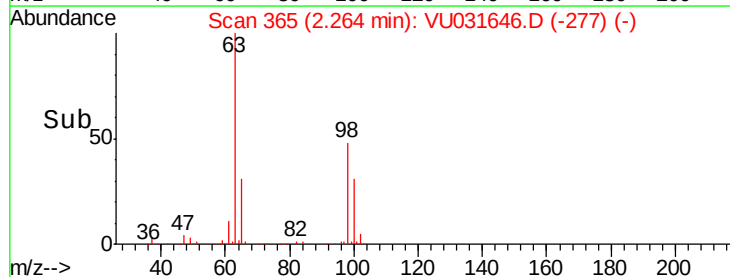
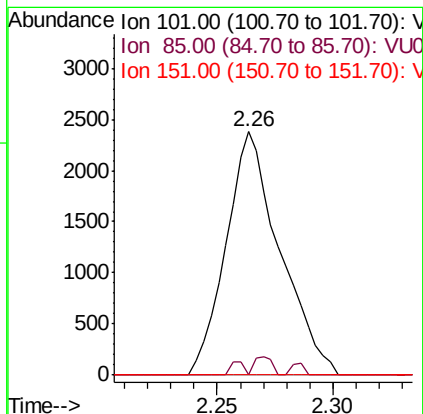
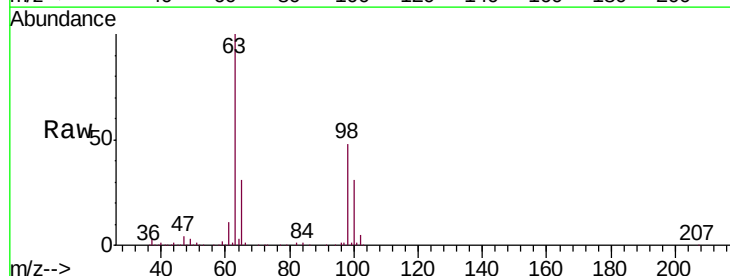


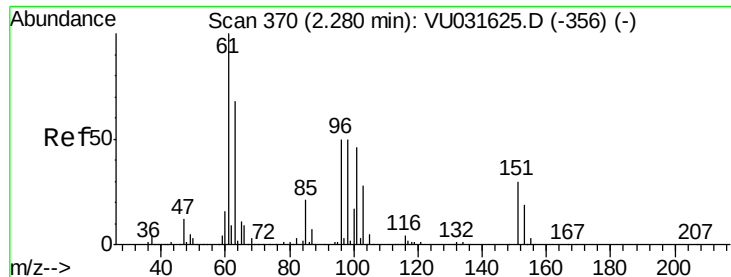

#12
 1,1-Dichloroethene
 Concen: 0.694 ug/L
 RT: 2.27 min Scan# 366
 Delta R.T. -0.01 min
 Lab File: VU031646.D
 Acq: 30 Apr 2019 19:59




Instrument :
 MSVOA_U
 ClientSampleId :
 C0X79


Tgt Ion: 96 Resp: 3638
 Ion Ratio Lower Upper
 96 100
 61 1487.6 135.0 250.6#
 63 13232.5 103.5 192.3#

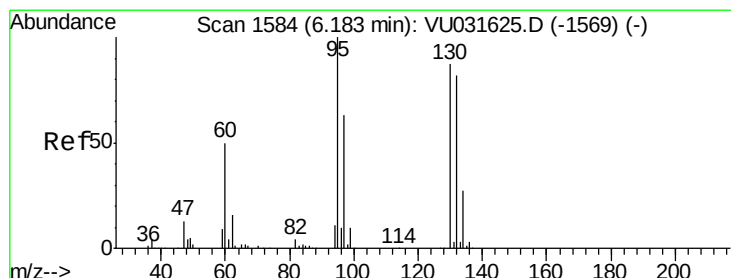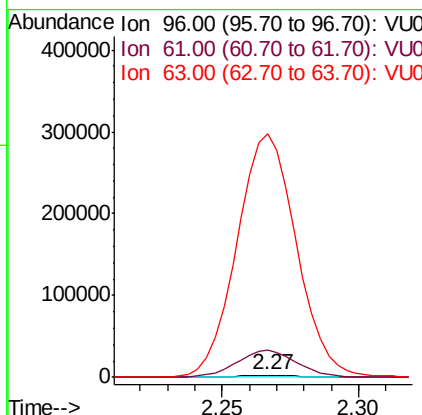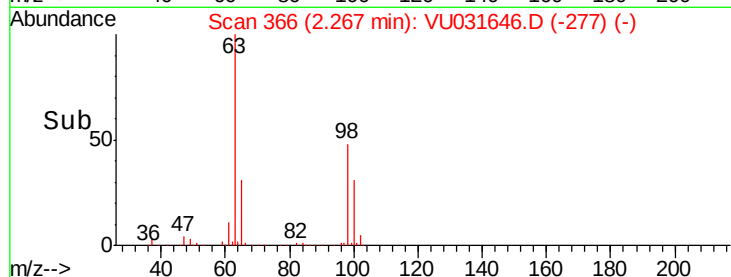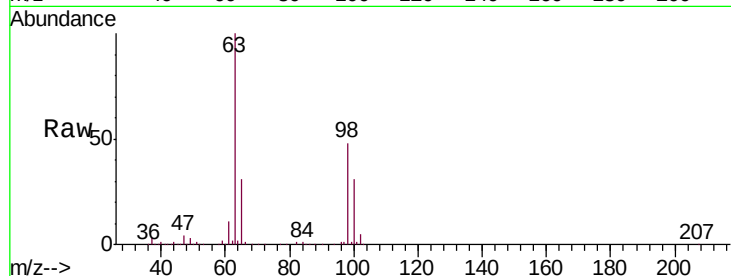

#34
 Trichloroethene
 Concen: 675.513 ug/L
 RT: 6.18 min Scan# 1583
 Delta R.T. -0.00 min
 Lab File: VU031646.D
 Acq: 30 Apr 2019 19:59

Tgt Ion: 95 Resp: 3973553
 Ion Ratio Lower Upper
 95 100
 97 62.7 44.8 83.2
 132 81.6 63.1 117.1
 130 86.4 66.5 123.5

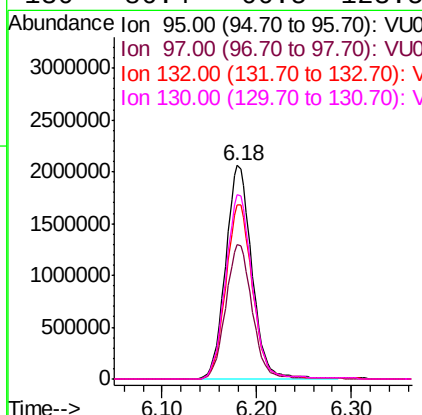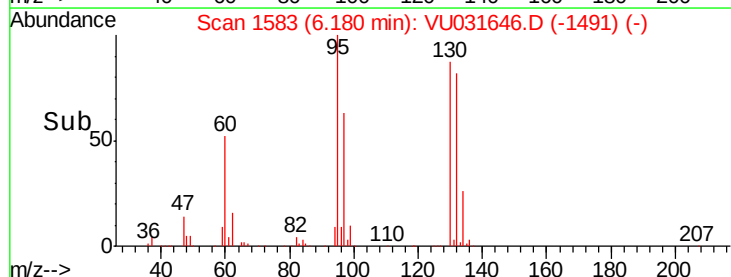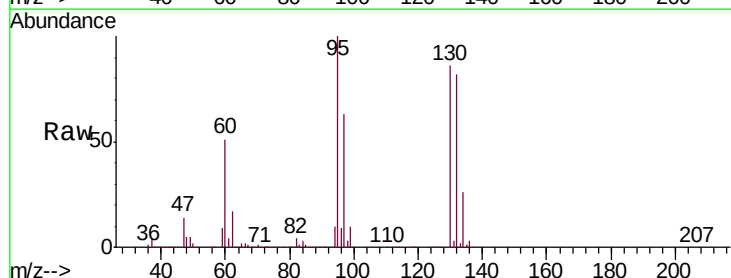

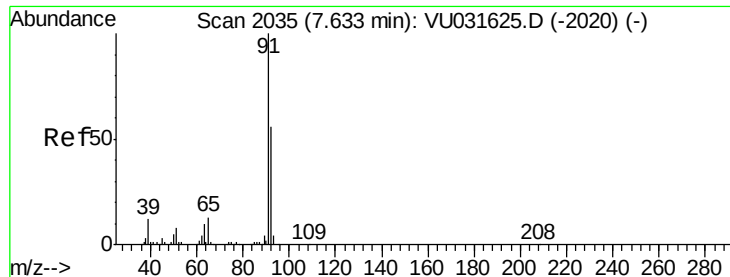

#42

Toluene

Concen: 0.556 ug/L

RT: 7.64 min Scan# 2037

Delta R.T. 0.01 min

Lab File: VU031646.D

Acq: 30 Apr 2019 19:59

Instrument :

MSVOA_U

ClientSampleId :


C0X79

Tgt Ion: 91 Resp: 13439

Ion Ratio Lower Upper




91 100

92 60.0 39.0 72.4

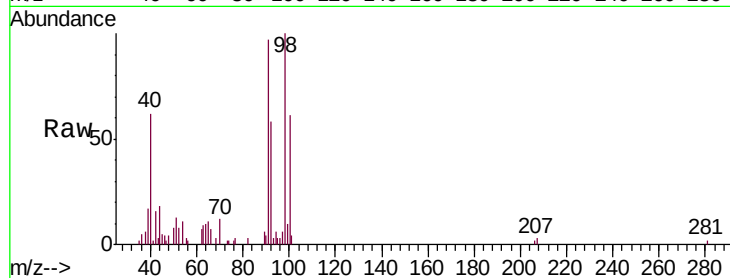

Abundance Ion 91.00 (90.70 to 91.70): VU031625.D (-2020) (-)

Ion 92.00 (91.70 to 92.70): VU031625.D (-2020) (-)

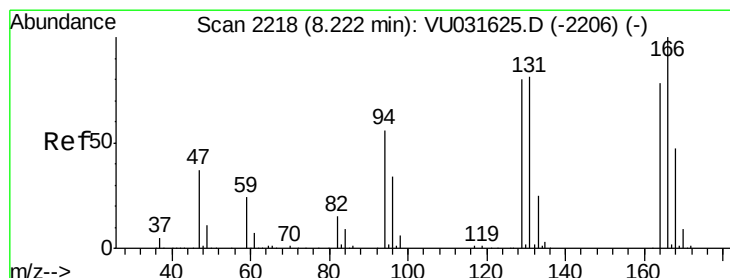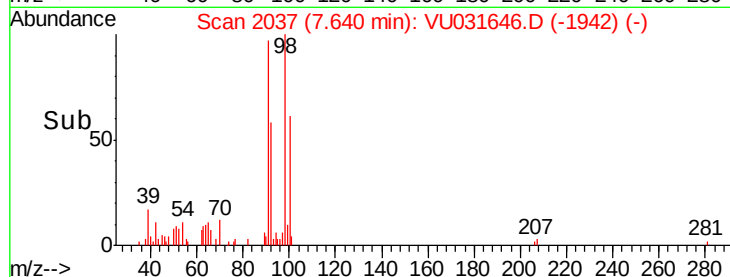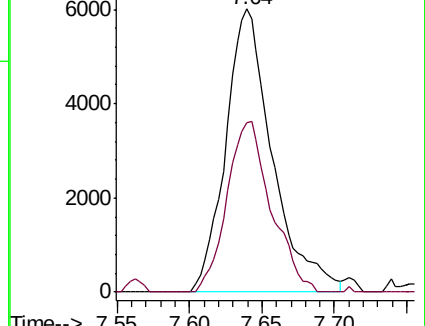

#46

Tetrachloroethene

Concen: 9.991 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. -0.00 min

Lab File: VU031646.D

Acq: 30 Apr 2019 19:59

Tgt Ion: 164 Resp: 40066


Ion Ratio Lower Upper

164 100

129 103.4 71.5 132.9

131 91.4 69.0 128.2

166 116.5 93.7 173.9


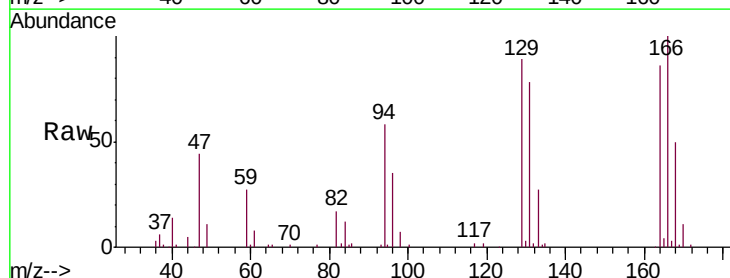



Abundance Ion 164.00 (163.70 to 164.70): VU031625.D (-2206) (-)

Ion 129.00 (128.70 to 129.70): VU031625.D (-2206) (-)

Ion 131.00 (130.70 to 131.70): VU031625.D (-2206) (-)

Ion 166.00 (165.70 to 166.70): VU031625.D (-2206) (-)



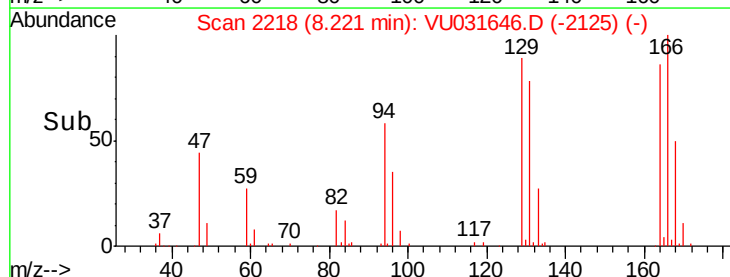
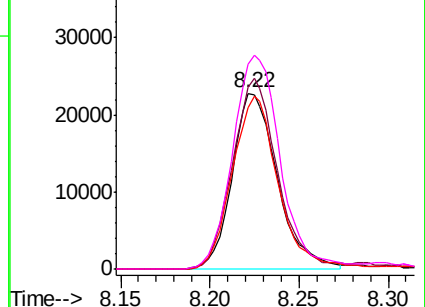


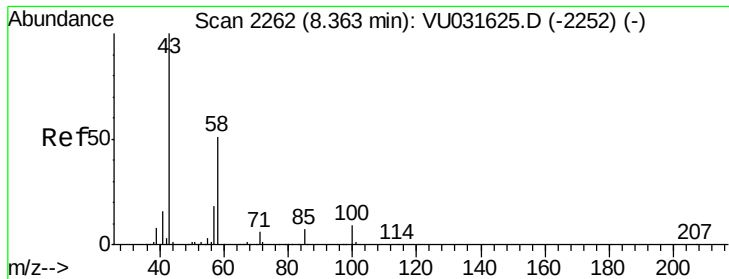

#48
2-Hexanone
Concen: 2.375 ug/L
RT: 8.37 min Scan# 2265
Delta R.T. 0.01 min
Lab File: VU031646.D
Acq: 30 Apr 2019 19:59

Instrument :
MSVOA_U
ClientSampleId :
C0X79

Tgt Ion: 43 Resp: 20358
Ion Ratio Lower Upper
43 100
58 32.1 42.1 63.1#
57 4.1 14.6 22.0#
100 1.4 7.2 10.8#

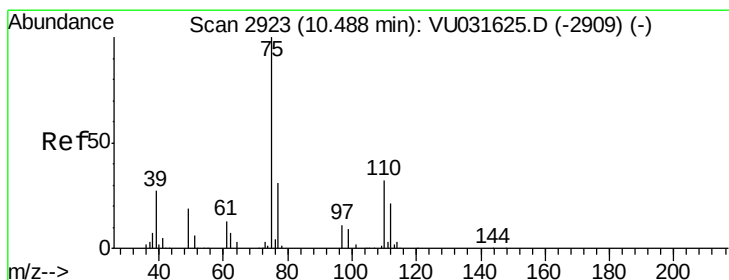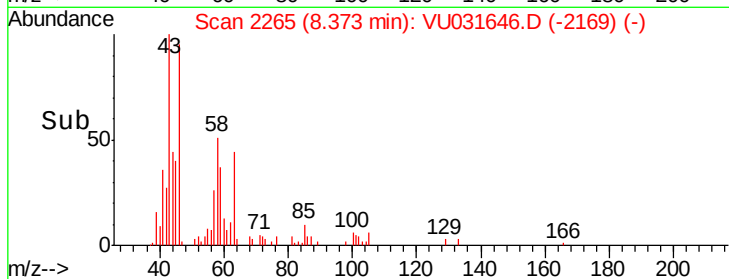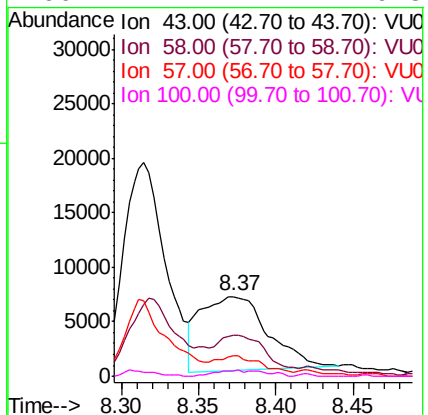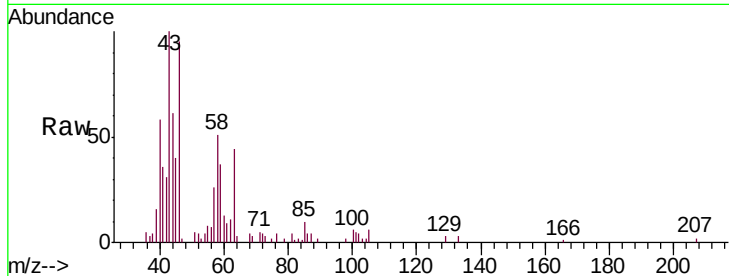

#59
1,2,3-Trichloropropane
Concen: 4.006 ug/L
RT: 11.48 min Scan# 3231
Delta R.T. 0.99 min
Lab File: VU031646.D
Acq: 30 Apr 2019 19:59

Tgt Ion: 75 Resp: 32721
Ion Ratio Lower Upper
75 100
77 37.4 25.9 38.9

