

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031627.D
 Acq On : 30 Apr 2019 12:36
 Operator : JC/SP
 Sample : K2606-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5143

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rVB4	21759	23469	0.75%	0.102%
2	1.395	88	95	106	rBV	462811	504555	16.13%	2.201%
3	1.678	176	183	196	rBV	348266	448247	14.33%	1.956%
4	2.267	356	366	378	rBV	744894	1136650	36.34%	4.959%
5	2.338	380	388	418	rVB	86808	219514	7.02%	0.958%
6	2.698	492	500	517	rVB	75960	142724	4.56%	0.623%
7	2.833	533	542	556	rVB3	14541	31422	1.00%	0.137%
8	2.977	584	587	588	rBV	1637	1033	0.03%	0.005%
9	2.990	588	591	594	rVV5	2629	2200	0.07%	0.010%
10	3.006	594	596	601	rVV4	2007	1724	0.06%	0.008%
11	3.032	601	604	610	rVB3	2508	2398	0.08%	0.010%
12	3.090	616	622	623	rBV4	1132	1031	0.03%	0.004%
13	3.129	631	634	637	rBV2	1447	1043	0.03%	0.005%
14	3.247	664	671	675	rVB5	1735	2064	0.07%	0.009%
15	3.296	680	686	692	rBV3	1499	1785	0.06%	0.008%
16	3.447	725	733	736	rVB4	1253	1240	0.04%	0.005%
17	3.502	745	750	753	rVB5	1367	1075	0.03%	0.005%
18	3.723	814	819	822	rBV4	1434	1080	0.03%	0.005%
19	3.749	822	827	830	rBV5	1258	1130	0.04%	0.005%
20	3.839	852	855	859	rVB2	1256	900	0.03%	0.004%
21	4.022	906	912	916	rBV4	1344	1576	0.05%	0.007%
22	4.077	927	929	934	rBV3	1695	1579	0.05%	0.007%
23	4.116	938	941	945	rVB2	1216	894	0.03%	0.004%
24	4.190	945	964	999	rBV	238002	839281	26.83%	3.661%
25	4.640	1086	1104	1128	rBV	522859	1283915	41.05%	5.601%
26	4.942	1194	1198	1202	rVB3	1856	1570	0.05%	0.007%
27	4.974	1202	1208	1211	rBV5	2638	3235	0.10%	0.014%
28	5.154	1259	1264	1266	rVV3	1884	1871	0.06%	0.008%
29	5.173	1266	1270	1276	rVB5	1457	1534	0.05%	0.007%
30	5.334	1297	1320	1345	rBV3	1046568	3127874	100.00%	13.646%
31	5.778	1455	1458	1461	rBV3	1686	1026	0.03%	0.004%
32	5.881	1475	1490	1515	rBV	806153	1672503	53.47%	7.296%
33	6.074	1548	1550	1558	rVB7	2407	1955	0.06%	0.009%
34	6.186	1573	1585	1597	rBV7	18360	43893	1.40%	0.191%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031627.D
 Acq On : 30 Apr 2019 12:36
 Operator : JC/SP
 Sample : K2606-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5143

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.325	1614	1628	1652	rBV	695601	1451136	46.39%	6.331%
36	6.701	1741	1745	1748	rBV5	1211	1152	0.04%	0.005%
37	6.730	1751	1754	1761	rVB6	1635	1748	0.06%	0.008%
38	6.759	1761	1763	1768	rBV4	1012	1128	0.04%	0.005%
39	6.788	1768	1772	1776	rVB5	1490	1229	0.04%	0.005%
40	6.871	1794	1798	1801	rVB3	1734	1442	0.05%	0.006%
41	6.894	1801	1805	1807	rBV2	1813	1257	0.04%	0.005%
42	6.935	1816	1818	1824	rVB5	1369	1107	0.04%	0.005%
43	7.128	1872	1878	1880	rBV3	2045	1717	0.05%	0.007%
44	7.225	1895	1908	1924	rBV	343057	642747	20.55%	2.804%
45	7.472	1977	1985	1992	rBV8	4721	7651	0.24%	0.033%
46	7.562	2000	2013	2035	rBV	1193940	2181494	69.74%	9.517%
47	7.849	2092	2102	2130	rBV	229847	430325	13.76%	1.877%
48	8.006	2148	2151	2154	rBV4	1062	955	0.03%	0.004%
49	8.087	2173	2176	2181	rVB5	1420	1171	0.04%	0.005%
50	8.119	2181	2186	2190	rBV4	1737	2157	0.07%	0.009%
51	8.173	2194	2203	2217	rVB3	24751	47731	1.53%	0.208%
52	8.260	2224	2230	2232	rBV5	1314	1130	0.04%	0.005%
53	8.312	2236	2246	2286	rVV2	800909	1721071	55.02%	7.508%
54	8.472	2289	2296	2309	rVB5	36606	68882	2.20%	0.301%
55	8.784	2390	2393	2395	rBV5	1856	1230	0.04%	0.005%
56	8.894	2422	2427	2434	rBV6	1509	2166	0.07%	0.009%
57	8.926	2434	2437	2440	rVB3	1639	1192	0.04%	0.005%
58	8.948	2440	2444	2447	rBV4	2121	1709	0.05%	0.007%
59	9.086	2474	2487	2521	rBV	1203516	2082726	66.59%	9.086%
60	9.382	2575	2579	2589	rVB8	2988	5143	0.16%	0.022%
61	9.427	2591	2593	2596	rBV3	1530	1067	0.03%	0.005%
62	9.501	2613	2616	2619	rBV2	1454	923	0.03%	0.004%
63	9.675	2668	2670	2674	rBV3	1189	1010	0.03%	0.004%
64	9.784	2696	2704	2707	rBV6	2524	2621	0.08%	0.011%
65	9.803	2707	2710	2712	rBV3	1591	1125	0.04%	0.005%
66	9.877	2730	2733	2736	rVB3	1413	1010	0.03%	0.004%
67	9.910	2739	2743	2747	rBV6	1305	1091	0.03%	0.005%
68	9.948	2750	2755	2756	rBV3	1681	1233	0.04%	0.005%
69	10.045	2776	2785	2793	rBV8	4601	8680	0.28%	0.038%
70	10.128	2807	2811	2813	rBV4	1790	1106	0.04%	0.005%
71	10.148	2813	2817	2822	rVB3	2136	2215	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031627.D
 Acq On : 30 Apr 2019 12:36
 Operator : JC/SP
 Sample : K2606-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5143

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.176	2822	2826	2827	rBV2	1167	887	0.03%	0.004%
73	10.250	2839	2849	2859	rVB7	4207	9781	0.31%	0.043%
74	10.427	2891	2904	2930	rBV	855244	1392462	44.52%	6.075%
75	10.604	2948	2959	2971	rBV2	20507	35403	1.13%	0.154%
76	10.746	3001	3003	3007	rVB3	1709	1077	0.03%	0.005%
77	10.775	3007	3012	3014	rBV	1952	1594	0.05%	0.007%
78	10.823	3025	3027	3032	rVB4	2145	1266	0.04%	0.006%
79	10.871	3039	3042	3046	rBV	1265	912	0.03%	0.004%
80	10.942	3060	3064	3070	rVB5	1416	1366	0.04%	0.006%
81	11.025	3085	3090	3093	rBV3	1137	1030	0.03%	0.004%
82	11.061	3098	3101	3104	rBV2	1396	1298	0.04%	0.006%
83	11.141	3120	3126	3127	rBV2	1353	1033	0.03%	0.005%
84	11.160	3128	3132	3138	rVV7	2915	3749	0.12%	0.016%
85	11.379	3197	3200	3204	rBV6	2675	2284	0.07%	0.010%
86	11.482	3220	3232	3251	rBV	964829	1568510	50.15%	6.843%
87	11.652	3281	3285	3289	rBV5	2021	2078	0.07%	0.009%
88	11.684	3293	3295	3301	rVB4	2642	1519	0.05%	0.007%
89	11.758	3311	3318	3330	rBV7	10943	22746	0.73%	0.099%
90	11.858	3337	3349	3371	rBV	987150	1655592	52.93%	7.223%
91	12.475	3533	3541	3551	rBV2	7234	11915	0.38%	0.052%
92	12.845	3654	3656	3662	rVB3	3227	2450	0.08%	0.011%
93	13.057	3719	3722	3726	rBV4	1488	1229	0.04%	0.005%
94	13.125	3741	3743	3749	rBV4	1208	1093	0.03%	0.005%
95	13.385	3821	3824	3831	rBV6	2019	1890	0.06%	0.008%
96	13.749	3934	3937	3939	rBV3	1395	955	0.03%	0.004%
97	14.180	4069	4071	4074	rVB2	1662	897	0.03%	0.004%
98	14.591	4196	4199	4202	rBV2	2085	1381	0.04%	0.006%
99	14.652	4216	4218	4225	rVB6	2718	2202	0.07%	0.010%
100	15.260	4404	4407	4410	rBV4	2443	2191	0.07%	0.010%


Sum of corrected areas: 22922257

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031627.D
Acq On : 30 Apr 2019 12:36
Operator : JC/SP
Sample : K2606-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5143

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

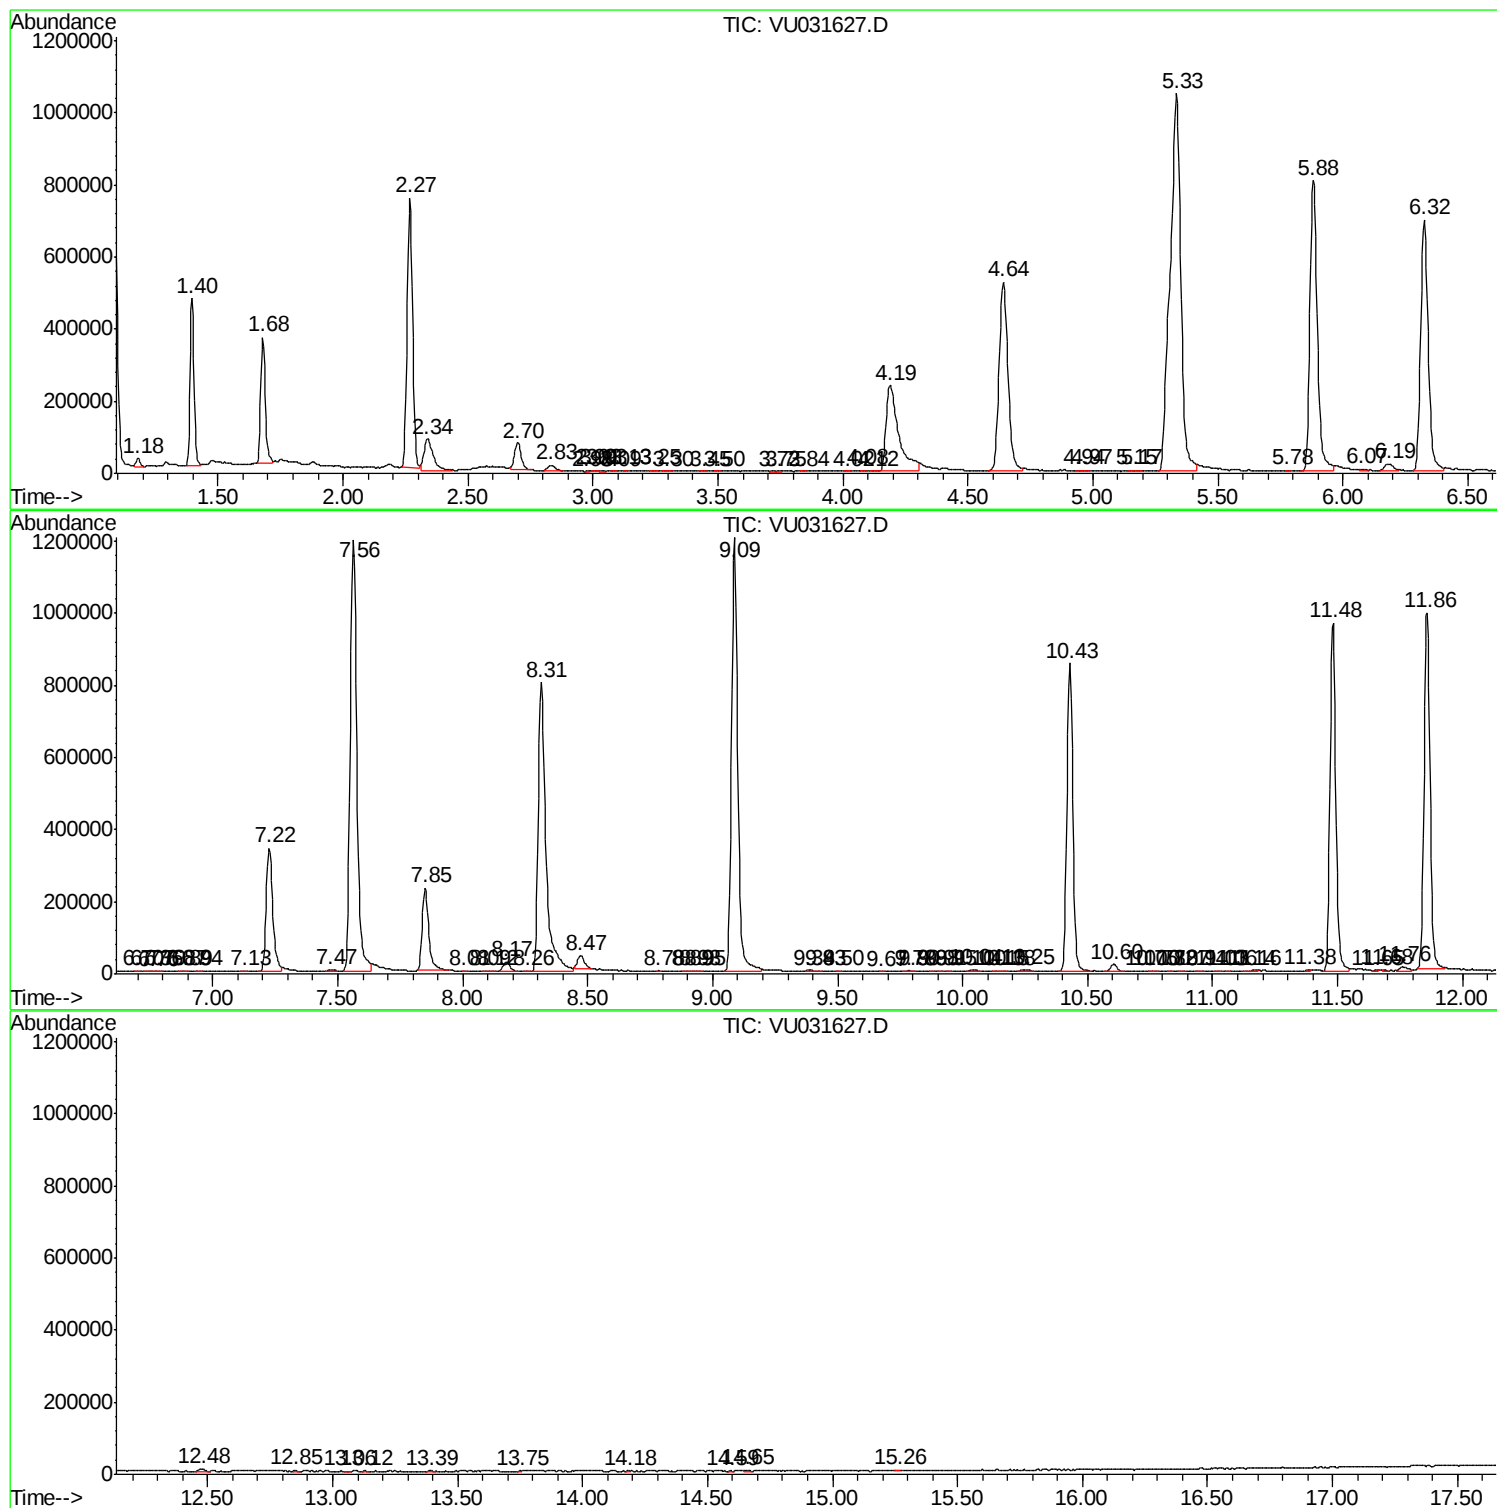

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031627.D
Acq On : 30 Apr 2019 12:36
Operator : JC/SP
Sample : K2606-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5143

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031627.D
Acq On : 30 Apr 2019 12:36
Operator : JC/SP
Sample : K2606-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5143

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc