

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031637.D
 Acq On : 30 Apr 2019 16:29
 Operator : JC/SP
 Sample : K2593-05DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB	15336	14322	0.45%	0.058%
2	1.290	59	62	67	rVB	12487	9762	0.31%	0.040%
3	1.396	87	95	107	rBV	445870	499345	15.62%	2.028%
4	1.675	175	182	198	rBV	366630	453520	14.19%	1.842%
5	2.267	355	366	379	rVB	746720	1131458	35.40%	4.596%
6	2.695	495	499	500	rBV4	1896	1277	0.04%	0.005%
7	2.823	535	539	543	rBV5	972	987	0.03%	0.004%
8	2.846	543	546	550	rVV3	1035	619	0.02%	0.003%
9	2.997	591	593	596	rBV2	1135	652	0.02%	0.003%
10	3.132	631	635	637	rVB2	1065	688	0.02%	0.003%
11	3.154	638	642	645	rBV2	1223	1079	0.03%	0.004%
12	3.309	687	690	695	rVB4	1314	718	0.02%	0.003%
13	3.334	695	698	702	rVB2	1225	1003	0.03%	0.004%
14	3.354	702	704	706	rBV3	1113	545	0.02%	0.002%
15	3.379	706	712	714	rBV5	989	1080	0.03%	0.004%
16	3.518	752	755	760	rVB3	1247	963	0.03%	0.004%
17	3.559	763	768	771	rBV	878	803	0.03%	0.003%
18	3.701	810	812	818	rVB2	1525	1316	0.04%	0.005%
19	3.791	836	840	842	rBV2	1088	850	0.03%	0.003%
20	3.878	863	867	870	rBV2	811	801	0.03%	0.003%
21	3.932	881	884	889	rVB3	752	565	0.02%	0.002%
22	4.061	922	924	928	rVB2	1034	569	0.02%	0.002%
23	4.132	942	946	950	rVB2	1145	1100	0.03%	0.004%
24	4.186	950	963	994	rBV	258274	798005	24.97%	3.241%
25	4.640	1085	1104	1132	rBV	518227	1238382	38.75%	5.030%
26	4.810	1154	1157	1158	rBV2	1238	708	0.02%	0.003%
27	4.945	1194	1199	1203	rVB6	1229	1358	0.04%	0.006%
28	4.977	1204	1209	1211	rBV3	3291	3100	0.10%	0.013%
29	5.032	1223	1226	1229	rVB3	1401	992	0.03%	0.004%
30	5.129	1252	1256	1261	rBV5	1708	2044	0.06%	0.008%
31	5.219	1281	1284	1287	rBV3	1176	737	0.02%	0.003%
32	5.334	1296	1320	1362	rBV2	1058749	3195895	100.00%	12.982%
33	5.624	1408	1410	1412	rBV3	932	555	0.02%	0.002%
34	5.736	1442	1445	1452	rVB5	1960	1566	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031637.D
 Acq On : 30 Apr 2019 16:29
 Operator : JC/SP
 Sample : K2593-05DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 C0XD7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.765	1452	1454	1457	rBV3	1524	688	0.02%	0.003%
36	5.833	1469	1475	1477	rBV3	1050	1015	0.03%	0.004%
37	5.881	1477	1490	1507	rBV	879212	1772349	55.46%	7.199%
38	6.180	1570	1583	1609	rBV2	1024557	2062136	64.52%	8.376%
39	6.325	1616	1628	1658	rVB	717438	1466777	45.90%	5.958%
40	6.559	1698	1701	1709	rVB7	2040	2060	0.06%	0.008%
41	6.656	1728	1731	1734	rVB3	1734	876	0.03%	0.004%
42	6.685	1738	1740	1742	rVB3	1240	540	0.02%	0.002%
43	6.756	1759	1762	1765	rVB2	1627	1013	0.03%	0.004%
44	6.887	1797	1803	1806	rBV7	1569	1833	0.06%	0.007%
45	6.984	1829	1833	1834	rBV3	1062	597	0.02%	0.002%
46	7.055	1849	1855	1860	rVB5	1074	1260	0.04%	0.005%
47	7.090	1860	1866	1869	rBV3	1483	1336	0.04%	0.005%
48	7.116	1869	1874	1877	rBV3	1530	1527	0.05%	0.006%
49	7.225	1896	1908	1927	rBV	343787	649672	20.33%	2.639%
50	7.563	1999	2013	2039	rBV	1206367	2206523	69.04%	8.963%
51	7.849	2091	2102	2126	rBV	230845	425409	13.31%	1.728%
52	8.103	2178	2181	2183	rBV2	1236	930	0.03%	0.004%
53	8.161	2196	2199	2202	rBV5	1079	863	0.03%	0.004%
54	8.228	2209	2220	2230	rBV4	33199	58508	1.83%	0.238%
55	8.312	2235	2246	2281	rBV	854229	1721108	53.85%	6.991%
56	8.572	2325	2327	2331	rBV3	1359	774	0.02%	0.003%
57	8.714	2368	2371	2376	rBV2	1590	1155	0.04%	0.005%
58	8.900	2426	2429	2432	rBV4	1559	963	0.03%	0.004%
59	8.961	2444	2448	2453	rBV3	1295	1216	0.04%	0.005%
60	8.984	2453	2455	2458	rVB4	880	540	0.02%	0.002%
61	9.032	2465	2470	2474	rBV4	1671	1766	0.06%	0.007%
62	9.087	2474	2487	2532	rVV	1288671	2254597	70.55%	9.158%
63	9.421	2589	2591	2595	rVB4	1116	855	0.03%	0.003%
64	9.440	2595	2597	2600	rBV3	1287	842	0.03%	0.003%
65	9.460	2601	2603	2609	rVB5	1593	1450	0.05%	0.006%
66	9.485	2609	2611	2614	rBV2	953	624	0.02%	0.003%
67	9.505	2614	2617	2619	rBV3	1177	680	0.02%	0.003%
68	9.543	2626	2629	2634	rVB5	1094	1044	0.03%	0.004%
69	9.755	2693	2695	2700	rVB4	780	567	0.02%	0.002%
70	9.788	2700	2705	2709	rBV5	1268	1146	0.04%	0.005%
71	9.939	2748	2752	2758	rVB3	1454	1385	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031637.D
 Acq On : 30 Apr 2019 16:29
 Operator : JC/SP
 Sample : K2593-05DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.968	2758	2761	2763	rBV2	1481	922	0.03%	0.004%
73	10.019	2772	2777	2782	rBV4	1621	1845	0.06%	0.007%
74	10.112	2801	2806	2807	rBV2	1116	969	0.03%	0.004%
75	10.122	2807	2809	2812	rVB	1566	825	0.03%	0.003%
76	10.167	2817	2823	2828	rBV5	2013	2899	0.09%	0.012%
77	10.231	2840	2843	2845	rBV2	837	578	0.02%	0.002%
78	10.427	2891	2904	2923	rBV	865104	1391259	43.53%	5.651%
79	10.537	2936	2938	2941	rVB	1264	623	0.02%	0.003%
80	10.672	2977	2980	2982	rBV4	1460	1082	0.03%	0.004%
81	10.762	3006	3008	3013	rVB2	2070	1032	0.03%	0.004%
82	10.791	3014	3017	3019	rBV3	1054	669	0.02%	0.003%
83	10.894	3042	3049	3055	rVB4	1382	1887	0.06%	0.008%
84	10.958	3066	3069	3071	rVB3	982	562	0.02%	0.002%
85	10.990	3072	3079	3083	rBV5	1373	1729	0.05%	0.007%
86	11.042	3093	3095	3100	rVB2	1220	752	0.02%	0.003%
87	11.067	3100	3103	3104	rBV3	1426	892	0.03%	0.004%
88	11.151	3126	3129	3132	rBV2	1077	844	0.03%	0.003%
89	11.170	3133	3135	3138	rVV2	1007	540	0.02%	0.002%
90	11.218	3145	3150	3153	rVB2	1593	1469	0.05%	0.006%
91	11.244	3153	3158	3159	rBV2	578	543	0.02%	0.002%
92	11.315	3176	3180	3182	rBV2	985	787	0.02%	0.003%
93	11.431	3213	3216	3219	rBV3	1564	1174	0.04%	0.005%
94	11.482	3219	3232	3259	rBV	965508	1578786	49.40%	6.413%
95	11.858	3334	3349	3371	rBV	948831	1606383	50.26%	6.525%
96	12.360	3503	3505	3508	rBV2	993	600	0.02%	0.002%
97	12.771	3629	3633	3634	rBV	1803	1264	0.04%	0.005%
98	12.974	3693	3696	3697	rBV	1674	853	0.03%	0.003%
99	13.099	3732	3735	3740	rBV4	1569	1464	0.05%	0.006%
100	13.614	3892	3895	3897	rBV3	1668	1242	0.04%	0.005%


Sum of corrected areas: 24618462

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031637.D
Acq On : 30 Apr 2019 16:29
Operator : JC/SP
Sample : K2593-05DL 2500X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

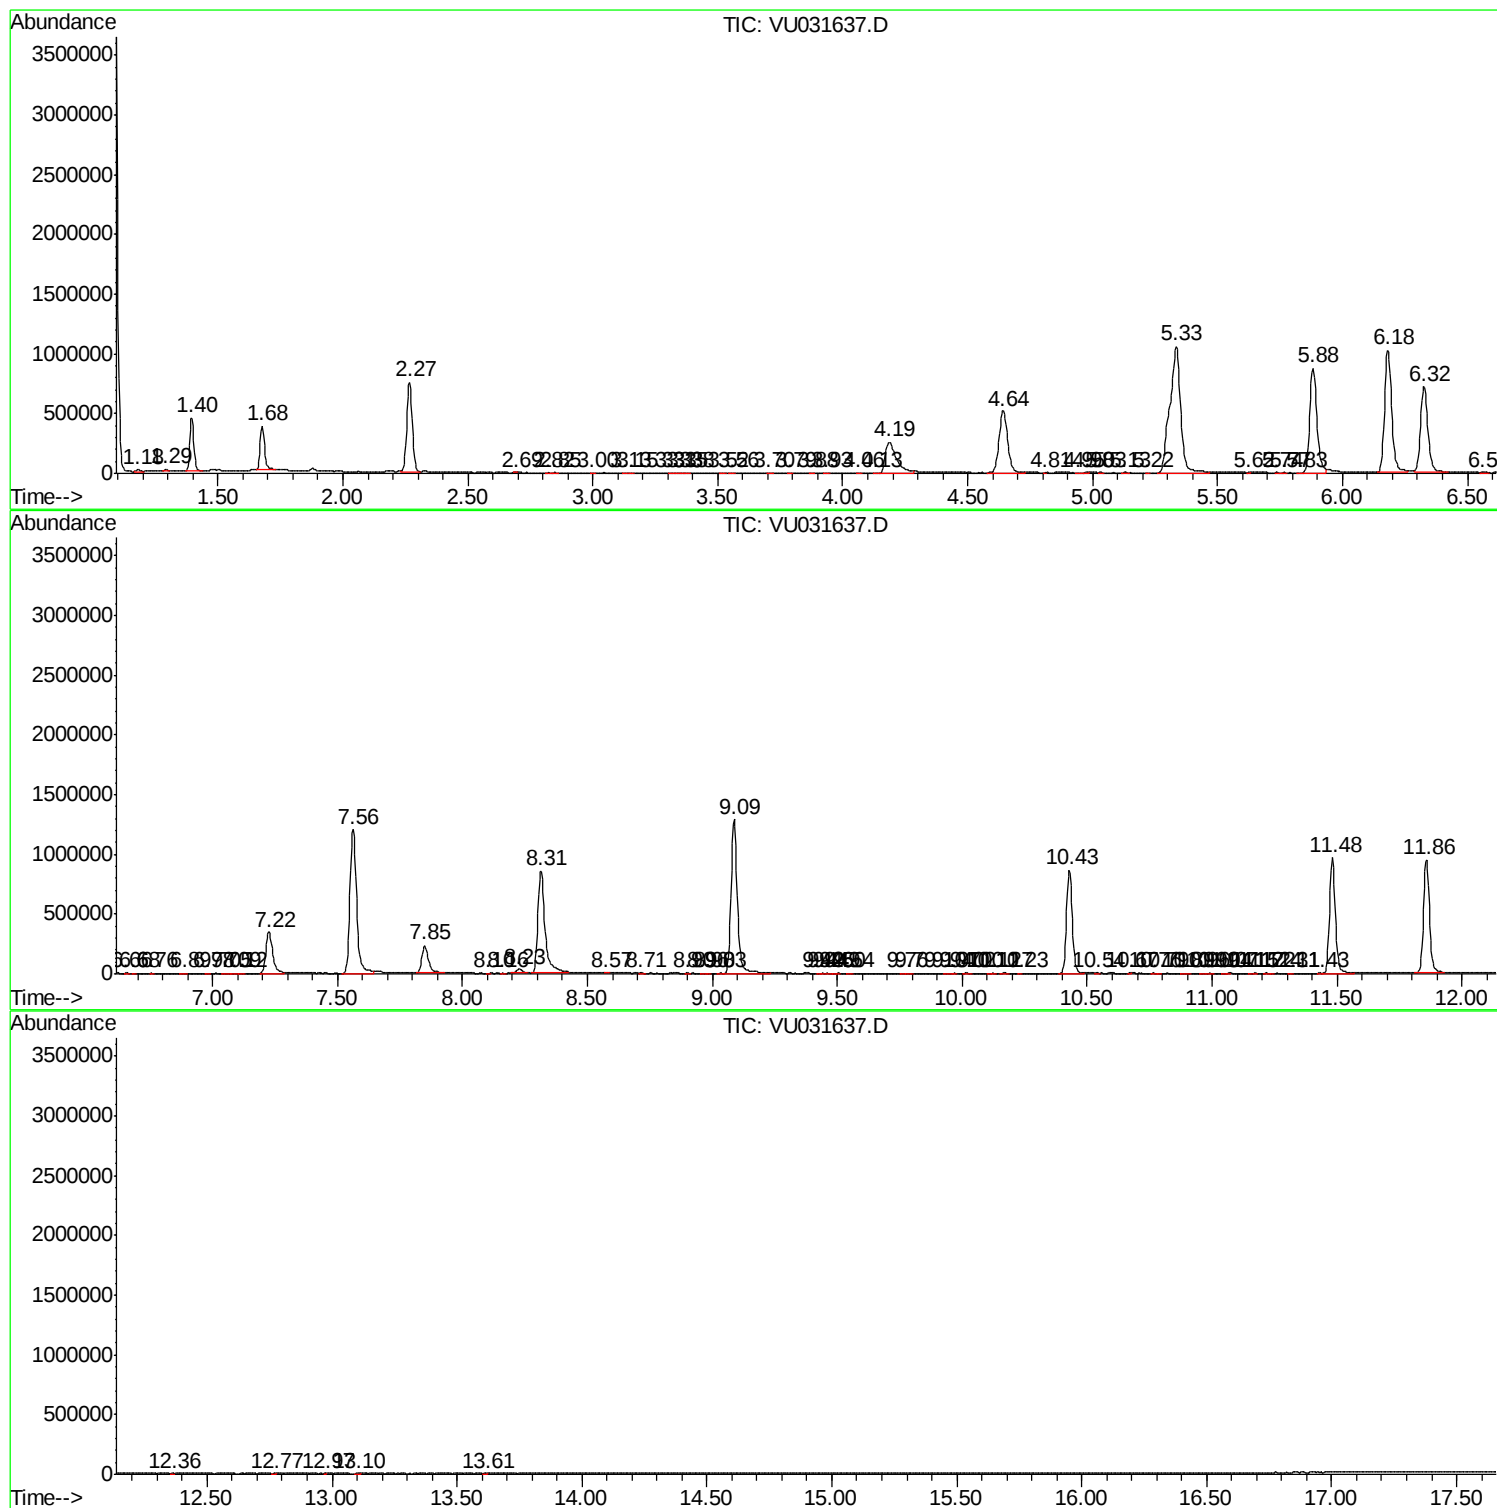

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031637.D
Acq On : 30 Apr 2019 16:29
Operator : JC/SP
Sample : K2593-05DL 2500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU043019\
Data File : VU031637.D
Acq On : 30 Apr 2019 16:29
Operator : JC/SP
Sample : K2593-05DL 2500X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0XD7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc