

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031638.D
 Acq On : 30 Apr 2019 16:52
 Operator : JC/SP
 Sample : K2593-06DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	33	rBV	17567	17526	0.55%	0.072%
2	1.396	87	95	106	rBV	464912	497111	15.58%	2.049%
3	1.679	175	183	196	rBV	356836	450753	14.13%	1.858%
4	2.267	355	366	381	rVB	740711	1129758	35.42%	4.658%
5	2.457	423	425	428	rBV3	1114	846	0.03%	0.003%
6	2.525	443	446	450	rVB3	1282	850	0.03%	0.004%
7	2.627	470	478	480	rBV5	2159	2080	0.07%	0.009%
8	2.701	496	501	511	rVB6	2709	3425	0.11%	0.014%
9	2.762	518	520	524	rVB2	1240	828	0.03%	0.003%
10	2.795	528	530	533	rBV	1336	872	0.03%	0.004%
11	2.827	537	540	543	rBV2	1093	717	0.02%	0.003%
12	2.920	564	569	572	rVV4	904	916	0.03%	0.004%
13	2.946	572	577	579	rVV3	1223	1164	0.04%	0.005%
14	3.039	604	606	611	rVB4	1824	1302	0.04%	0.005%
15	3.068	611	615	620	rVB3	903	844	0.03%	0.003%
16	3.129	630	634	637	rVB2	1625	1031	0.03%	0.004%
17	3.152	637	641	644	rBV2	977	743	0.02%	0.003%
18	3.190	651	653	656	rVB2	1625	955	0.03%	0.004%
19	3.213	656	660	662	rBV2	1270	828	0.03%	0.003%
20	3.351	698	703	706	rVV3	1146	1250	0.04%	0.005%
21	3.373	706	710	716	rVB5	1160	1079	0.03%	0.004%
22	3.463	735	738	743	rVB4	1429	1255	0.04%	0.005%
23	3.499	743	749	753	rBV4	895	1091	0.03%	0.004%
24	3.524	753	757	760	rBV3	836	821	0.03%	0.003%
25	3.560	765	768	774	rVB4	941	944	0.03%	0.004%
26	3.615	780	785	787	rBV	1750	1582	0.05%	0.007%
27	3.708	811	814	820	rVB2	985	957	0.03%	0.004%
28	3.833	849	853	856	rBV2	1037	753	0.02%	0.003%
29	3.991	898	902	906	rBV2	1389	1155	0.04%	0.005%
30	4.116	935	941	943	rBV4	946	836	0.03%	0.003%
31	4.187	951	963	1000	rBV2	247156	801620	25.13%	3.305%
32	4.573	1080	1083	1086	rBV2	1428	1096	0.03%	0.005%
33	4.640	1089	1104	1131	rVV	518881	1235166	38.72%	5.092%
34	4.987	1209	1212	1216	rBV3	1775	1230	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031638.D
 Acq On : 30 Apr 2019 16:52
 Operator : JC/SP
 Sample : K2593-06DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.052	1230	1232	1237	rVB	962	820	0.03%	0.003%
36	5.145	1256	1261	1264	rBV4	1529	1505	0.05%	0.006%
37	5.164	1264	1267	1272	rVB5	1038	756	0.02%	0.003%
38	5.335	1297	1320	1364	rBV2	1055096	3189796	100.00%	13.150%
39	5.881	1477	1490	1517	rBV	876341	1822795	57.14%	7.515%
40	6.180	1570	1583	1612	rBV	810566	1620223	50.79%	6.680%
41	6.325	1616	1628	1657	rVB	710889	1445252	45.31%	5.958%
42	6.659	1730	1732	1736	rVB4	1178	741	0.02%	0.003%
43	6.913	1807	1811	1814	rVV4	1437	1297	0.04%	0.005%
44	6.933	1814	1817	1820	rVV3	1829	1252	0.04%	0.005%
45	7.055	1849	1855	1858	rVB6	956	884	0.03%	0.004%
46	7.129	1872	1878	1883	rVB5	1376	1635	0.05%	0.007%
47	7.171	1883	1891	1893	rBV2	1118	1092	0.03%	0.005%
48	7.225	1896	1908	1932	rBV	347760	652132	20.44%	2.688%
49	7.431	1968	1972	1975	rBV4	1733	1389	0.04%	0.006%
50	7.511	1992	1997	1999	rBV5	1062	1003	0.03%	0.004%
51	7.563	1999	2013	2048	rBV	1191859	2211560	69.33%	9.117%
52	7.846	2090	2101	2131	rBV	232615	442015	13.86%	1.822%
53	8.145	2189	2194	2198	rBV5	927	908	0.03%	0.004%
54	8.225	2209	2219	2234	rBV3	24661	45033	1.41%	0.186%
55	8.312	2235	2246	2283	rBV	854263	1740805	54.57%	7.177%
56	8.733	2374	2377	2381	rBV4	1442	1049	0.03%	0.004%
57	8.900	2427	2429	2434	rVB4	1506	1311	0.04%	0.005%
58	8.933	2434	2439	2442	rBV4	1524	1475	0.05%	0.006%
59	9.026	2461	2468	2472	rBV5	1266	1958	0.06%	0.008%
60	9.087	2473	2487	2529	rVV	1287380	2261412	70.90%	9.323%
61	9.389	2577	2581	2584	rBV4	900	768	0.02%	0.003%
62	9.489	2604	2612	2616	rBV9	1197	1896	0.06%	0.008%
63	9.531	2621	2625	2629	rBV5	1445	1237	0.04%	0.005%
64	9.637	2655	2658	2665	rVB4	1636	1501	0.05%	0.006%
65	9.669	2665	2668	2671	rBV3	1403	752	0.02%	0.003%
66	9.688	2671	2674	2677	rBV3	1168	986	0.03%	0.004%
67	9.762	2694	2697	2700	rBV3	1359	1014	0.03%	0.004%
68	9.952	2751	2756	2758	rBV2	1026	750	0.02%	0.003%
69	9.974	2760	2763	2766	rVV3	1318	791	0.02%	0.003%
70	10.087	2792	2798	2802	rBV3	1309	1216	0.04%	0.005%
71	10.106	2802	2804	2808	rBV4	1181	887	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031638.D
 Acq On : 30 Apr 2019 16:52
 Operator : JC/SP
 Sample : K2593-06DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.363	2878	2884	2887	rVB5	970	926	0.03%	0.004%
73	10.428	2887	2904	2927	rBV	861342	1395580	43.75%	5.753%
74	10.659	2970	2976	2979	rBV5	1422	1570	0.05%	0.006%
75	10.727	2991	2997	3001	rVB5	1319	1531	0.05%	0.006%
76	10.749	3001	3004	3009	rVB2	869	722	0.02%	0.003%
77	10.810	3020	3023	3027	rVB2	1285	850	0.03%	0.004%
78	10.839	3027	3032	3035	rVB4	980	903	0.03%	0.004%
79	10.859	3035	3038	3041	rBV3	1375	1314	0.04%	0.005%
80	10.897	3047	3050	3054	rBV4	1005	881	0.03%	0.004%
81	10.916	3054	3056	3061	rVB3	1008	808	0.03%	0.003%
82	10.942	3061	3064	3068	rBV2	1355	1050	0.03%	0.004%
83	10.965	3068	3071	3076	rBV4	1104	987	0.03%	0.004%
84	11.058	3095	3100	3105	rBV5	1163	1267	0.04%	0.005%
85	11.087	3105	3109	3111	rBV	2656	2215	0.07%	0.009%
86	11.113	3115	3117	3121	rVV3	1473	1043	0.03%	0.004%
87	11.132	3121	3123	3127	rVV2	845	712	0.02%	0.003%
88	11.177	3135	3137	3142	rVB2	1371	898	0.03%	0.004%
89	11.412	3207	3210	3213	rVV2	1576	983	0.03%	0.004%
90	11.479	3219	3231	3255	rBV	986319	1595611	50.02%	6.578%
91	11.855	3336	3348	3378	rBV	951470	1610576	50.49%	6.640%
92	12.572	3568	3571	3574	rBV2	1092	811	0.03%	0.003%
93	12.830	3647	3651	3656	rVB6	1328	1517	0.05%	0.006%
94	12.936	3679	3684	3687	rVB6	1104	1068	0.03%	0.004%
95	13.341	3804	3810	3813	rBV3	1426	1714	0.05%	0.007%
96	13.656	3905	3908	3912	rBV3	1594	961	0.03%	0.004%
97	13.727	3928	3930	3938	rVB4	1589	1598	0.05%	0.007%
98	13.958	3998	4002	4003	rBV2	1562	975	0.03%	0.004%
99	14.071	4035	4037	4041	rVB3	1483	839	0.03%	0.003%
100	15.235	4397	4399	4403	rBV4	1928	1297	0.04%	0.005%


Sum of corrected areas: 24256487

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031638.D
Acq On : 30 Apr 2019 16:52
Operator : JC/SP
Sample : K2593-06DL 2500X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

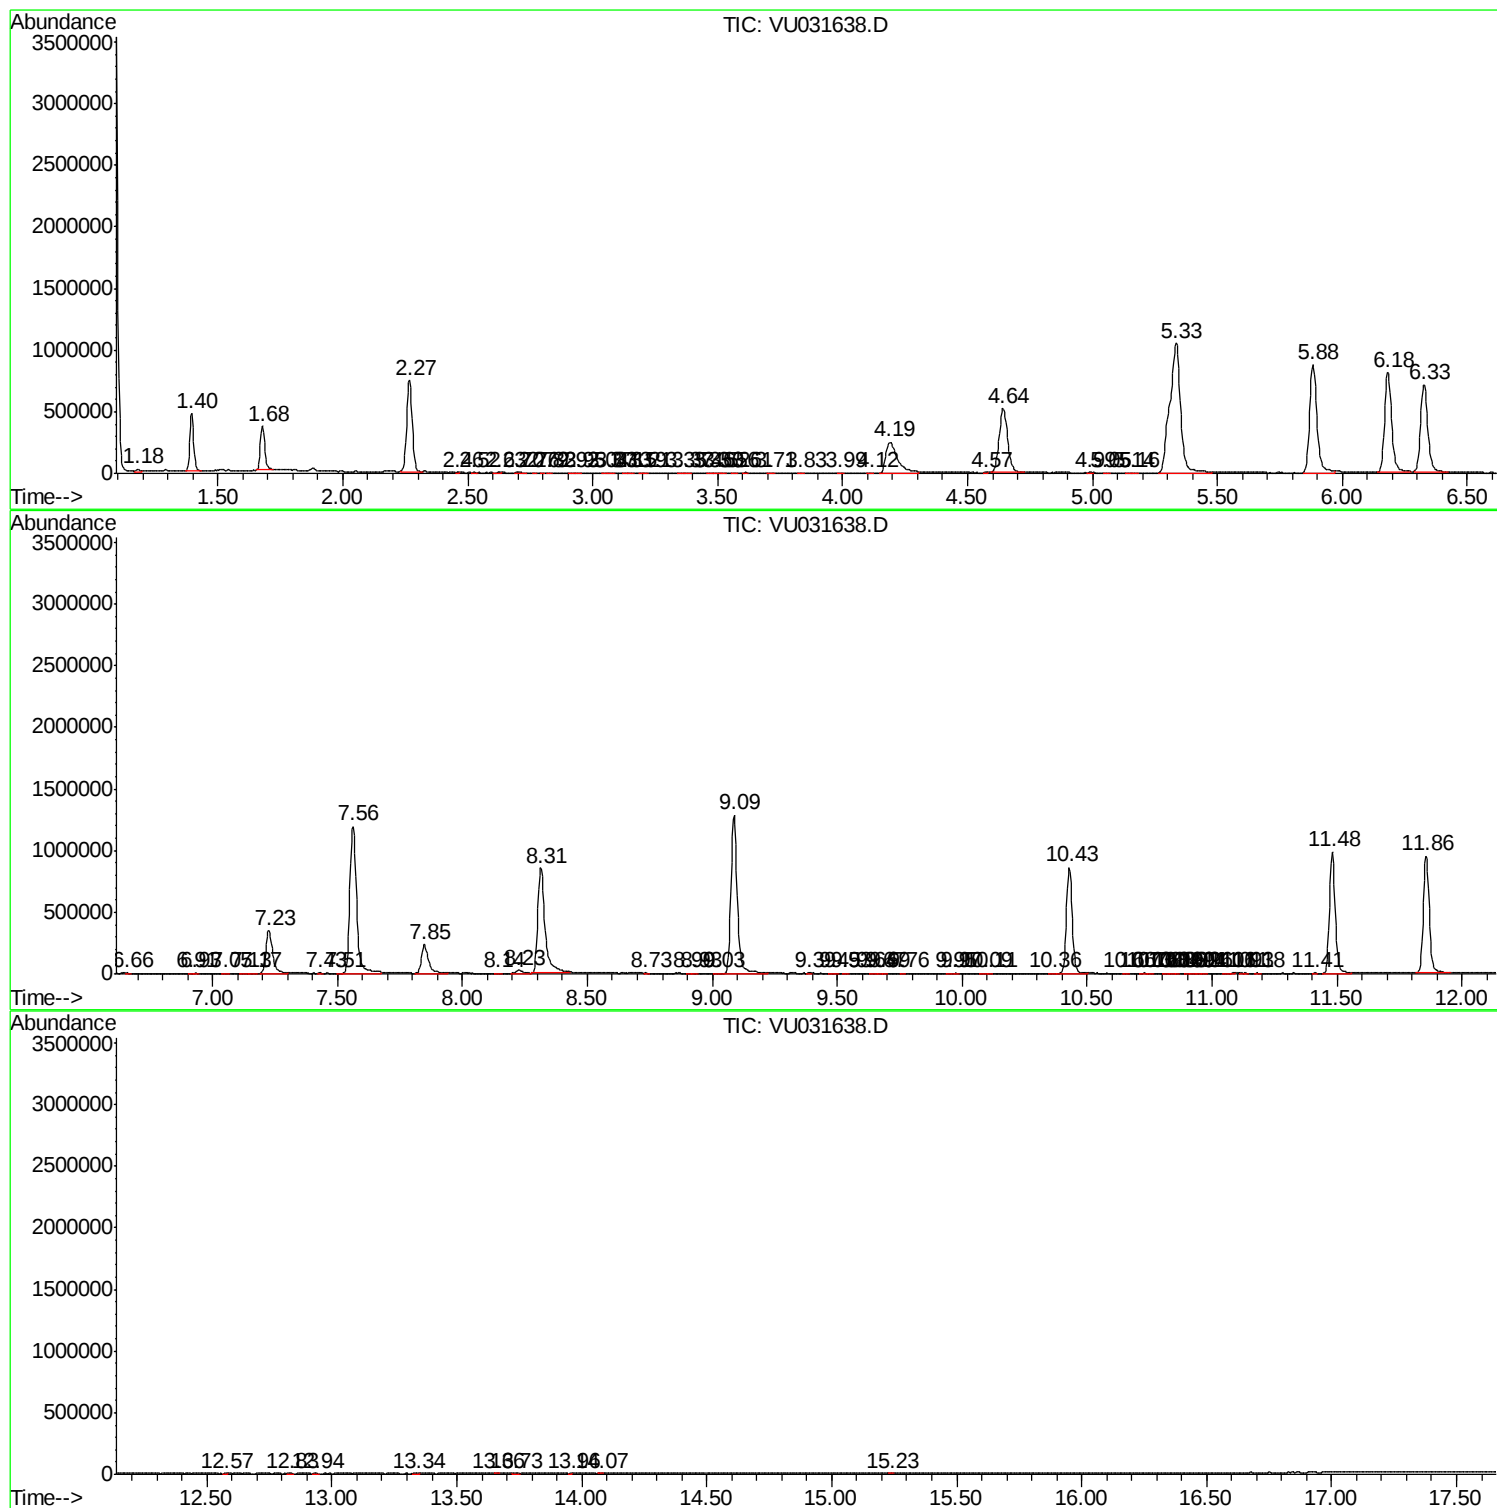

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031638.D
Acq On : 30 Apr 2019 16:52
Operator : JC/SP
Sample : K2593-06DL 2500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031638.D
Acq On : 30 Apr 2019 16:52
Operator : JC/SP
Sample : K2593-06DL 2500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc