

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031639.D
 Acq On : 30 Apr 2019 17:15
 Operator : JC/SP
 Sample : K2593-08DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB	15348	12992	0.40%	0.053%
2	1.289	59	62	67	rBV	14714	11672	0.36%	0.047%
3	1.395	87	95	109	rBV	451666	507682	15.75%	2.053%
4	1.678	175	183	194	rBV	353999	445100	13.81%	1.800%
5	2.267	355	366	380	rVB	779783	1153902	35.80%	4.665%
6	2.527	443	447	450	rBV5	1665	1293	0.04%	0.005%
7	2.630	476	479	483	rBV5	988	647	0.02%	0.003%
8	2.698	493	500	510	rVB5	4457	8288	0.26%	0.034%
9	2.743	512	514	521	rVB6	1365	1268	0.04%	0.005%
10	2.778	521	525	528	rVB2	1119	841	0.03%	0.003%
11	2.797	528	531	533	rBV3	1610	1085	0.03%	0.004%
12	2.839	542	544	551	rVB5	1235	1066	0.03%	0.004%
13	2.971	579	585	587	rBV3	1121	1208	0.04%	0.005%
14	3.061	609	613	614	rBV2	883	622	0.02%	0.003%
15	3.167	641	646	648	rBV3	1178	1039	0.03%	0.004%
16	3.209	657	659	664	rVB2	1199	997	0.03%	0.004%
17	3.235	664	667	670	rBV3	948	744	0.02%	0.003%
18	3.254	671	673	680	rVB4	1104	879	0.03%	0.004%
19	3.305	687	689	692	rBV	1077	664	0.02%	0.003%
20	3.421	719	725	728	rBV4	676	725	0.02%	0.003%
21	3.508	749	752	756	rVB3	1010	681	0.02%	0.003%
22	3.575	769	773	777	rVB2	1505	1377	0.04%	0.006%
23	3.601	777	781	782	rBV	1315	911	0.03%	0.004%
24	3.739	820	824	827	rBV3	1131	789	0.02%	0.003%
25	3.788	835	839	841	rVB2	1456	1003	0.03%	0.004%
26	3.804	841	844	849	rBV4	1468	1345	0.04%	0.005%
27	3.849	855	858	862	rVV2	1360	1154	0.04%	0.005%
28	3.871	862	865	870	rVB4	1133	729	0.02%	0.003%
29	3.916	874	879	882	rBV4	1366	1097	0.03%	0.004%
30	4.048	914	920	922	rBV	963	963	0.03%	0.004%
31	4.190	952	964	1001	rBV	246786	804727	24.97%	3.254%
32	4.643	1088	1105	1129	rBV	529307	1261253	39.14%	5.099%
33	4.858	1169	1172	1175	rBV3	1441	1039	0.03%	0.004%
34	4.874	1175	1177	1179	rBV3	1677	847	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031639.D
 Acq On : 30 Apr 2019 17:15
 Operator : JC/SP
 Sample : K2593-08DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.977	1205	1209	1211	rBV4	2255	1767	0.05%	0.007%
36	5.022	1221	1223	1225	rBV3	1450	791	0.02%	0.003%
37	5.170	1265	1269	1274	rBV3	1557	1406	0.04%	0.006%
38	5.334	1297	1320	1354	rBV2	1064025	3222793	100.00%	13.030%
39	5.730	1440	1443	1445	rBV3	1610	1162	0.04%	0.005%
40	5.881	1476	1490	1530	rBV	895660	1895410	58.81%	7.663%
41	6.183	1570	1584	1611	rBV	927137	1886789	58.55%	7.628%
42	6.328	1616	1629	1649	rVV	716655	1442881	44.77%	5.834%
43	6.665	1730	1734	1737	rBV4	1349	867	0.03%	0.004%
44	6.768	1763	1766	1770	rBV3	996	618	0.02%	0.002%
45	6.820	1780	1782	1788	rVB4	962	743	0.02%	0.003%
46	6.849	1788	1791	1794	rBV3	1125	926	0.03%	0.004%
47	6.868	1794	1797	1807	rVB5	1478	1787	0.06%	0.007%
48	6.906	1807	1809	1816	rVB4	810	927	0.03%	0.004%
49	6.945	1816	1821	1824	rBV4	1890	1697	0.05%	0.007%
50	7.038	1847	1850	1854	rVV4	1389	1022	0.03%	0.004%
51	7.164	1885	1889	1895	rBV5	1616	2148	0.07%	0.009%
52	7.225	1895	1908	1935	rBV	344537	663772	20.60%	2.684%
53	7.479	1984	1987	1996	rVB7	1813	1833	0.06%	0.007%
54	7.562	1997	2013	2043	rBV	1215060	2242277	69.58%	9.066%
55	7.849	2091	2102	2126	rBV	233225	431075	13.38%	1.743%
56	8.000	2147	2149	2152	rBV4	1507	893	0.03%	0.004%
57	8.025	2155	2157	2159	rVB2	2607	1202	0.04%	0.005%
58	8.225	2214	2219	2228	rBV9	3271	4688	0.15%	0.019%
59	8.315	2235	2247	2290	rBV	839113	1750206	54.31%	7.076%
60	8.623	2340	2343	2347	rBV3	1831	1408	0.04%	0.006%
61	8.643	2347	2349	2351	rBV3	1496	721	0.02%	0.003%
62	8.697	2362	2366	2367	rBV2	1318	901	0.03%	0.004%
63	8.768	2384	2388	2392	rBV4	1271	1144	0.04%	0.005%
64	8.839	2407	2410	2413	rBV3	1625	968	0.03%	0.004%
65	8.939	2438	2441	2445	rBV3	1761	1554	0.05%	0.006%
66	9.003	2456	2461	2464	rBV5	1396	1154	0.04%	0.005%
67	9.022	2464	2467	2469	rBV4	909	614	0.02%	0.002%
68	9.086	2474	2487	2532	rBV	1292405	2297605	71.29%	9.289%
69	9.492	2606	2613	2616	rBV3	2187	2443	0.08%	0.010%
70	9.607	2647	2649	2651	rBV2	974	631	0.02%	0.003%
71	9.656	2661	2664	2666	rBV4	1353	749	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031639.D
 Acq On : 30 Apr 2019 17:15
 Operator : JC/SP
 Sample : K2593-08DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.720	2680	2684	2687	rBV4	1828	1332	0.04%	0.005%
73	9.762	2695	2697	2701	rVB3	1175	797	0.02%	0.003%
74	9.800	2706	2709	2712	rBV3	1293	906	0.03%	0.004%
75	9.903	2738	2741	2746	rBV5	1002	993	0.03%	0.004%
76	9.996	2768	2770	2777	rVB2	947	802	0.02%	0.003%
77	10.061	2784	2790	2793	rBV5	1200	1139	0.04%	0.005%
78	10.096	2798	2801	2804	rBV3	1184	808	0.03%	0.003%
79	10.180	2822	2827	2829	rBV2	1098	788	0.02%	0.003%
80	10.209	2834	2836	2840	rVB3	1093	648	0.02%	0.003%
81	10.289	2859	2861	2864	rVB3	1501	838	0.03%	0.003%
82	10.315	2866	2869	2872	rVB2	1360	786	0.02%	0.003%
83	10.334	2872	2875	2877	rBV2	1390	846	0.03%	0.003%
84	10.350	2877	2880	2883	rVB3	962	610	0.02%	0.002%
85	10.427	2892	2904	2924	rBV	852871	1396635	43.34%	5.647%
86	10.672	2976	2980	2981	rBV2	1326	932	0.03%	0.004%
87	10.800	3017	3020	3023	rBV2	1415	1056	0.03%	0.004%
88	11.125	3117	3121	3124	rBV	1393	1410	0.04%	0.006%
89	11.173	3133	3136	3138	rBV2	1006	789	0.02%	0.003%
90	11.221	3148	3151	3154	rBV2	1314	783	0.02%	0.003%
91	11.350	3188	3191	3193	rBV2	935	634	0.02%	0.003%
92	11.482	3219	3232	3252	rBV	991878	1614062	50.08%	6.526%
93	11.858	3337	3349	3379	rBV	945820	1597397	49.57%	6.458%
94	12.556	3561	3566	3569	rBV5	1531	1690	0.05%	0.007%
95	12.935	3681	3684	3686	rBV3	1698	1136	0.04%	0.005%
96	13.009	3703	3707	3710	rBV2	1649	1536	0.05%	0.006%
97	13.270	3786	3788	3795	rVB4	2292	2026	0.06%	0.008%
98	13.337	3807	3809	3811	rBV2	1206	643	0.02%	0.003%
99	13.880	3976	3978	3983	rBV	1642	986	0.03%	0.004%
100	14.189	4071	4074	4076	rBV2	1469	890	0.03%	0.004%


Sum of corrected areas: 24734099

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031639.D
Acq On : 30 Apr 2019 17:15
Operator : JC/SP
Sample : K2593-08DL 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

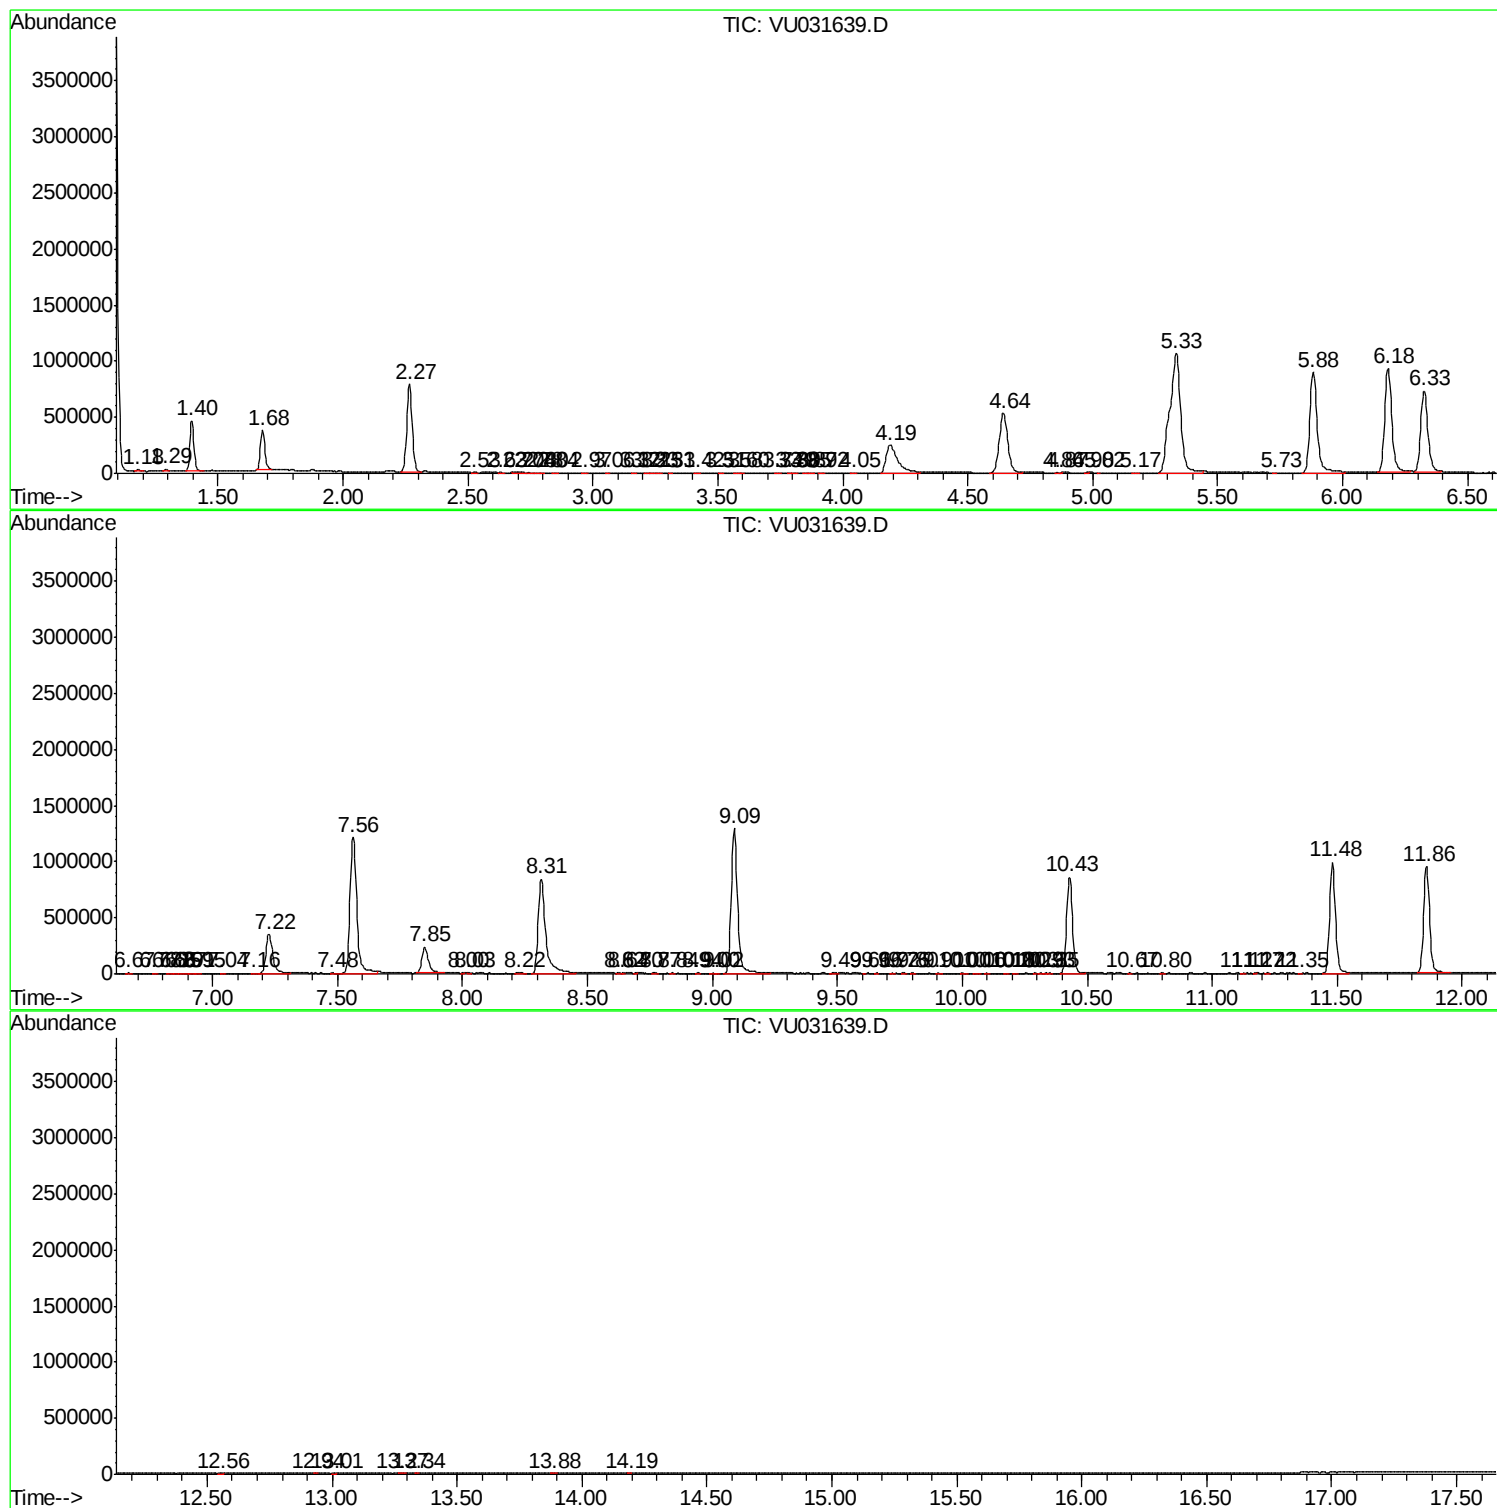

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031639.D
Acq On : 30 Apr 2019 17:15
Operator : JC/SP
Sample : K2593-08DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031639.D
Acq On : 30 Apr 2019 17:15
Operator : JC/SP
Sample : K2593-08DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc