

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031640.D
 Acq On : 30 Apr 2019 17:39
 Operator : JC/SP
 Sample : K2593-09DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X73DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	37	rVB3	16261	14163	0.37%	0.053%
2	1.290	59	62	67	rVB	14029	10710	0.28%	0.040%
3	1.396	87	95	109	rBV	449622	504570	13.17%	1.901%
4	1.675	175	182	198	rBV	348345	443749	11.58%	1.672%
5	1.875	240	244	260	rVB2	27779	37577	0.98%	0.142%
6	2.264	354	365	380	rVB	737407	1132847	29.57%	4.268%
7	2.470	422	429	434	rBV8	2705	3753	0.10%	0.014%
8	2.572	457	461	464	rVB5	1641	1068	0.03%	0.004%
9	2.701	496	501	510	rVB7	5397	7670	0.20%	0.029%
10	2.749	514	516	521	rVB4	1552	1108	0.03%	0.004%
11	2.794	521	530	534	rVB4	1852	2463	0.06%	0.009%
12	2.859	547	550	553	rVB3	1278	847	0.02%	0.003%
13	2.878	553	556	559	rBV3	1413	1133	0.03%	0.004%
14	2.939	569	575	577	rBV3	1805	1302	0.03%	0.005%
15	3.000	590	594	598	rVB3	1324	1063	0.03%	0.004%
16	3.026	598	602	607	rBV3	1562	1463	0.04%	0.006%
17	3.061	607	613	615	rVV4	1017	1058	0.03%	0.004%
18	3.170	642	647	652	rBV2	1629	1927	0.05%	0.007%
19	3.235	661	667	670	rVV4	1241	1260	0.03%	0.005%
20	3.441	725	731	737	rVB6	1268	1794	0.05%	0.007%
21	3.489	742	746	749	rBV3	1294	861	0.02%	0.003%
22	3.556	765	767	775	rVB3	1259	1557	0.04%	0.006%
23	3.598	775	780	785	rVB4	1455	1521	0.04%	0.006%
24	3.643	789	794	796	rBV3	1016	947	0.02%	0.004%
25	3.868	857	864	869	rBV4	736	1147	0.03%	0.004%
26	3.955	887	891	894	rBV2	1135	992	0.03%	0.004%
27	4.071	922	927	934	rVB5	1113	1519	0.04%	0.006%
28	4.186	950	963	1000	rBV	254774	814386	21.26%	3.068%
29	4.640	1085	1104	1130	rBV	521048	1259328	32.88%	4.744%
30	4.859	1167	1172	1173	rBV4	1273	867	0.02%	0.003%
31	4.881	1175	1179	1180	rBV3	1986	1264	0.03%	0.005%
32	4.971	1204	1207	1210	rBV4	1786	1648	0.04%	0.006%
33	5.132	1254	1257	1265	rVB8	1368	1222	0.03%	0.005%
34	5.180	1269	1272	1277	rBV4	1188	1297	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031640.D
 Acq On : 30 Apr 2019 17:39
 Operator : JC/SP
 Sample : K2593-09DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X73DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.212	1279	1282	1286	rVB2	1583	1163	0.03%	0.004%
36	5.241	1289	1291	1295	rBV3	942	833	0.02%	0.003%
37	5.334	1297	1320	1352	rBV2	1050576	3177297	82.95%	11.970%
38	5.881	1476	1490	1524	rBV	888394	1854381	48.41%	6.986%
39	6.180	1568	1583	1615	rVV	1900441	3830589	100.00%	14.432%
40	6.325	1616	1628	1659	rVB	721188	1501645	39.20%	5.657%
41	6.559	1699	1701	1707	rVB7	1657	1472	0.04%	0.006%
42	6.588	1707	1710	1714	rBV4	1620	1202	0.03%	0.005%
43	6.685	1738	1740	1745	rVB5	1826	1523	0.04%	0.006%
44	6.759	1761	1763	1772	rVB3	1325	1308	0.03%	0.005%
45	6.881	1797	1801	1803	rBV4	1318	860	0.02%	0.003%
46	6.974	1828	1830	1839	rVB5	1339	1728	0.05%	0.007%
47	7.151	1882	1885	1888	rVB2	1410	850	0.02%	0.003%
48	7.225	1896	1908	1932	rBV	347116	660624	17.25%	2.489%
49	7.421	1967	1969	1977	rVB6	1239	1012	0.03%	0.004%
50	7.563	2000	2013	2032	rBV	1208648	2184843	57.04%	8.231%
51	7.849	2091	2102	2131	rBV	230969	438470	11.45%	1.652%
52	8.161	2196	2199	2203	rBV4	1274	1144	0.03%	0.004%
53	8.225	2212	2219	2231	rVB8	12162	20091	0.52%	0.076%
54	8.315	2236	2247	2286	rBV	841203	1746652	45.60%	6.580%
55	8.598	2334	2335	2339	rVB4	1781	848	0.02%	0.003%
56	8.624	2340	2343	2345	rVB4	1487	844	0.02%	0.003%
57	8.640	2345	2348	2352	rBV5	1112	853	0.02%	0.003%
58	8.707	2365	2369	2372	rVV6	1689	1325	0.03%	0.005%
59	9.087	2472	2487	2528	rBV	1282190	2253383	58.83%	8.490%
60	9.376	2573	2577	2578	rBV2	1974	1216	0.03%	0.005%
61	9.530	2621	2625	2628	rBV3	907	1018	0.03%	0.004%
62	9.553	2628	2632	2633	rBV3	1221	948	0.02%	0.004%
63	9.591	2640	2644	2649	rBV5	1627	1320	0.03%	0.005%
64	9.614	2649	2651	2656	rBV5	1368	1287	0.03%	0.005%
65	9.755	2689	2695	2697	rBV4	1298	1133	0.03%	0.004%
66	9.778	2697	2702	2704	rBV3	1094	1086	0.03%	0.004%
67	9.855	2721	2726	2728	rBV3	1174	1040	0.03%	0.004%
68	9.955	2752	2757	2764	rVB4	1395	1930	0.05%	0.007%
69	10.029	2777	2780	2783	rVB2	2334	1494	0.04%	0.006%
70	10.067	2788	2792	2794	rBV2	1509	1201	0.03%	0.005%
71	10.125	2807	2810	2816	rBV3	1255	1306	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031640.D
 Acq On : 30 Apr 2019 17:39
 Operator : JC/SP
 Sample : K2593-09DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X73DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.247	2846	2848	2854	rVB2	1686	1233	0.03%	0.005%
73	10.286	2857	2860	2865	rBV4	1567	991	0.03%	0.004%
74	10.328	2870	2873	2877	rVB3	1292	894	0.02%	0.003%
75	10.370	2884	2886	2892	rVB4	997	1030	0.03%	0.004%
76	10.427	2892	2904	2928	rBV	857990	1397586	36.48%	5.265%
77	10.588	2951	2954	2957	rBV3	1829	1275	0.03%	0.005%
78	10.762	3005	3008	3012	rVB4	1878	1324	0.03%	0.005%
79	10.784	3012	3015	3020	rBV3	1522	1566	0.04%	0.006%
80	10.923	3056	3058	3063	rVB2	1557	1075	0.03%	0.004%
81	11.064	3098	3102	3105	rBV2	2260	1613	0.04%	0.006%
82	11.151	3125	3129	3132	rVB3	1382	1137	0.03%	0.004%
83	11.482	3220	3232	3256	rBV	956054	1574854	41.11%	5.933%
84	11.858	3337	3349	3369	rBV	970894	1577264	41.18%	5.942%
85	12.363	3503	3506	3508	rBV2	1580	1168	0.03%	0.004%
86	12.617	3582	3585	3589	rVB2	3159	2229	0.06%	0.008%
87	12.640	3589	3592	3595	rBV3	1764	1464	0.04%	0.006%
88	12.749	3623	3626	3630	rBV2	1077	855	0.02%	0.003%
89	12.868	3659	3663	3666	rBV2	2019	1936	0.05%	0.007%
90	12.958	3688	3691	3694	rBV2	1860	1325	0.03%	0.005%
91	12.980	3695	3698	3701	rBV3	1634	1316	0.03%	0.005%
92	13.148	3748	3750	3755	rBV2	1205	1089	0.03%	0.004%
93	13.292	3793	3795	3799	rVB2	1179	900	0.02%	0.003%
94	13.318	3800	3803	3808	rBV5	1714	1627	0.04%	0.006%
95	13.929	3990	3993	3996	rBV2	1268	862	0.02%	0.003%
96	14.054	4028	4032	4034	rBV2	1603	1318	0.03%	0.005%
97	14.221	4081	4084	4087	rBV3	1622	1016	0.03%	0.004%
98	14.492	4165	4168	4171	rVB2	2758	1707	0.04%	0.006%
99	14.820	4268	4270	4274	rBV3	1338	1103	0.03%	0.004%
100	14.868	4282	4285	4287	rBV2	1923	1364	0.04%	0.005%


Sum of corrected areas: 26543121

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031640.D
Acq On : 30 Apr 2019 17:39
Operator : JC/SP
Sample : K2593-09DL 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X73DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

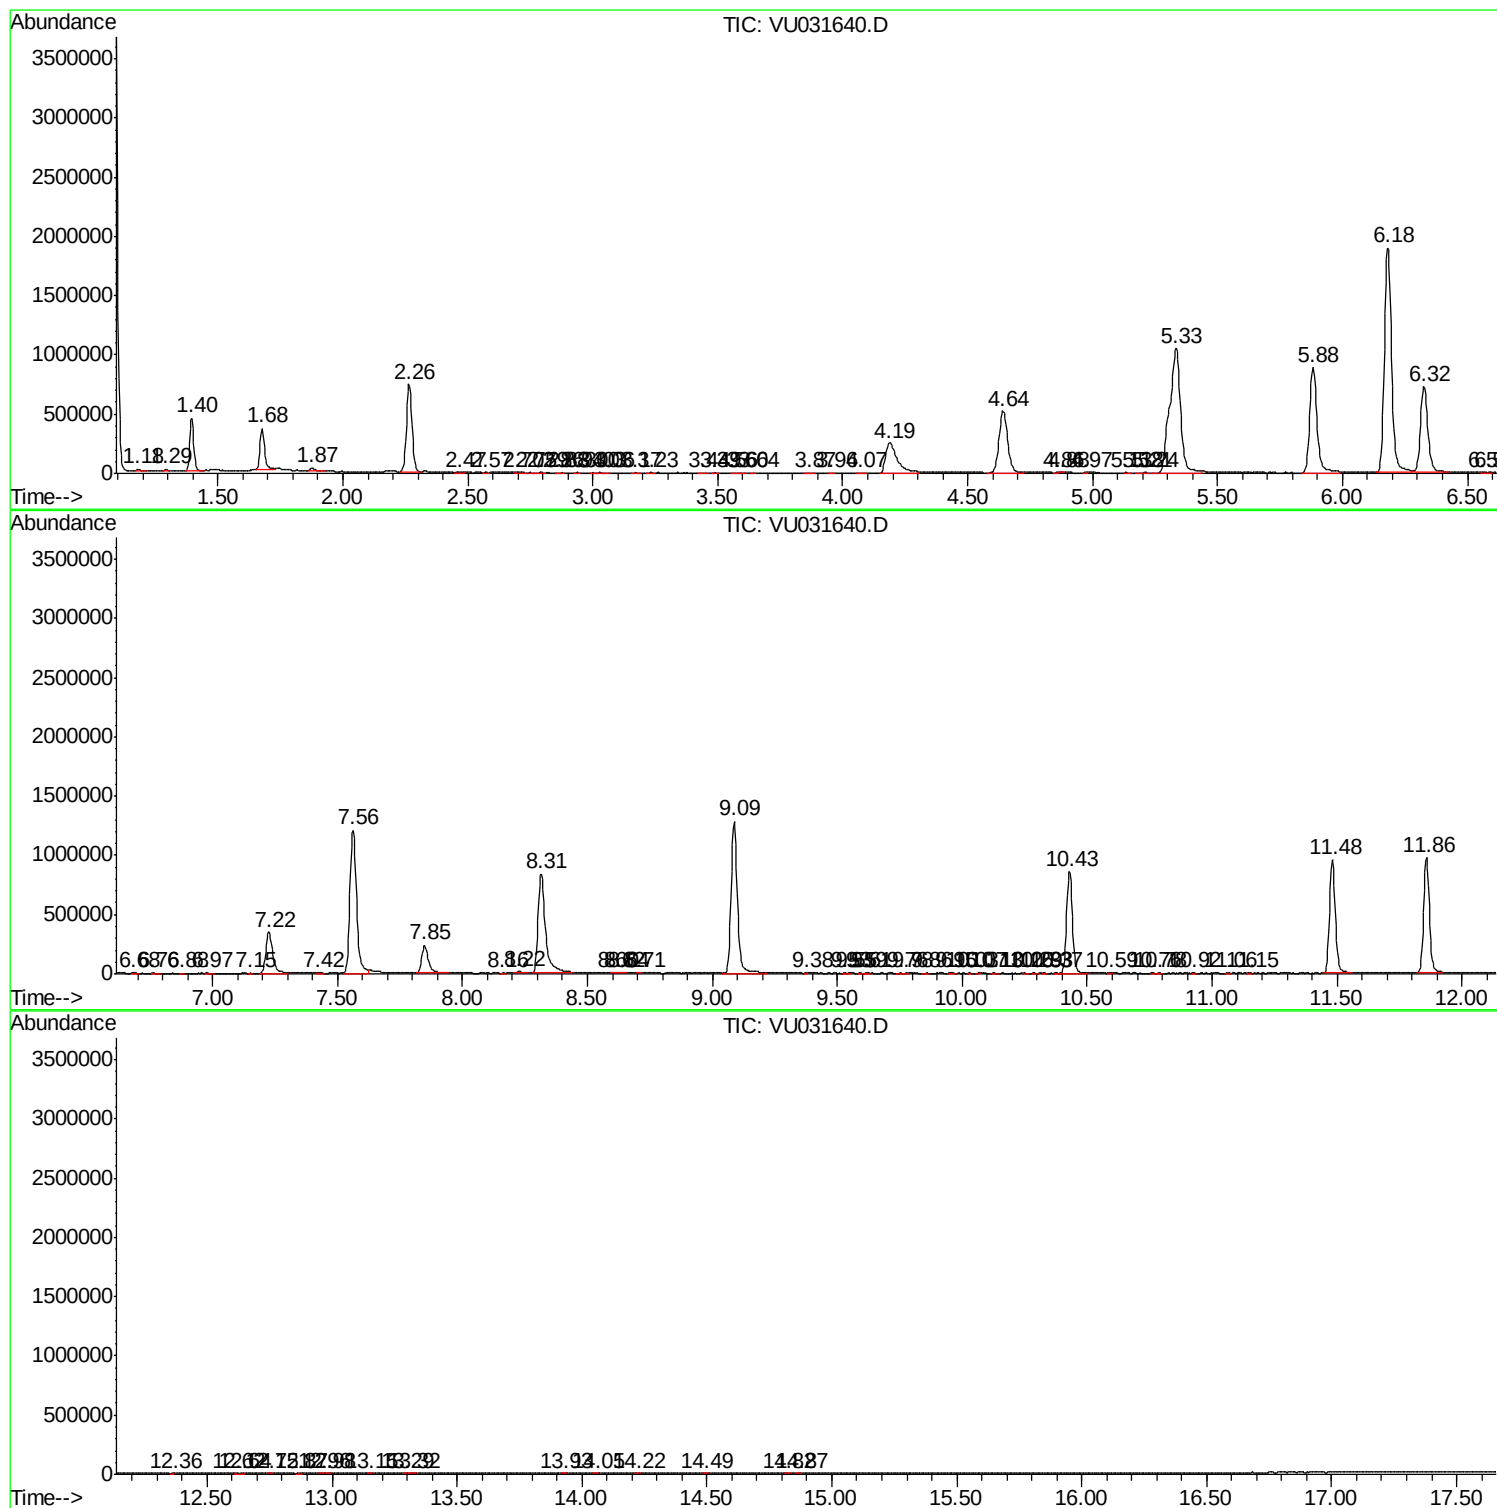

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031640.D
Acq On : 30 Apr 2019 17:39
Operator : JC/SP
Sample : K2593-09DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X73DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031640.D
Acq On : 30 Apr 2019 17:39
Operator : JC/SP
Sample : K2593-09DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X73DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc