

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031641.D
 Acq On : 30 Apr 2019 18:02
 Operator : JC/SP
 Sample : K2593-10DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X74DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	37	rVB2	16008	14538	0.38%	0.056%
2	1.289	58	62	67	rBV	20085	19271	0.51%	0.074%
3	1.395	88	95	109	rBV	437435	476538	12.50%	1.830%
4	1.675	175	182	199	rBV	339045	427582	11.22%	1.642%
5	2.267	355	366	381	rVB	743872	1122362	29.44%	4.310%
6	2.440	417	420	423	rVB3	2169	1269	0.03%	0.005%
7	2.460	423	426	427	rBV3	1246	794	0.02%	0.003%
8	2.495	435	437	440	rVB2	1540	758	0.02%	0.003%
9	2.527	445	447	451	rVB3	1232	709	0.02%	0.003%
10	2.582	461	464	465	rBV2	1337	749	0.02%	0.003%
11	2.694	495	499	506	rVB4	4332	4791	0.13%	0.018%
12	2.852	542	548	549	rBV2	1317	1258	0.03%	0.005%
13	2.920	566	569	572	rBV2	1052	829	0.02%	0.003%
14	2.993	590	592	600	rVB3	1946	1795	0.05%	0.007%
15	3.038	600	606	615	rBV5	1772	1986	0.05%	0.008%
16	3.334	694	698	701	rVV	941	781	0.02%	0.003%
17	3.543	760	763	768	rBV3	1117	830	0.02%	0.003%
18	3.743	820	825	829	rBV2	1547	1787	0.05%	0.007%
19	3.791	837	840	846	rBV4	1280	1287	0.03%	0.005%
20	3.948	884	889	893	rVB4	763	720	0.02%	0.003%
21	4.006	899	907	910	rBV3	1544	1753	0.05%	0.007%
22	4.048	917	920	922	rVB2	1146	691	0.02%	0.003%
23	4.064	922	925	928	rBV2	1171	914	0.02%	0.004%
24	4.103	934	937	940	rBV2	1158	673	0.02%	0.003%
25	4.128	940	945	948	rBV2	1464	1361	0.04%	0.005%
26	4.186	951	963	1006	rBV	251375	799274	20.97%	3.069%
27	4.440	1040	1042	1043	rBV	1459	656	0.02%	0.003%
28	4.518	1063	1066	1069	rBV4	1250	1036	0.03%	0.004%
29	4.559	1076	1079	1082	rBV3	1089	806	0.02%	0.003%
30	4.643	1086	1105	1132	rBV	507895	1223201	32.09%	4.697%
31	4.942	1194	1198	1200	rBV4	1735	1595	0.04%	0.006%
32	5.035	1222	1227	1229	rBV2	1378	1114	0.03%	0.004%
33	5.241	1288	1291	1294	rVB3	963	664	0.02%	0.003%
34	5.334	1294	1320	1361	rBV2	1029381	3135692	82.25%	12.040%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031641.D
 Acq On : 30 Apr 2019 18:02
 Operator : JC/SP
 Sample : K2593-10DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X74DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.636	1411	1414	1417	rVB2	1978	1200	0.03%	0.005%
36	5.710	1434	1437	1439	rBV2	1146	784	0.02%	0.003%
37	5.749	1447	1449	1458	rVB7	2039	2698	0.07%	0.010%
38	5.881	1474	1490	1521	rBV	849791	1781547	46.73%	6.841%
39	6.180	1569	1583	1616	rBV	1906059	3812355	100.00%	14.639%
40	6.325	1616	1628	1662	rVB	713049	1485042	38.95%	5.702%
41	6.723	1750	1752	1758	rBV4	747	775	0.02%	0.003%
42	6.765	1761	1765	1768	rVV3	1382	1195	0.03%	0.005%
43	6.781	1768	1770	1777	rVB5	1343	1148	0.03%	0.004%
44	6.858	1791	1794	1797	rBV5	1203	994	0.03%	0.004%
45	6.958	1819	1825	1828	rBV4	1289	1498	0.04%	0.006%
46	7.096	1866	1868	1870	rBV2	1445	710	0.02%	0.003%
47	7.109	1870	1872	1875	rVB2	1680	872	0.02%	0.003%
48	7.225	1896	1908	1937	rBV	336980	650608	17.07%	2.498%
49	7.476	1984	1986	1992	rVB4	1412	936	0.02%	0.004%
50	7.562	2000	2013	2050	rBV	1191134	2198090	57.66%	8.440%
51	7.849	2091	2102	2127	rBV	229671	426699	11.19%	1.638%
52	8.038	2159	2161	2168	rVB4	1325	1071	0.03%	0.004%
53	8.228	2210	2220	2235	rBV7	13337	24973	0.66%	0.096%
54	8.315	2235	2247	2295	rBV	826951	1703282	44.68%	6.540%
55	8.675	2354	2359	2362	rBV4	1615	1649	0.04%	0.006%
56	9.025	2466	2468	2471	rVB2	1478	704	0.02%	0.003%
57	9.086	2471	2487	2519	rBV	1257502	2198213	57.66%	8.441%
58	9.408	2583	2587	2592	rBV5	1264	1191	0.03%	0.005%
59	9.459	2601	2603	2605	rBV3	1211	752	0.02%	0.003%
60	9.585	2639	2642	2646	rBV3	1550	1227	0.03%	0.005%
61	9.620	2650	2653	2657	rBV3	870	656	0.02%	0.003%
62	9.659	2663	2665	2668	rVB2	1433	728	0.02%	0.003%
63	9.685	2668	2673	2674	rBV4	1433	1306	0.03%	0.005%
64	9.775	2699	2701	2704	rBV3	1316	832	0.02%	0.003%
65	9.935	2748	2751	2754	rBV3	938	815	0.02%	0.003%
66	10.022	2775	2778	2781	rBV2	1000	814	0.02%	0.003%
67	10.061	2787	2790	2793	rBV2	2322	1611	0.04%	0.006%
68	10.193	2828	2831	2833	rBV2	1380	727	0.02%	0.003%
69	10.241	2844	2846	2852	rVB4	1411	1260	0.03%	0.005%
70	10.270	2852	2855	2861	rVB3	1331	1362	0.04%	0.005%
71	10.312	2866	2868	2871	rBV2	1274	840	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031641.D
 Acq On : 30 Apr 2019 18:02
 Operator : JC/SP
 Sample : K2593-10DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X74DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.427	2891	2904	2923	rBV	825150	1358322	35.63%	5.216%
73	10.601	2955	2958	2961	rVB2	1578	1029	0.03%	0.004%
74	10.623	2961	2965	2966	rBV	1530	984	0.03%	0.004%
75	10.691	2979	2986	2994	rBV4	1927	3178	0.08%	0.012%
76	10.742	2999	3002	3007	rVV3	927	707	0.02%	0.003%
77	10.800	3017	3020	3024	rBV5	1111	1051	0.03%	0.004%
78	10.913	3046	3055	3059	rBV4	1156	1836	0.05%	0.007%
79	11.048	3091	3097	3100	rBV4	750	960	0.03%	0.004%
80	11.080	3103	3107	3110	rVV3	1231	1226	0.03%	0.005%
81	11.122	3117	3120	3124	rVB3	1725	1274	0.03%	0.005%
82	11.283	3167	3170	3172	rBV2	867	652	0.02%	0.003%
83	11.414	3204	3211	3212	rBV3	2140	2214	0.06%	0.009%
84	11.482	3220	3232	3255	rBV	936497	1521500	39.91%	5.842%
85	11.858	3334	3349	3374	rBV	940020	1566049	41.08%	6.013%
86	12.176	3445	3448	3452	rBV5	2523	2318	0.06%	0.009%
87	12.225	3461	3463	3467	rBV5	1341	953	0.02%	0.004%
88	12.363	3503	3506	3510	rBV4	1487	1382	0.04%	0.005%
89	12.463	3533	3537	3539	rBV	1640	1264	0.03%	0.005%
90	12.527	3554	3557	3559	rBV4	1089	803	0.02%	0.003%
91	12.646	3592	3594	3598	rBV2	1264	897	0.02%	0.003%
92	12.784	3634	3637	3643	rBV3	1127	1479	0.04%	0.006%
93	12.906	3671	3675	3681	rBV3	1930	2367	0.06%	0.009%
94	13.028	3710	3713	3716	rBV2	1938	1551	0.04%	0.006%
95	13.070	3723	3726	3730	rBV2	2194	1970	0.05%	0.008%
96	13.241	3776	3779	3782	rBV3	1125	761	0.02%	0.003%
97	13.514	3861	3864	3867	rBV2	1731	995	0.03%	0.004%
98	13.861	3967	3972	3976	rBV	1989	2299	0.06%	0.009%
99	14.250	4091	4093	4095	rBV2	1467	700	0.02%	0.003%
100	14.376	4129	4132	4134	rBV2	1456	963	0.03%	0.004%


Sum of corrected areas: 26042912

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031641.D
Acq On : 30 Apr 2019 18:02
Operator : JC/SP
Sample : K2593-10DL 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X74DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

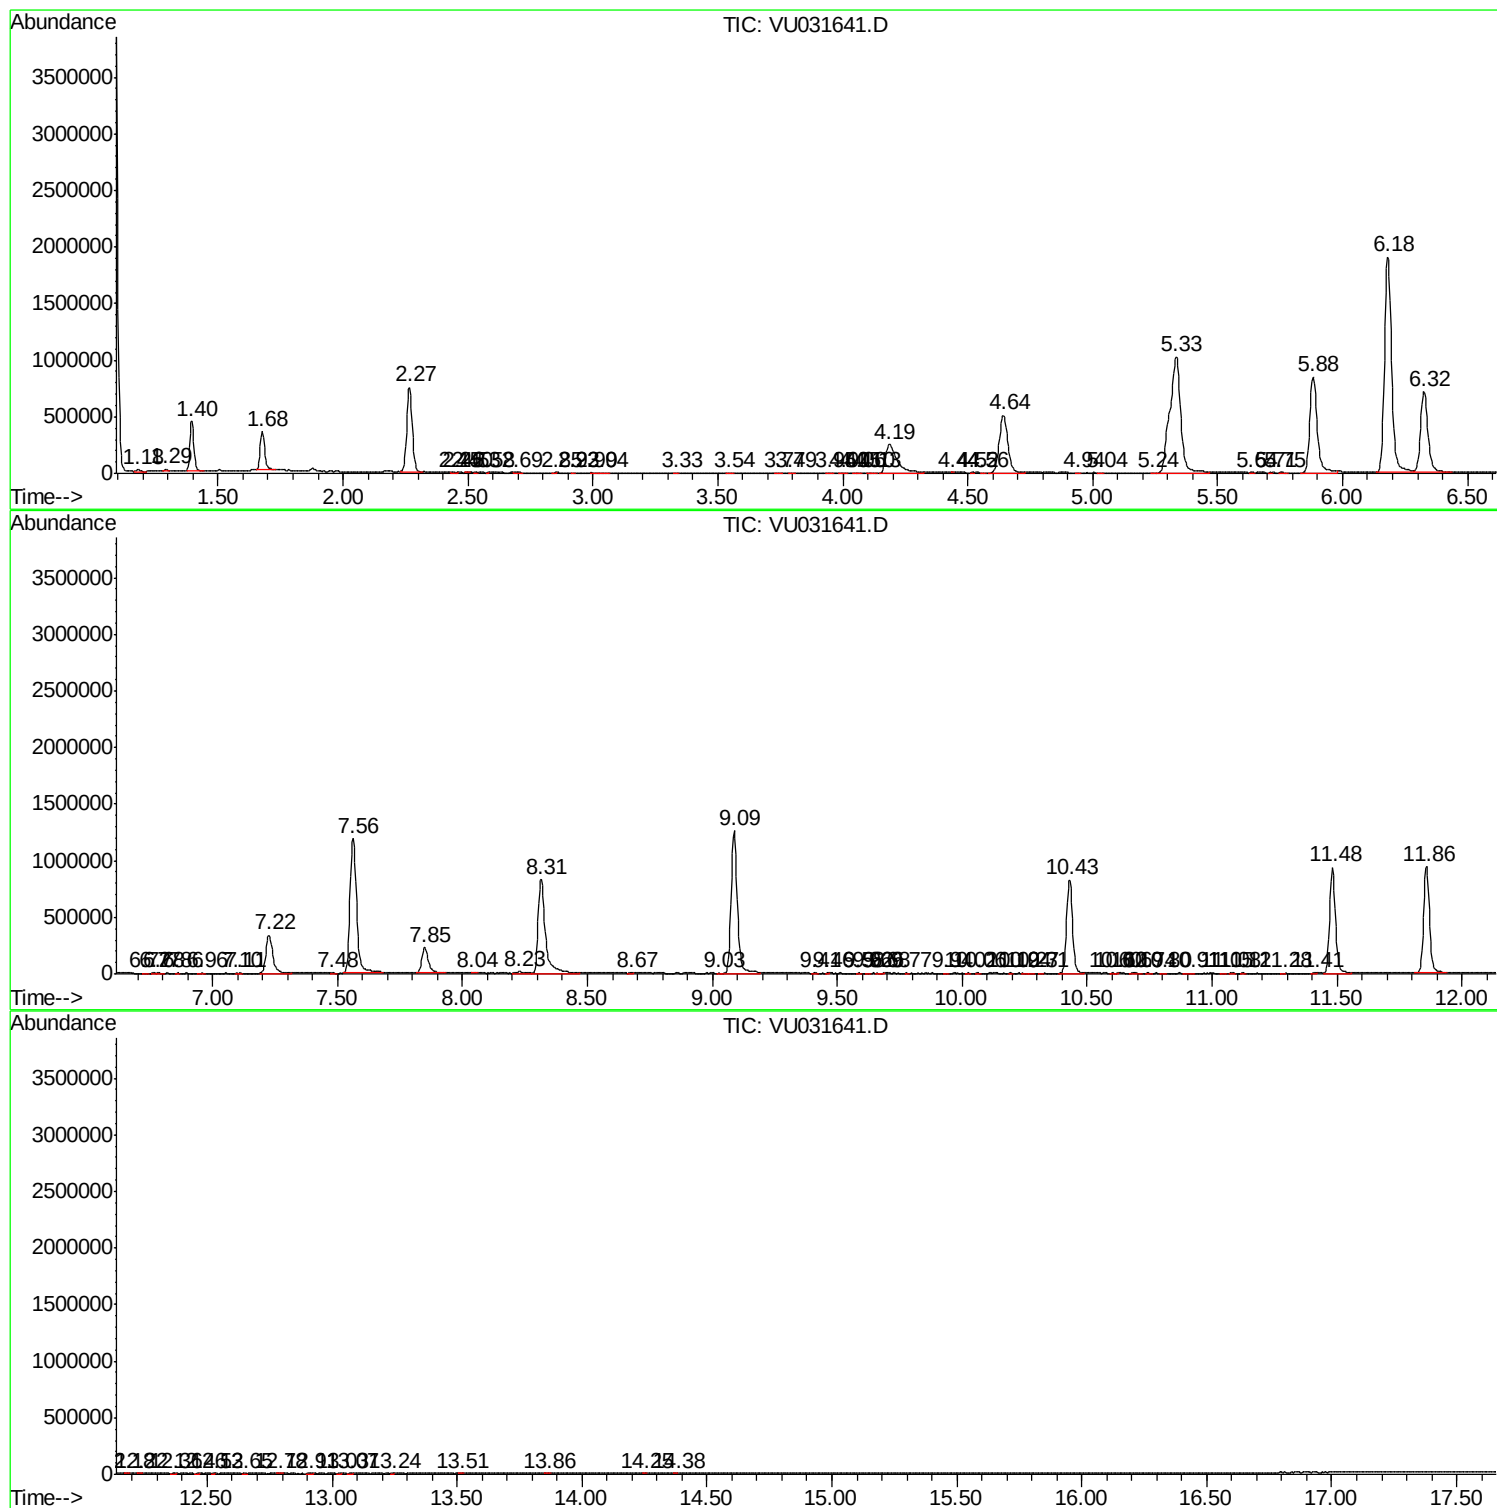

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031641.D
Acq On : 30 Apr 2019 18:02
Operator : JC/SP
Sample : K2593-10DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X74DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031641.D
Acq On : 30 Apr 2019 18:02
Operator : JC/SP
Sample : K2593-10DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X74DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc