

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031642.D
 Acq On : 30 Apr 2019 18:26
 Operator : JC/SP
 Sample : K2593-11DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X75DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rVB	13258	11150	0.31%	0.043%
2	1.289	59	62	68	rVB2	15398	12889	0.35%	0.050%
3	1.396	88	95	107	rBV	454658	488554	13.40%	1.889%
4	1.675	175	182	197	rVB	351224	416796	11.43%	1.612%
5	2.267	355	366	381	rVB	730374	1105105	30.31%	4.274%
6	2.431	414	417	421	rBV4	1631	1326	0.04%	0.005%
7	2.508	438	441	443	rBV2	1189	918	0.03%	0.004%
8	2.688	494	497	499	rBV4	2914	1917	0.05%	0.007%
9	2.801	526	532	536	rBV4	1417	1642	0.05%	0.006%
10	2.823	536	539	544	rBV6	1405	1321	0.04%	0.005%
11	3.032	601	604	610	rVB4	1360	1393	0.04%	0.005%
12	3.061	610	613	615	rBV3	1448	1062	0.03%	0.004%
13	3.190	649	653	655	rBV3	1674	1068	0.03%	0.004%
14	3.254	667	673	675	rBV2	1375	1175	0.03%	0.005%
15	3.376	708	711	716	rBV5	1351	1076	0.03%	0.004%
16	3.408	716	721	724	rVV5	1294	1186	0.03%	0.005%
17	3.502	747	750	755	rVB3	1244	1078	0.03%	0.004%
18	3.756	827	829	834	rBV2	883	848	0.02%	0.003%
19	3.829	846	852	855	rBV3	947	1056	0.03%	0.004%
20	3.858	858	861	864	rVV	1541	1199	0.03%	0.005%
21	3.881	864	868	873	rVV2	1447	1749	0.05%	0.007%
22	3.990	898	902	908	rVB5	926	1002	0.03%	0.004%
23	4.019	908	911	917	rVB4	1147	892	0.02%	0.003%
24	4.096	929	935	937	rBV4	1172	1187	0.03%	0.005%
25	4.186	951	963	1001	rBV2	254574	790553	21.68%	3.057%
26	4.640	1086	1104	1129	rBV	506429	1223914	33.57%	4.733%
27	4.846	1165	1168	1171	rBV4	1150	977	0.03%	0.004%
28	4.884	1175	1180	1183	rVV6	1865	1938	0.05%	0.007%
29	5.109	1246	1250	1254	rVB3	1535	1234	0.03%	0.005%
30	5.151	1260	1263	1271	rVV4	1030	1106	0.03%	0.004%
31	5.199	1276	1278	1282	rVB4	1238	851	0.02%	0.003%
32	5.334	1297	1320	1353	rBV2	1045929	3144218	86.25%	12.159%
33	5.743	1445	1447	1450	rVB3	1505	868	0.02%	0.003%
34	5.765	1450	1454	1457	rBV5	1514	1170	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031642.D
 Acq On : 30 Apr 2019 18:26
 Operator : JC/SP
 Sample : K2593-11DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X75DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.881	1476	1490	1525	rBV	878711	1818693	49.89%	7.033%
36	6.180	1568	1583	1615	rBV	1819236	3645655	100.00%	14.098%
37	6.325	1616	1628	1659	rVB	714010	1474377	40.44%	5.702%
38	6.543	1689	1696	1697	rBV7	1514	1625	0.04%	0.006%
39	6.595	1708	1712	1714	rBV5	868	865	0.02%	0.003%
40	6.659	1727	1732	1733	rBV3	1175	870	0.02%	0.003%
41	6.749	1757	1760	1764	rVB3	2027	1234	0.03%	0.005%
42	6.797	1772	1775	1777	rBV	1680	1031	0.03%	0.004%
43	6.813	1777	1780	1789	rVB8	1940	2478	0.07%	0.010%
44	6.858	1789	1794	1797	rBV4	1571	1691	0.05%	0.007%
45	7.016	1839	1843	1847	rVB4	1581	1463	0.04%	0.006%
46	7.045	1847	1852	1855	rBV5	1534	1451	0.04%	0.006%
47	7.167	1887	1890	1893	rVB2	1588	1040	0.03%	0.004%
48	7.225	1893	1908	1940	rBV	342382	656040	18.00%	2.537%
49	7.376	1951	1955	1958	rVB3	2059	1740	0.05%	0.007%
50	7.398	1958	1962	1964	rBV2	1481	1086	0.03%	0.004%
51	7.460	1979	1981	1984	rBV2	1572	959	0.03%	0.004%
52	7.562	2000	2013	2037	rBV	1181598	2165990	59.41%	8.376%
53	7.849	2091	2102	2127	rBV	227146	427740	11.73%	1.654%
54	8.064	2166	2169	2174	rBV5	1330	1330	0.04%	0.005%
55	8.228	2208	2220	2233	rBV7	12090	23859	0.65%	0.092%
56	8.315	2233	2247	2283	rBV2	810676	1693525	46.45%	6.549%
57	8.572	2324	2327	2330	rVB4	1558	829	0.02%	0.003%
58	8.707	2367	2369	2373	rBV2	1720	932	0.03%	0.004%
59	8.855	2411	2415	2420	rBV5	1621	1873	0.05%	0.007%
60	9.087	2474	2487	2506	rBV	1269492	2169967	59.52%	8.391%
61	9.328	2558	2562	2564	rBV2	2381	1911	0.05%	0.007%
62	9.453	2597	2601	2603	rBV4	1172	1092	0.03%	0.004%
63	9.530	2619	2625	2628	rBV6	1445	1241	0.03%	0.005%
64	9.598	2643	2646	2649	rBV5	1395	1099	0.03%	0.004%
65	9.646	2656	2661	2665	rBV4	2054	2091	0.06%	0.008%
66	9.730	2683	2687	2690	rBV2	1535	1202	0.03%	0.005%
67	9.807	2708	2711	2714	rVB3	1803	1245	0.03%	0.005%
68	9.868	2726	2730	2733	rVB3	1663	1225	0.03%	0.005%
69	10.029	2777	2780	2782	rBV2	1161	865	0.02%	0.003%
70	10.067	2789	2792	2795	rBV2	1459	850	0.02%	0.003%
71	10.122	2806	2809	2812	rVB3	1978	1320	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031642.D
 Acq On : 30 Apr 2019 18:26
 Operator : JC/SP
 Sample : K2593-11DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X75DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.238	2841	2845	2850	rVB6	1104	1024	0.03%	0.004%
73	10.321	2868	2871	2875	rVB3	1381	991	0.03%	0.004%
74	10.427	2891	2904	2929	rBV	837705	1378522	37.81%	5.331%
75	10.524	2929	2934	2943	rVB8	1693	2393	0.07%	0.009%
76	10.566	2943	2947	2951	rVB3	1859	1675	0.05%	0.006%
77	10.694	2984	2987	2993	rVB5	1776	1362	0.04%	0.005%
78	10.781	3010	3014	3015	rBV3	1406	908	0.02%	0.004%
79	10.855	3032	3037	3040	rBV4	1096	1003	0.03%	0.004%
80	10.877	3040	3044	3049	rBV3	1564	1302	0.04%	0.005%
81	10.939	3059	3063	3066	rBV3	1307	1223	0.03%	0.005%
82	11.067	3098	3103	3105	rBV3	1153	922	0.03%	0.004%
83	11.138	3120	3125	3128	rBV4	1545	1298	0.04%	0.005%
84	11.205	3143	3146	3149	rVB3	1405	854	0.02%	0.003%
85	11.228	3150	3153	3157	rVB2	1738	1038	0.03%	0.004%
86	11.482	3217	3232	3252	rBV	953053	1554763	42.65%	6.012%
87	11.858	3336	3349	3366	rBV	926363	1554566	42.64%	6.012%
88	12.347	3499	3501	3506	rVB3	1557	1305	0.04%	0.005%
89	12.402	3516	3518	3524	rBV5	1558	1126	0.03%	0.004%
90	12.620	3582	3586	3591	rBV2	1819	1984	0.05%	0.008%
91	12.784	3634	3637	3642	rVB4	2586	2114	0.06%	0.008%
92	12.813	3642	3646	3649	rBV4	1784	2036	0.06%	0.008%
93	13.073	3724	3727	3729	rBV2	1541	970	0.03%	0.004%
94	13.260	3782	3785	3789	rBV4	1328	975	0.03%	0.004%
95	13.305	3795	3799	3805	rVB3	1912	1911	0.05%	0.007%
96	13.350	3809	3813	3818	rBV4	1542	1655	0.05%	0.006%
97	13.668	3909	3912	3914	rBV2	1299	985	0.03%	0.004%
98	14.327	4114	4117	4119	rBV3	1505	1115	0.03%	0.004%
99	14.781	4255	4258	4263	rBV5	1784	1616	0.04%	0.006%
100	15.118	4361	4363	4365	rBV4	1615	915	0.03%	0.004%


Sum of corrected areas: 25859453

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031642.D
Acq On : 30 Apr 2019 18:26
Operator : JC/SP
Sample : K2593-11DL 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X75DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

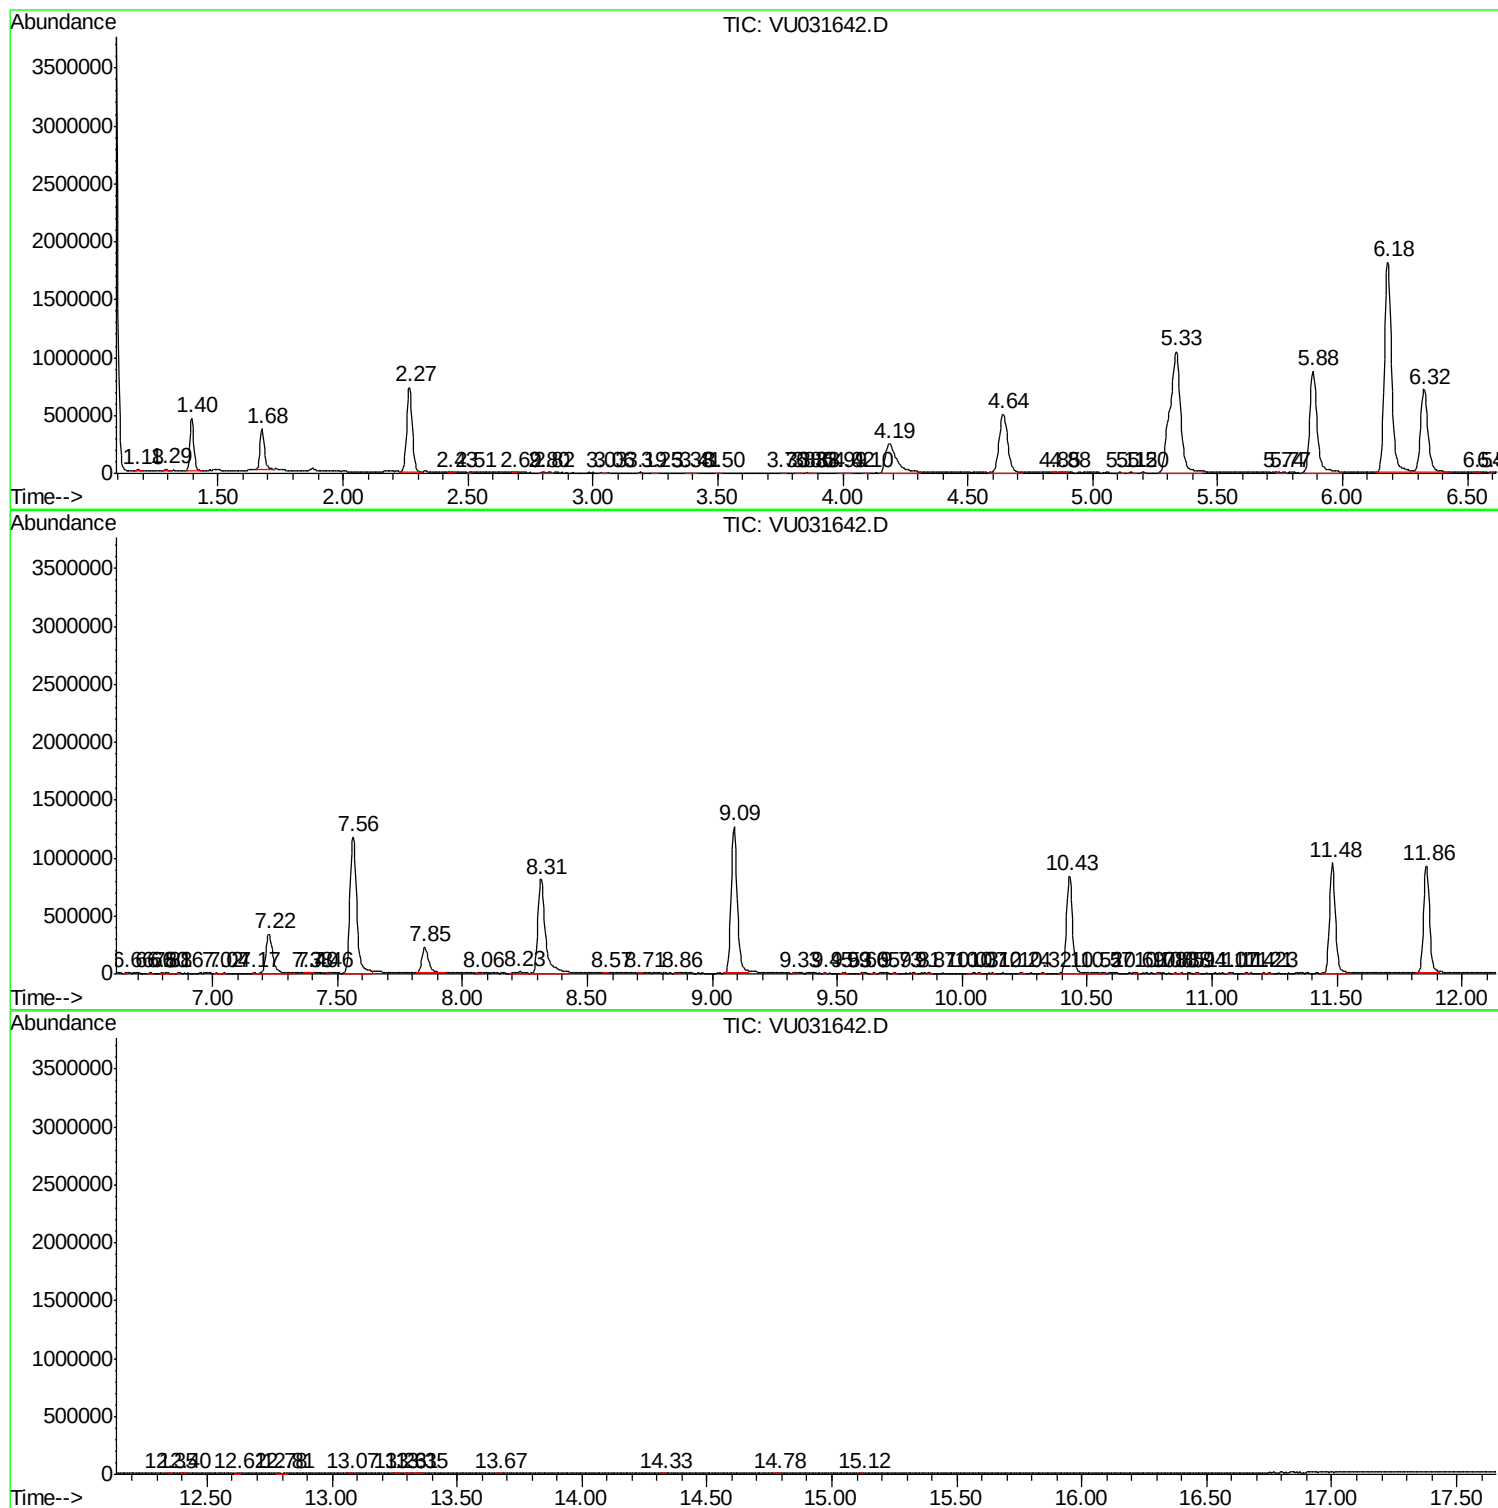

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031642.D
Acq On : 30 Apr 2019 18:26
Operator : JC/SP
Sample : K2593-11DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X75DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031642.D
Acq On : 30 Apr 2019 18:26
Operator : JC/SP
Sample : K2593-11DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X75DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc