

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031646.D
 Acq On : 30 Apr 2019 19:59
 Operator : JC/SP
 Sample : K2593-13 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB2	17228	16803	0.08%	0.038%
2	1.395	87	95	108	rBV	455841	486600	2.29%	1.102%
3	1.678	175	183	197	rBV	350752	433462	2.04%	0.982%
4	1.878	238	245	254	rVB	97327	133523	0.63%	0.303%
5	2.267	355	366	380	rVB	742565	1129247	5.33%	2.558%
6	2.524	443	446	451	rBV2	3201	2275	0.01%	0.005%
7	2.546	451	453	456	rVV2	1799	1111	0.01%	0.003%
8	2.566	456	459	464	rVB2	2655	2160	0.01%	0.005%
9	2.672	489	492	494	rBV	1777	1199	0.01%	0.003%
10	2.698	495	500	511	rVB5	5927	8764	0.04%	0.020%
11	2.765	518	521	525	rVB3	1196	933	0.00%	0.002%
12	2.794	525	530	533	rBV4	1245	1190	0.01%	0.003%
13	2.871	552	554	558	rBV3	1105	871	0.00%	0.002%
14	2.939	571	575	578	rBV2	1261	1113	0.01%	0.003%
15	2.971	582	585	588	rBV4	1255	987	0.00%	0.002%
16	3.016	596	599	604	rVB4	1281	1022	0.00%	0.002%
17	3.090	619	622	626	rBV2	1135	906	0.00%	0.002%
18	3.122	629	632	635	rBV2	1458	891	0.00%	0.002%
19	3.164	641	645	650	rVB3	1401	1323	0.01%	0.003%
20	3.193	650	654	658	rBV3	1888	1627	0.01%	0.004%
21	3.244	665	670	672	rBV2	1058	1127	0.01%	0.003%
22	3.260	672	675	680	rVV4	1234	1327	0.01%	0.003%
23	3.411	717	722	727	rVB6	1473	1734	0.01%	0.004%
24	3.485	742	745	754	rVB3	1471	1572	0.01%	0.004%
25	3.530	754	759	762	rBV2	1035	1004	0.00%	0.002%
26	3.595	774	779	781	rBV2	1041	845	0.00%	0.002%
27	3.862	859	862	870	rBV4	2195	2235	0.01%	0.005%
28	3.903	870	875	879	rBV2	1330	1258	0.01%	0.003%
29	3.952	885	890	894	rBV3	741	917	0.00%	0.002%
30	4.186	950	963	998	rBV2	250600	809985	3.82%	1.835%
31	4.460	1045	1048	1049	rBV3	1752	1054	0.00%	0.002%
32	4.524	1065	1068	1071	rVB	2352	1362	0.01%	0.003%
33	4.643	1087	1105	1134	rBV	520487	1233903	5.82%	2.796%
34	4.804	1152	1155	1160	rBV3	1175	1098	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031646.D
 Acq On : 30 Apr 2019 19:59
 Operator : JC/SP
 Sample : K2593-13 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.839	1163	1166	1170	rVB3	1597	1282	0.01%	0.003%
36	4.868	1170	1175	1176	rBV4	2263	1516	0.01%	0.003%
37	4.977	1203	1209	1216	rBV7	1515	2331	0.01%	0.005%
38	5.199	1274	1278	1281	rBV4	938	907	0.00%	0.002%
39	5.334	1295	1320	1344	rBV2	1046700	3130260	14.76%	7.092%
40	5.633	1409	1413	1417	rVB5	2046	2026	0.01%	0.005%
41	5.662	1417	1422	1425	rBV5	1668	1597	0.01%	0.004%
42	5.881	1477	1490	1515	rBV	876204	1794444	8.46%	4.066%
43	6.180	1566	1583	1616	rBV	10877045	21204897	100.00%	48.043%
44	6.324	1618	1628	1662	rVB	738370	1583659	7.47%	3.588%
45	6.623	1718	1721	1725	rVB6	1736	1480	0.01%	0.003%
46	6.910	1808	1810	1814	rVB3	1625	1072	0.01%	0.002%
47	7.225	1896	1908	1931	rBV	346827	654816	3.09%	1.484%
48	7.453	1972	1979	1981	rBV6	1507	1621	0.01%	0.004%
49	7.562	1999	2013	2030	rBV	1213827	2166909	10.22%	4.909%
50	7.787	2081	2083	2087	rVB4	2117	1183	0.01%	0.003%
51	7.848	2092	2102	2123	rVV	233317	424521	2.00%	0.962%
52	8.035	2158	2160	2164	rVB3	1550	877	0.00%	0.002%
53	8.173	2201	2203	2208	rVB4	1281	906	0.00%	0.002%
54	8.225	2208	2219	2236	rBV2	192360	343725	1.62%	0.779%
55	8.315	2236	2247	2291	rVV2	820463	1703395	8.03%	3.859%
56	8.617	2337	2341	2344	rBV4	1685	1226	0.01%	0.003%
57	8.771	2386	2389	2394	rBV4	1132	1201	0.01%	0.003%
58	8.832	2405	2408	2413	rVB5	1738	1212	0.01%	0.003%
59	8.897	2424	2428	2429	rBV2	1234	992	0.00%	0.002%
60	8.951	2437	2445	2446	rBV5	1760	1873	0.01%	0.004%
61	8.990	2453	2457	2459	rBV3	1321	1056	0.00%	0.002%
62	9.032	2465	2470	2474	rBV5	1485	1482	0.01%	0.003%
63	9.086	2474	2487	2509	rBV	1289147	2223546	10.49%	5.038%
64	9.244	2533	2536	2537	rBV3	1703	1035	0.00%	0.002%
65	9.784	2699	2704	2711	rVV6	2162	3282	0.02%	0.007%
66	9.900	2737	2740	2744	rVV	1610	1506	0.01%	0.003%
67	9.922	2745	2747	2752	rVB3	1801	1190	0.01%	0.003%
68	9.980	2760	2765	2767	rBV4	1127	964	0.00%	0.002%
69	10.019	2773	2777	2780	rBV4	1069	946	0.00%	0.002%
70	10.109	2800	2805	2807	rBV4	885	881	0.00%	0.002%
71	10.170	2821	2824	2828	rVV2	1726	1239	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031646.D
 Acq On : 30 Apr 2019 19:59
 Operator : JC/SP
 Sample : K2593-13 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.221	2837	2840	2843	rBV2	1380	940	0.00%	0.002%
73	10.427	2888	2904	2926	rBV	853576	1385262	6.53%	3.139%
74	10.649	2968	2973	2974	rBV3	1473	1226	0.01%	0.003%
75	10.659	2974	2976	2981	rVB2	1384	1023	0.00%	0.002%
76	10.717	2991	2994	3000	rVB4	1229	884	0.00%	0.002%
77	10.778	3009	3013	3015	rBV2	1399	1091	0.01%	0.002%
78	10.929	3058	3060	3064	rVB2	1569	876	0.00%	0.002%
79	10.987	3075	3078	3080	rBV3	1511	1076	0.01%	0.002%
80	11.054	3093	3099	3100	rBV3	1454	1257	0.01%	0.003%
81	11.144	3125	3127	3132	rVV2	1079	973	0.00%	0.002%
82	11.225	3149	3152	3155	rVB3	1510	943	0.00%	0.002%
83	11.244	3155	3158	3162	rBV2	1663	1497	0.01%	0.003%
84	11.395	3202	3205	3212	rVB3	1563	1568	0.01%	0.004%
85	11.482	3220	3232	3252	rBV	973762	1581004	7.46%	3.582%
86	11.858	3336	3349	3373	rBV	943114	1585487	7.48%	3.592%
87	12.157	3437	3442	3444	rBV5	1853	1918	0.01%	0.004%
88	12.768	3627	3632	3634	rBV2	1412	1326	0.01%	0.003%
89	12.800	3638	3642	3646	rVB4	1866	1503	0.01%	0.003%
90	12.826	3647	3650	3653	rVB2	1816	1133	0.01%	0.003%
91	12.977	3690	3697	3700	rBV5	1611	2177	0.01%	0.005%
92	13.331	3804	3807	3811	rBV3	1860	1660	0.01%	0.004%
93	13.450	3841	3844	3852	rVB4	2216	2218	0.01%	0.005%
94	13.530	3866	3869	3873	rBV2	1166	1121	0.01%	0.003%
95	13.652	3904	3907	3910	rBV2	1684	1259	0.01%	0.003%
96	13.945	3996	3998	4001	rVB3	1761	892	0.00%	0.002%
97	13.980	4006	4009	4013	rVV3	1350	1081	0.01%	0.002%
98	14.199	4074	4077	4080	rBV3	2231	1539	0.01%	0.003%
99	14.437	4148	4151	4154	rVB3	1716	965	0.00%	0.002%
100	14.739	4243	4245	4248	rBV3	1500	835	0.00%	0.002%


Sum of corrected areas: 44137217

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031646.D
Acq On : 30 Apr 2019 19:59
Operator : JC/SP
Sample : K2593-13 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

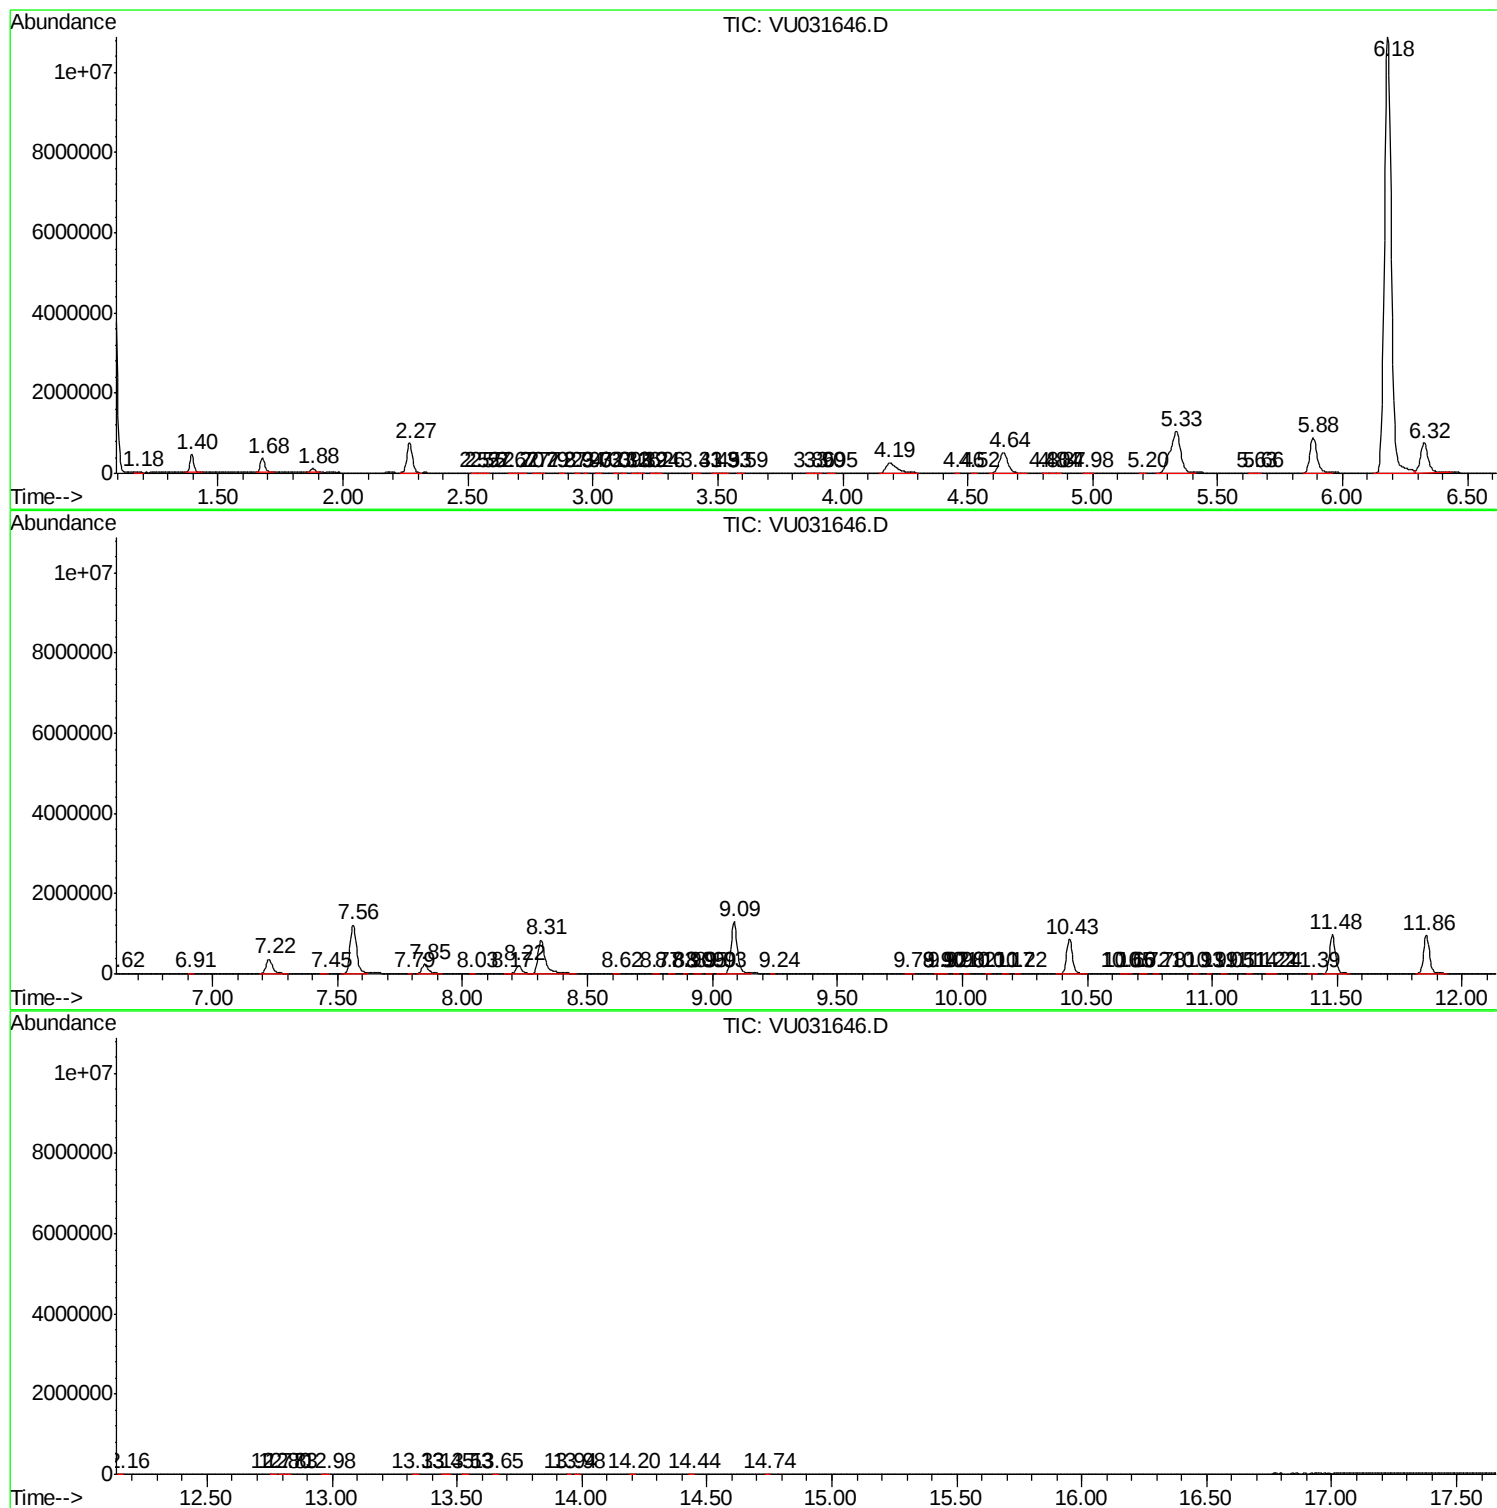

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031646.D
Acq On : 30 Apr 2019 19:59
Operator : JC/SP
Sample : K2593-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031646.D
Acq On : 30 Apr 2019 19:59
Operator : JC/SP
Sample : K2593-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X79

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc