

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031647.D
 Acq On : 30 Apr 2019 20:22
 Operator : JC/SP
 Sample : K2593-14 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	37	rVB3	16485	17337	0.02%	0.017%
2	1.290	59	62	68	rVB	17136	14078	0.02%	0.014%
3	1.396	87	95	110	rBV	454177	496571	0.66%	0.496%
4	1.675	175	182	193	rBV	337860	417089	0.55%	0.417%
5	1.878	236	245	257	rVB	380534	530325	0.70%	0.530%
6	2.267	355	366	380	rVB	754904	1159324	1.54%	1.159%
7	2.450	420	423	426	rBV3	1794	1546	0.00%	0.002%
8	2.540	448	451	453	rBV3	1546	884	0.00%	0.001%
9	2.621	471	476	480	rBV5	1536	1952	0.00%	0.002%
10	2.698	489	500	513	rVB3	15771	29592	0.04%	0.030%
11	2.749	513	516	522	rVB4	2505	2206	0.00%	0.002%
12	2.817	532	537	541	rBV5	1370	1569	0.00%	0.002%
13	2.978	580	587	588	rBV6	2872	2676	0.00%	0.003%
14	3.129	631	634	637	rBV3	1309	893	0.00%	0.001%
15	3.187	646	652	657	rVB4	1233	1318	0.00%	0.001%
16	3.219	657	662	664	rBV2	1194	1124	0.00%	0.001%
17	3.325	688	695	697	rBV2	1278	1148	0.00%	0.001%
18	3.386	710	714	717	rVV2	1289	1001	0.00%	0.001%
19	3.576	769	773	777	rVB3	1370	1293	0.00%	0.001%
20	3.630	782	790	792	rBV5	1246	1468	0.00%	0.001%
21	4.080	925	930	937	rBV5	1449	2356	0.00%	0.002%
22	4.186	949	963	1010	rBV	273189	918690	1.22%	0.918%
23	4.643	1087	1105	1130	rVV	530091	1261834	1.67%	1.261%
24	4.839	1160	1166	1167	rBV3	1540	1450	0.00%	0.001%
25	4.871	1173	1176	1179	rBV4	1760	1293	0.00%	0.001%
26	4.968	1201	1206	1207	rBV4	1052	882	0.00%	0.001%
27	5.051	1227	1232	1237	rVB6	1022	1377	0.00%	0.001%
28	5.077	1237	1240	1243	rBV3	1522	1004	0.00%	0.001%
29	5.125	1247	1255	1265	rBV7	5087	10696	0.01%	0.011%
30	5.167	1265	1268	1273	rVB6	2047	1676	0.00%	0.002%
31	5.334	1297	1320	1341	rBV2	1061418	3169241	4.20%	3.168%
32	5.688	1427	1430	1434	rVB2	1848	1246	0.00%	0.001%
33	5.711	1434	1437	1439	rVV2	1611	988	0.00%	0.001%
34	5.762	1450	1453	1456	rVB3	1291	834	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031647.D
 Acq On : 30 Apr 2019 20:22
 Operator : JC/SP
 Sample : K2593-14 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.804	1463	1466	1472	rBV6	1804	2025	0.00%	0.002%
36	5.881	1477	1490	1523	rBV	890453	1851436	2.45%	1.851%
37	6.183	1565	1584	1618	rBV	39049011	75484243	100.00%	75.450%
38	6.325	1620	1628	1665	rVB	785559	1756274	2.33%	1.755%
39	6.804	1775	1777	1779	rBV3	1509	922	0.00%	0.001%
40	6.884	1798	1802	1804	rBV4	1235	1044	0.00%	0.001%
41	7.048	1851	1853	1856	rVB2	1892	1038	0.00%	0.001%
42	7.077	1856	1862	1865	rBV6	1581	1629	0.00%	0.002%
43	7.145	1879	1883	1888	rVB4	1527	1444	0.00%	0.001%
44	7.225	1896	1908	1938	rBV	361500	688290	0.91%	0.688%
45	7.328	1938	1940	1944	rVB4	1944	1164	0.00%	0.001%
46	7.563	1999	2013	2027	rBV	1225670	2199950	2.91%	2.199%
47	7.849	2090	2102	2122	rBV	241472	439163	0.58%	0.439%
48	8.067	2165	2170	2172	rBV5	4020	3464	0.00%	0.003%
49	8.225	2207	2219	2234	rVV	373753	663455	0.88%	0.663%
50	8.315	2236	2247	2291	rVB2	905193	1842725	2.44%	1.842%
51	8.633	2344	2346	2347	rBV2	2120	951	0.00%	0.001%
52	8.678	2356	2360	2362	rBV2	1462	1009	0.00%	0.001%
53	8.717	2369	2372	2374	rBV3	1470	1039	0.00%	0.001%
54	8.807	2394	2400	2402	rBV4	1253	1394	0.00%	0.001%
55	8.868	2412	2419	2424	rBV6	1922	2736	0.00%	0.003%
56	8.910	2428	2432	2434	rBV3	1607	1235	0.00%	0.001%
57	8.961	2445	2448	2451	rBV5	1151	814	0.00%	0.001%
58	9.003	2455	2461	2463	rBV4	1682	1551	0.00%	0.002%
59	9.087	2473	2487	2519	rBV	1328219	2288369	3.03%	2.287%
60	9.379	2570	2578	2588	rBV4	13392	23515	0.03%	0.024%
61	9.508	2613	2618	2620	rBV4	1065	1007	0.00%	0.001%
62	9.575	2635	2639	2642	rBV4	1133	1258	0.00%	0.001%
63	9.781	2695	2703	2714	rBV6	7802	12971	0.02%	0.013%
64	9.823	2714	2716	2723	rVB5	1526	1132	0.00%	0.001%
65	9.884	2729	2735	2740	rBV6	2029	2234	0.00%	0.002%
66	9.913	2740	2744	2747	rBV2	1248	818	0.00%	0.001%
67	9.958	2753	2758	2760	rBV4	1067	1181	0.00%	0.001%
68	10.180	2824	2827	2830	rVB	1419	852	0.00%	0.001%
69	10.296	2857	2863	2870	rVB4	2201	2963	0.00%	0.003%
70	10.328	2870	2873	2875	rBV2	2247	1493	0.00%	0.001%
71	10.427	2891	2904	2927	rBV	882738	1427819	1.89%	1.427%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031647.D
 Acq On : 30 Apr 2019 20:22
 Operator : JC/SP
 Sample : K2593-14 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.588	2951	2954	2956	rVB	1618	878	0.00%	0.001%
73	10.672	2974	2980	2982	rBV3	1971	1970	0.00%	0.002%
74	10.697	2986	2988	2994	rVB6	2799	2328	0.00%	0.002%
75	10.910	3049	3054	3060	rVB5	1241	1811	0.00%	0.002%
76	10.942	3060	3064	3066	rBV2	1668	1250	0.00%	0.001%
77	11.154	3121	3130	3144	rVB8	6530	11661	0.02%	0.012%
78	11.212	3144	3148	3152	rVB3	1073	1008	0.00%	0.001%
79	11.238	3152	3156	3158	rBV3	1213	857	0.00%	0.001%
80	11.315	3175	3180	3184	rVB3	1114	1012	0.00%	0.001%
81	11.350	3187	3191	3196	rBV5	2156	2150	0.00%	0.002%
82	11.482	3217	3232	3252	rBV	985384	1616671	2.14%	1.616%
83	11.855	3337	3348	3373	rBV	946122	1607093	2.13%	1.606%
84	12.157	3437	3442	3448	rVB7	1654	1924	0.00%	0.002%
85	12.289	3480	3483	3486	rBV3	1916	1334	0.00%	0.001%
86	12.466	3534	3538	3542	rBV4	2021	1857	0.00%	0.002%
87	12.527	3553	3557	3559	rBV2	1344	1141	0.00%	0.001%
88	12.784	3634	3637	3640	rVB4	2075	1404	0.00%	0.001%
89	12.804	3640	3643	3649	rVB5	1266	1047	0.00%	0.001%
90	12.926	3678	3681	3686	rVB3	1942	1484	0.00%	0.001%
91	12.958	3687	3691	3692	rBV3	1217	957	0.00%	0.001%
92	13.183	3757	3761	3764	rBV2	1170	990	0.00%	0.001%
93	13.299	3793	3797	3801	rBV	2483	2345	0.00%	0.002%
94	13.324	3801	3805	3810	rVV4	1994	2212	0.00%	0.002%
95	13.424	3833	3836	3840	rVB3	2114	1280	0.00%	0.001%
96	13.594	3886	3889	3893	rBV3	1531	1364	0.00%	0.001%
97	13.675	3910	3914	3918	rBV3	1972	2149	0.00%	0.002%
98	14.057	4029	4033	4036	rBV3	2151	1454	0.00%	0.001%
99	14.173	4066	4069	4071	rBV3	1552	1027	0.00%	0.001%
100	14.987	4320	4322	4325	rBV	1884	1047	0.00%	0.001%


Sum of corrected areas: 100045273

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031647.D
Acq On : 30 Apr 2019 20:22
Operator : JC/SP
Sample : K2593-14 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

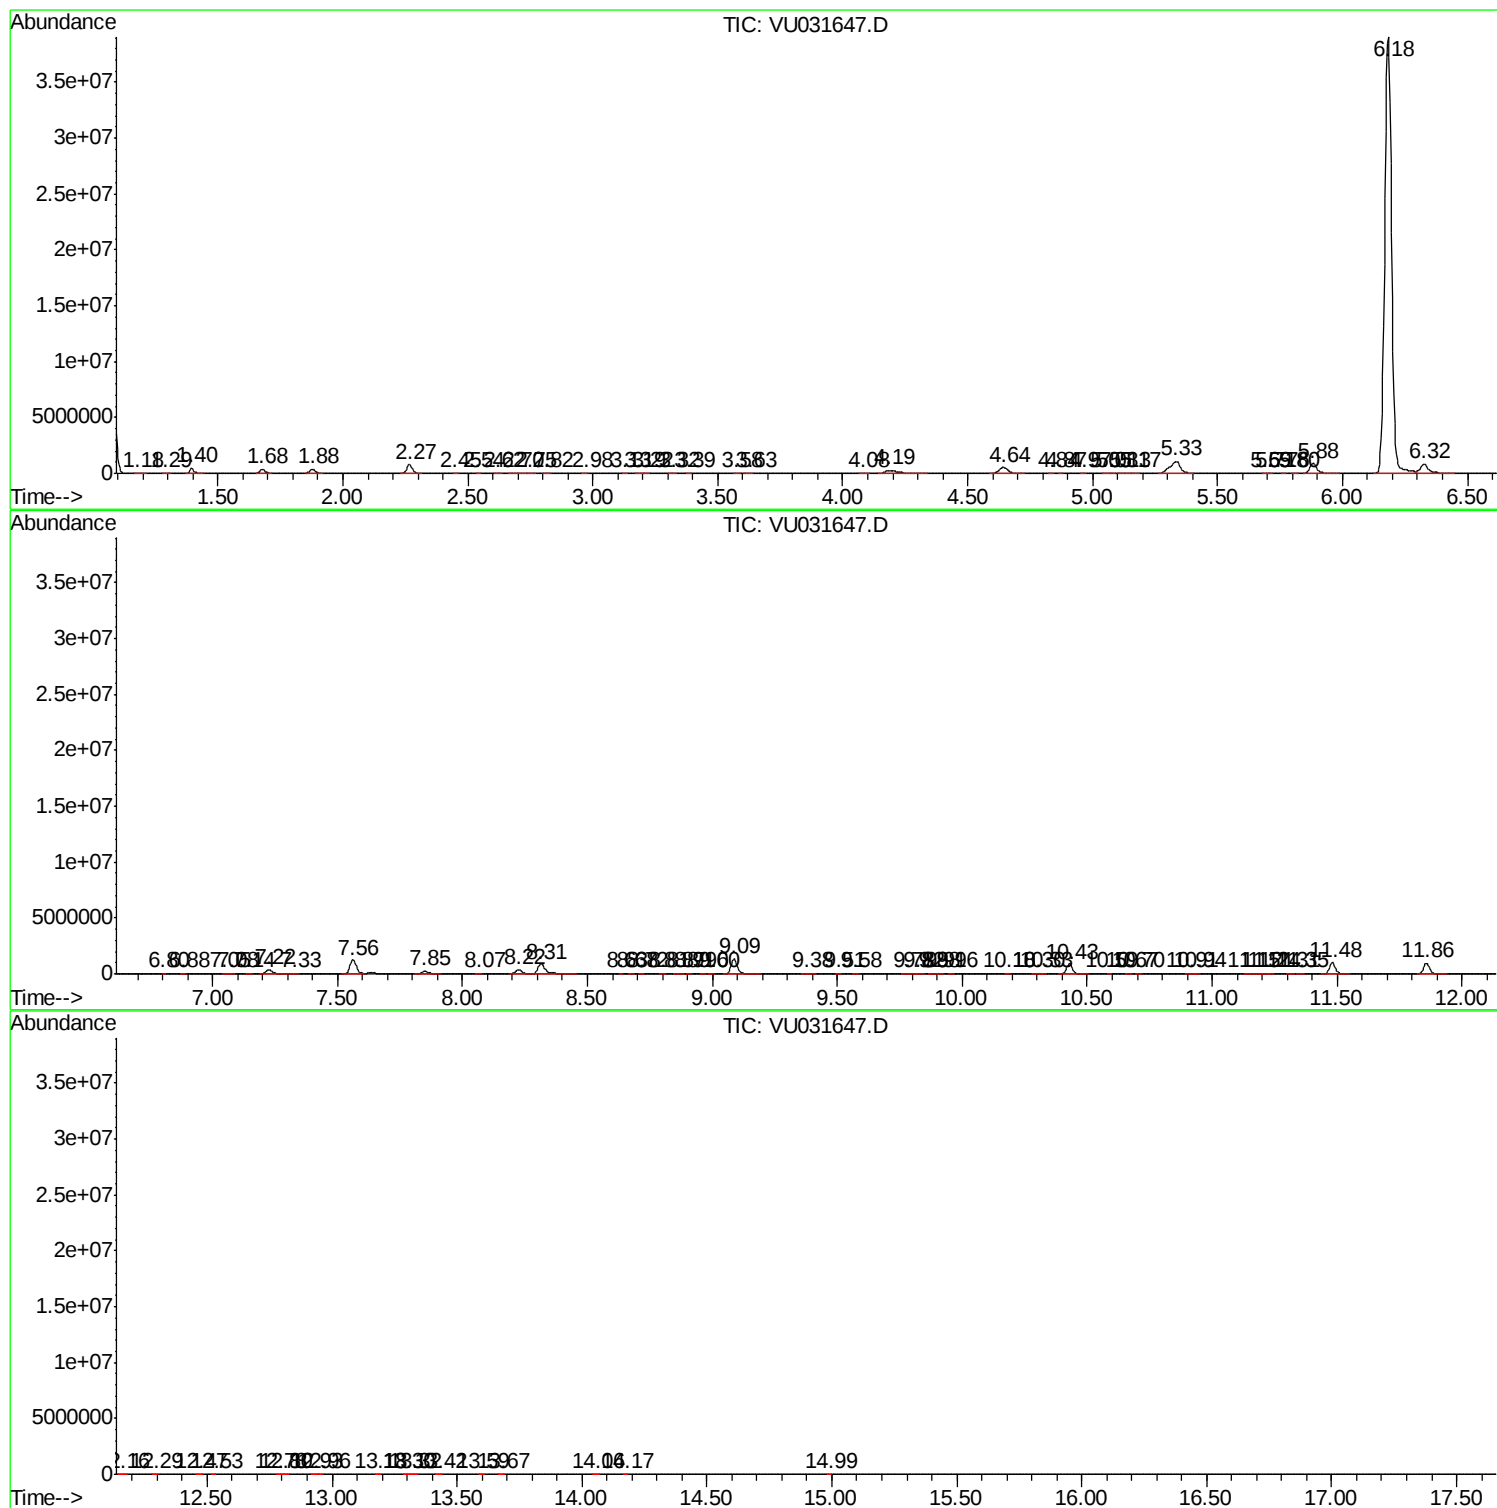

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031647.D
Acq On : 30 Apr 2019 20:22
Operator : JC/SP
Sample : K2593-14 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031647.D
Acq On : 30 Apr 2019 20:22
Operator : JC/SP
Sample : K2593-14 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc