

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031648.D
 Acq On : 30 Apr 2019 20:46
 Operator : JC/SP
 Sample : K2593-15 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rVB	15590	12980	0.02%	0.014%
2	1.290	59	62	68	rVB2	16166	13546	0.02%	0.015%
3	1.392	87	94	106	rBV	445429	502121	0.76%	0.542%
4	1.675	175	182	197	rBV	367616	462195	0.70%	0.498%
5	1.875	236	244	262	rVB	348870	502519	0.76%	0.542%
6	2.264	355	365	379	rVB	771371	1176971	1.77%	1.269%
7	2.579	460	463	467	rVB4	1421	1038	0.00%	0.001%
8	2.698	491	500	507	rBV7	4186	6982	0.01%	0.008%
9	2.794	526	530	535	rBV5	1377	1222	0.00%	0.001%
10	2.823	535	539	540	rBV4	1498	1038	0.00%	0.001%
11	2.952	575	579	581	rBV2	1201	806	0.00%	0.001%
12	2.974	582	586	591	rVV7	1712	1911	0.00%	0.002%
13	3.000	591	594	597	rVB3	1223	784	0.00%	0.001%
14	3.058	606	612	616	rVB5	1809	2038	0.00%	0.002%
15	3.080	616	619	623	rBV2	1179	1251	0.00%	0.001%
16	3.106	623	627	633	rVV5	1371	1632	0.00%	0.002%
17	3.135	633	636	642	rVB4	870	854	0.00%	0.001%
18	3.171	642	647	651	rBV4	1486	1508	0.00%	0.002%
19	3.219	658	662	664	rBV4	1044	976	0.00%	0.001%
20	3.450	730	734	739	rBV4	1207	1149	0.00%	0.001%
21	3.659	795	799	803	rVV2	990	915	0.00%	0.001%
22	3.939	882	886	889	rBV3	1090	887	0.00%	0.001%
23	4.084	927	931	935	rVB4	1487	1169	0.00%	0.001%
24	4.187	951	963	1003	rBV	268485	865412	1.30%	0.933%
25	4.531	1065	1070	1075	rBV5	2280	2185	0.00%	0.002%
26	4.560	1075	1079	1085	rBV3	1310	1556	0.00%	0.002%
27	4.643	1088	1105	1132	rVV2	541643	1289891	1.94%	1.391%
28	4.884	1177	1180	1183	rVB3	1384	914	0.00%	0.001%
29	4.926	1191	1193	1198	rBV3	1555	1341	0.00%	0.001%
30	4.968	1202	1206	1210	rBV5	999	1091	0.00%	0.001%
31	5.055	1230	1233	1239	rVB	1727	1516	0.00%	0.002%
32	5.135	1244	1258	1268	rVB3	9640	21356	0.03%	0.023%
33	5.241	1284	1291	1293	rBV5	1502	1344	0.00%	0.001%
34	5.334	1297	1320	1345	rBV2	1107536	3309675	4.98%	3.569%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031648.D
 Acq On : 30 Apr 2019 20:46
 Operator : JC/SP
 Sample : K2593-15 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.682	1425	1428	1431	rVV5	1594	1065	0.00%	0.001%
36	5.759	1449	1452	1457	rVB5	1767	1434	0.00%	0.002%
37	5.785	1457	1460	1466	rBV4	1568	1674	0.00%	0.002%
38	5.881	1475	1490	1526	rBV	933790	1949231	2.93%	2.102%
39	6.183	1565	1584	1618	rBV	34654209	66498785	100.00%	71.715%
40	6.325	1620	1628	1661	rVB	799267	1742725	2.62%	1.879%
41	6.730	1752	1754	1758	rBV4	1533	1098	0.00%	0.001%
42	6.868	1795	1797	1802	rVB3	1691	1231	0.00%	0.001%
43	6.903	1805	1808	1817	rVB7	2151	2125	0.00%	0.002%
44	6.961	1823	1826	1827	rBV2	1932	946	0.00%	0.001%
45	7.010	1837	1841	1845	rVB6	1204	1098	0.00%	0.001%
46	7.039	1845	1850	1852	rBV4	1237	993	0.00%	0.001%
47	7.161	1884	1888	1890	rVB3	1374	899	0.00%	0.001%
48	7.225	1896	1908	1929	rBV	371954	691121	1.04%	0.745%
49	7.370	1950	1953	1958	rVB3	2312	2159	0.00%	0.002%
50	7.395	1958	1961	1963	rBV3	1329	846	0.00%	0.001%
51	7.511	1994	1997	2000	rBV4	1631	1019	0.00%	0.001%
52	7.563	2000	2013	2029	rBV	1277022	2302700	3.46%	2.483%
53	7.849	2091	2102	2132	rVV	243078	453202	0.68%	0.489%
54	8.055	2163	2166	2167	rBV	2204	1381	0.00%	0.001%
55	8.222	2204	2218	2236	rBV	951028	1683627	2.53%	1.816%
56	8.315	2237	2247	2281	rVB	931648	1845173	2.77%	1.990%
57	8.682	2356	2361	2363	rBV3	1393	1398	0.00%	0.002%
58	8.903	2426	2430	2431	rBV4	1600	978	0.00%	0.001%
59	8.987	2453	2456	2458	rBV3	1736	1200	0.00%	0.001%
60	9.087	2475	2487	2530	rBV	1354197	2354380	3.54%	2.539%
61	9.376	2565	2577	2588	rBV3	32408	58576	0.09%	0.063%
62	9.604	2645	2648	2654	rVB3	1701	1721	0.00%	0.002%
63	9.643	2657	2660	2663	rVB3	1774	1044	0.00%	0.001%
64	9.675	2663	2670	2672	rBV3	1676	1794	0.00%	0.002%
65	9.704	2677	2679	2685	rBV3	961	834	0.00%	0.001%
66	9.736	2685	2689	2692	rBV3	1204	1092	0.00%	0.001%
67	9.781	2693	2703	2712	rBV4	19579	33360	0.05%	0.036%
68	9.926	2743	2748	2751	rBV3	2273	1587	0.00%	0.002%
69	9.958	2755	2758	2761	rVB2	1569	992	0.00%	0.001%
70	10.067	2787	2792	2796	rBV3	2652	2593	0.00%	0.003%
71	10.099	2796	2802	2807	rBV7	1082	1663	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031648.D
 Acq On : 30 Apr 2019 20:46
 Operator : JC/SP
 Sample : K2593-15 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.164	2816	2822	2828	rBV6	3430	4602	0.01%	0.005%
73	10.270	2852	2855	2860	rVV2	1029	755	0.00%	0.001%
74	10.337	2871	2876	2879	rBV4	1123	1170	0.00%	0.001%
75	10.427	2891	2904	2925	rBV	885959	1450845	2.18%	1.565%
76	10.591	2951	2955	2959	rVB5	2254	2034	0.00%	0.002%
77	10.681	2973	2983	2985	rBV4	9257	11252	0.02%	0.012%
78	10.778	3005	3013	3022	rVB9	5003	8261	0.01%	0.009%
79	10.929	3055	3060	3063	rBV4	1136	1102	0.00%	0.001%
80	10.977	3063	3075	3082	rVV5	7388	11783	0.02%	0.013%
81	11.148	3120	3128	3139	rVV3	18658	29502	0.04%	0.032%
82	11.292	3171	3173	3178	rVB3	1221	905	0.00%	0.001%
83	11.382	3195	3201	3204	rBV2	2280	2388	0.00%	0.003%
84	11.421	3210	3213	3215	rVB3	1487	816	0.00%	0.001%
85	11.482	3219	3232	3252	rBV	1027845	1673960	2.52%	1.805%
86	11.752	3313	3316	3317	rBV2	1833	991	0.00%	0.001%
87	11.855	3336	3348	3375	rBV	984786	1666336	2.51%	1.797%
88	12.180	3445	3449	3453	rBV5	1531	1569	0.00%	0.002%
89	12.273	3473	3478	3481	rBV6	1894	2380	0.00%	0.003%
90	12.373	3506	3509	3511	rBV2	1896	1100	0.00%	0.001%
91	12.450	3530	3533	3535	rBV3	1951	1432	0.00%	0.002%
92	12.505	3547	3550	3552	rBV	1606	1139	0.00%	0.001%
93	12.707	3610	3613	3616	rVB3	1763	1183	0.00%	0.001%
94	12.964	3690	3693	3701	rVB2	2046	2370	0.00%	0.003%
95	13.868	3971	3974	3978	rBV2	1712	1580	0.00%	0.002%
96	14.074	4035	4038	4040	rBV2	2038	1496	0.00%	0.002%
97	14.141	4057	4059	4063	rBV2	1267	950	0.00%	0.001%
98	14.324	4112	4116	4119	rBV3	1348	1370	0.00%	0.001%
99	14.559	4187	4189	4194	rBV2	1493	1088	0.00%	0.001%
100	14.826	4270	4272	4278	rBV3	1819	1381	0.00%	0.001%


Sum of corrected areas: 92726257

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031648.D
Acq On : 30 Apr 2019 20:46
Operator : JC/SP
Sample : K2593-15 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

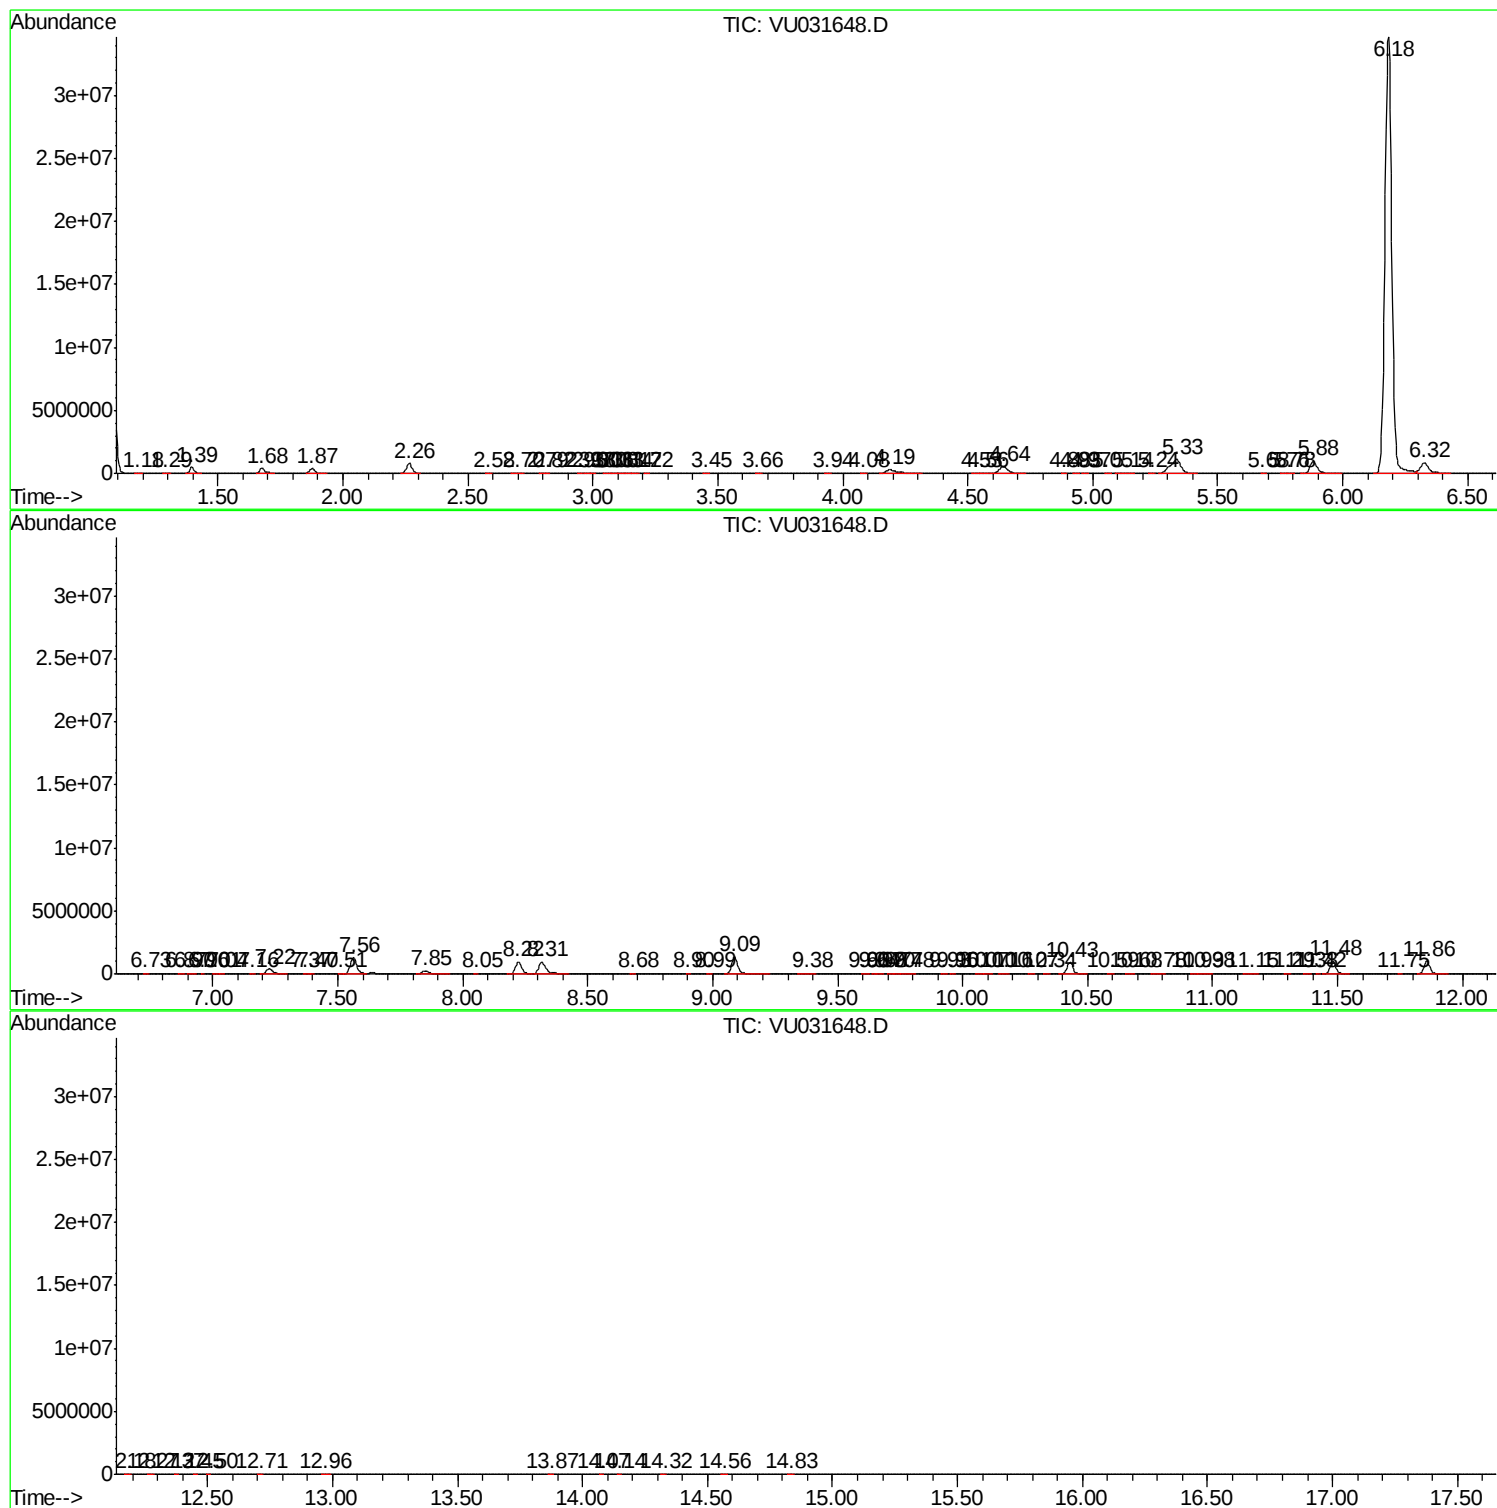

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031648.D
Acq On : 30 Apr 2019 20:46
Operator : JC/SP
Sample : K2593-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031648.D
Acq On : 30 Apr 2019 20:46
Operator : JC/SP
Sample : K2593-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc