

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031650.D
 Acq On : 30 Apr 2019 21:32
 Operator : JC/SP
 Sample : K2593-17 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	39	rVB4	15706	16024	0.04%	0.024%
2	1.396	87	95	106	rBV	434582	487249	1.13%	0.723%
3	1.675	175	182	193	rBV	344102	425010	0.98%	0.631%
4	1.878	237	245	257	rVB	191157	267128	0.62%	0.397%
5	2.264	355	365	379	rVB	734143	1127043	2.60%	1.673%
6	2.434	416	418	423	rBV5	1081	854	0.00%	0.001%
7	2.505	438	440	443	rBV3	1193	749	0.00%	0.001%
8	2.527	443	447	449	rVV3	1550	1140	0.00%	0.002%
9	2.592	465	467	471	rVB3	1973	1223	0.00%	0.002%
10	2.621	471	476	479	rBV6	2606	2608	0.01%	0.004%
11	2.701	496	501	513	rVB4	10567	16214	0.04%	0.024%
12	2.978	582	587	593	rBV5	2370	3376	0.01%	0.005%
13	3.074	613	617	621	rVB3	1326	1231	0.00%	0.002%
14	3.100	621	625	628	rBV4	1203	1218	0.00%	0.002%
15	3.119	628	631	636	rVV4	1492	1256	0.00%	0.002%
16	3.196	650	655	659	rVB4	1146	1109	0.00%	0.002%
17	3.225	659	664	668	rBV4	1047	1152	0.00%	0.002%
18	3.383	710	713	717	rVV2	1469	1163	0.00%	0.002%
19	3.402	717	719	724	rVB5	1355	759	0.00%	0.001%
20	3.495	743	748	751	rBV3	1227	1135	0.00%	0.002%
21	3.518	751	755	758	rVV2	1136	856	0.00%	0.001%
22	3.550	758	765	768	rVV6	967	1192	0.00%	0.002%
23	3.611	781	784	786	rBV	2252	1324	0.00%	0.002%
24	3.743	822	825	827	rBV2	1298	758	0.00%	0.001%
25	3.846	854	857	860	rVB3	1332	857	0.00%	0.001%
26	3.981	897	899	905	rVB2	1689	1005	0.00%	0.001%
27	4.026	910	913	918	rBV4	902	911	0.00%	0.001%
28	4.064	918	925	930	rVB2	1806	2737	0.01%	0.004%
29	4.186	951	963	995	rBV2	270594	887168	2.05%	1.317%
30	4.534	1064	1071	1073	rBV4	2901	2919	0.01%	0.004%
31	4.640	1088	1104	1135	rBV	536403	1277764	2.95%	1.897%
32	4.865	1171	1174	1176	rBV2	1331	926	0.00%	0.001%
33	4.974	1204	1208	1212	rBV4	1653	1548	0.00%	0.002%
34	5.006	1216	1218	1223	rVB4	1673	913	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031650.D
 Acq On : 30 Apr 2019 21:32
 Operator : JC/SP
 Sample : K2593-17 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.135	1247	1258	1261	rBV5	3233	5214	0.01%	0.008%
36	5.193	1272	1276	1279	rBV2	1646	1375	0.00%	0.002%
37	5.225	1283	1286	1289	rBV	1097	973	0.00%	0.001%
38	5.244	1289	1292	1296	rVB2	1154	1059	0.00%	0.002%
39	5.334	1296	1320	1347	rBV2	1075054	3228756	7.46%	4.793%
40	5.575	1392	1395	1397	rVB4	1557	820	0.00%	0.001%
41	5.710	1435	1437	1440	rVB2	2275	1139	0.00%	0.002%
42	5.733	1440	1444	1447	rBV4	2310	2080	0.00%	0.003%
43	5.784	1458	1460	1469	rVB6	1048	1139	0.00%	0.002%
44	5.881	1475	1490	1525	rBV	902951	1897546	4.38%	2.817%
45	6.180	1566	1583	1617	rBV	22404944	43291503	100.00%	64.270%
46	6.325	1619	1628	1666	rVB	775187	1701543	3.93%	2.526%
47	6.788	1769	1772	1775	rBV3	1183	753	0.00%	0.001%
48	6.846	1788	1790	1794	rBV4	1540	1424	0.00%	0.002%
49	6.907	1804	1809	1815	rBV5	2043	3083	0.01%	0.005%
50	6.993	1833	1836	1839	rVB3	1984	1093	0.00%	0.002%
51	7.013	1839	1842	1844	rBV3	1566	1138	0.00%	0.002%
52	7.141	1878	1882	1885	rBV2	1357	1203	0.00%	0.002%
53	7.225	1895	1908	1937	rBV	361562	686344	1.59%	1.019%
54	7.563	1999	2013	2029	rBV	1219505	2199038	5.08%	3.265%
55	7.849	2091	2102	2128	rBV	245415	447254	1.03%	0.664%
56	8.141	2188	2193	2197	rVB7	1438	1413	0.00%	0.002%
57	8.170	2197	2202	2205	rBV6	1671	1665	0.00%	0.002%
58	8.225	2207	2219	2235	rBV3	310285	556151	1.28%	0.826%
59	8.315	2236	2247	2282	rVV	922547	1825944	4.22%	2.711%
60	8.890	2422	2426	2429	rBV4	2205	1485	0.00%	0.002%
61	8.919	2432	2435	2443	rVB4	2259	2432	0.01%	0.004%
62	9.022	2463	2467	2470	rBV5	1965	1907	0.00%	0.003%
63	9.087	2474	2487	2521	rBV	1318721	2276395	5.26%	3.379%
64	9.325	2558	2561	2564	rBV3	1352	1327	0.00%	0.002%
65	9.382	2571	2579	2587	rBV7	8675	13452	0.03%	0.020%
66	9.562	2628	2635	2638	rBV5	1774	2247	0.01%	0.003%
67	9.627	2652	2655	2657	rBV	1229	807	0.00%	0.001%
68	9.691	2672	2675	2678	rBV3	1159	740	0.00%	0.001%
69	9.742	2688	2691	2696	rBV4	1121	765	0.00%	0.001%
70	9.781	2696	2703	2715	rVV10	6296	12001	0.03%	0.018%
71	9.916	2741	2745	2748	rVB4	1114	986	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043019\
 Data File : VU031650.D
 Acq On : 30 Apr 2019 21:32
 Operator : JC/SP
 Sample : K2593-17 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.968	2757	2761	2763	rBV2	994	853	0.00%	0.001%
73	9.987	2765	2767	2770	rVB3	1712	889	0.00%	0.001%
74	10.016	2770	2776	2779	rBV3	1860	2042	0.00%	0.003%
75	10.083	2793	2797	2801	rBV4	1284	1026	0.00%	0.002%
76	10.103	2801	2803	2809	rBV5	1270	1272	0.00%	0.002%
77	10.154	2814	2819	2820	rBV3	1257	1090	0.00%	0.002%
78	10.251	2846	2849	2852	rBV4	1089	794	0.00%	0.001%
79	10.427	2892	2904	2930	rBV	871442	1436046	3.32%	2.132%
80	10.591	2952	2955	2961	rVB4	1225	1187	0.00%	0.002%
81	10.643	2967	2971	2975	rBV2	1889	1515	0.00%	0.002%
82	10.681	2980	2983	2985	rBV2	1780	1198	0.00%	0.002%
83	10.906	3049	3053	3056	rVB3	1876	1348	0.00%	0.002%
84	10.977	3072	3075	3076	rBV2	1423	844	0.00%	0.001%
85	11.154	3120	3130	3137	rBV7	4190	7295	0.02%	0.011%
86	11.357	3190	3193	3196	rBV2	1350	906	0.00%	0.001%
87	11.482	3219	3232	3253	rBV	977844	1586122	3.66%	2.355%
88	11.858	3333	3349	3372	rBV	944395	1588449	3.67%	2.358%
89	12.572	3568	3571	3573	rBV2	1338	976	0.00%	0.001%
90	12.704	3610	3612	3616	rVB3	1043	731	0.00%	0.001%
91	12.746	3622	3625	3627	rBV2	1219	757	0.00%	0.001%
92	12.852	3655	3658	3661	rBV3	1514	1177	0.00%	0.002%
93	13.241	3774	3779	3783	rBV5	1759	2236	0.01%	0.003%
94	13.295	3792	3796	3797	rBV2	1477	984	0.00%	0.001%
95	13.874	3974	3976	3979	rBV4	1354	976	0.00%	0.001%
96	13.916	3986	3989	3991	rVB	1717	904	0.00%	0.001%
97	13.935	3992	3995	4003	rVB3	1805	2168	0.01%	0.003%
98	14.045	4026	4029	4031	rBV3	1412	976	0.00%	0.001%
99	14.077	4037	4039	4042	rBV2	1312	821	0.00%	0.001%
100	14.594	4198	4200	4203	rBV2	1688	1008	0.00%	0.001%


Sum of corrected areas: 67359303

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043019\
Data File : VU031650.D
Acq On : 30 Apr 2019 21:32
Operator : JC/SP
Sample : K2593-17 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

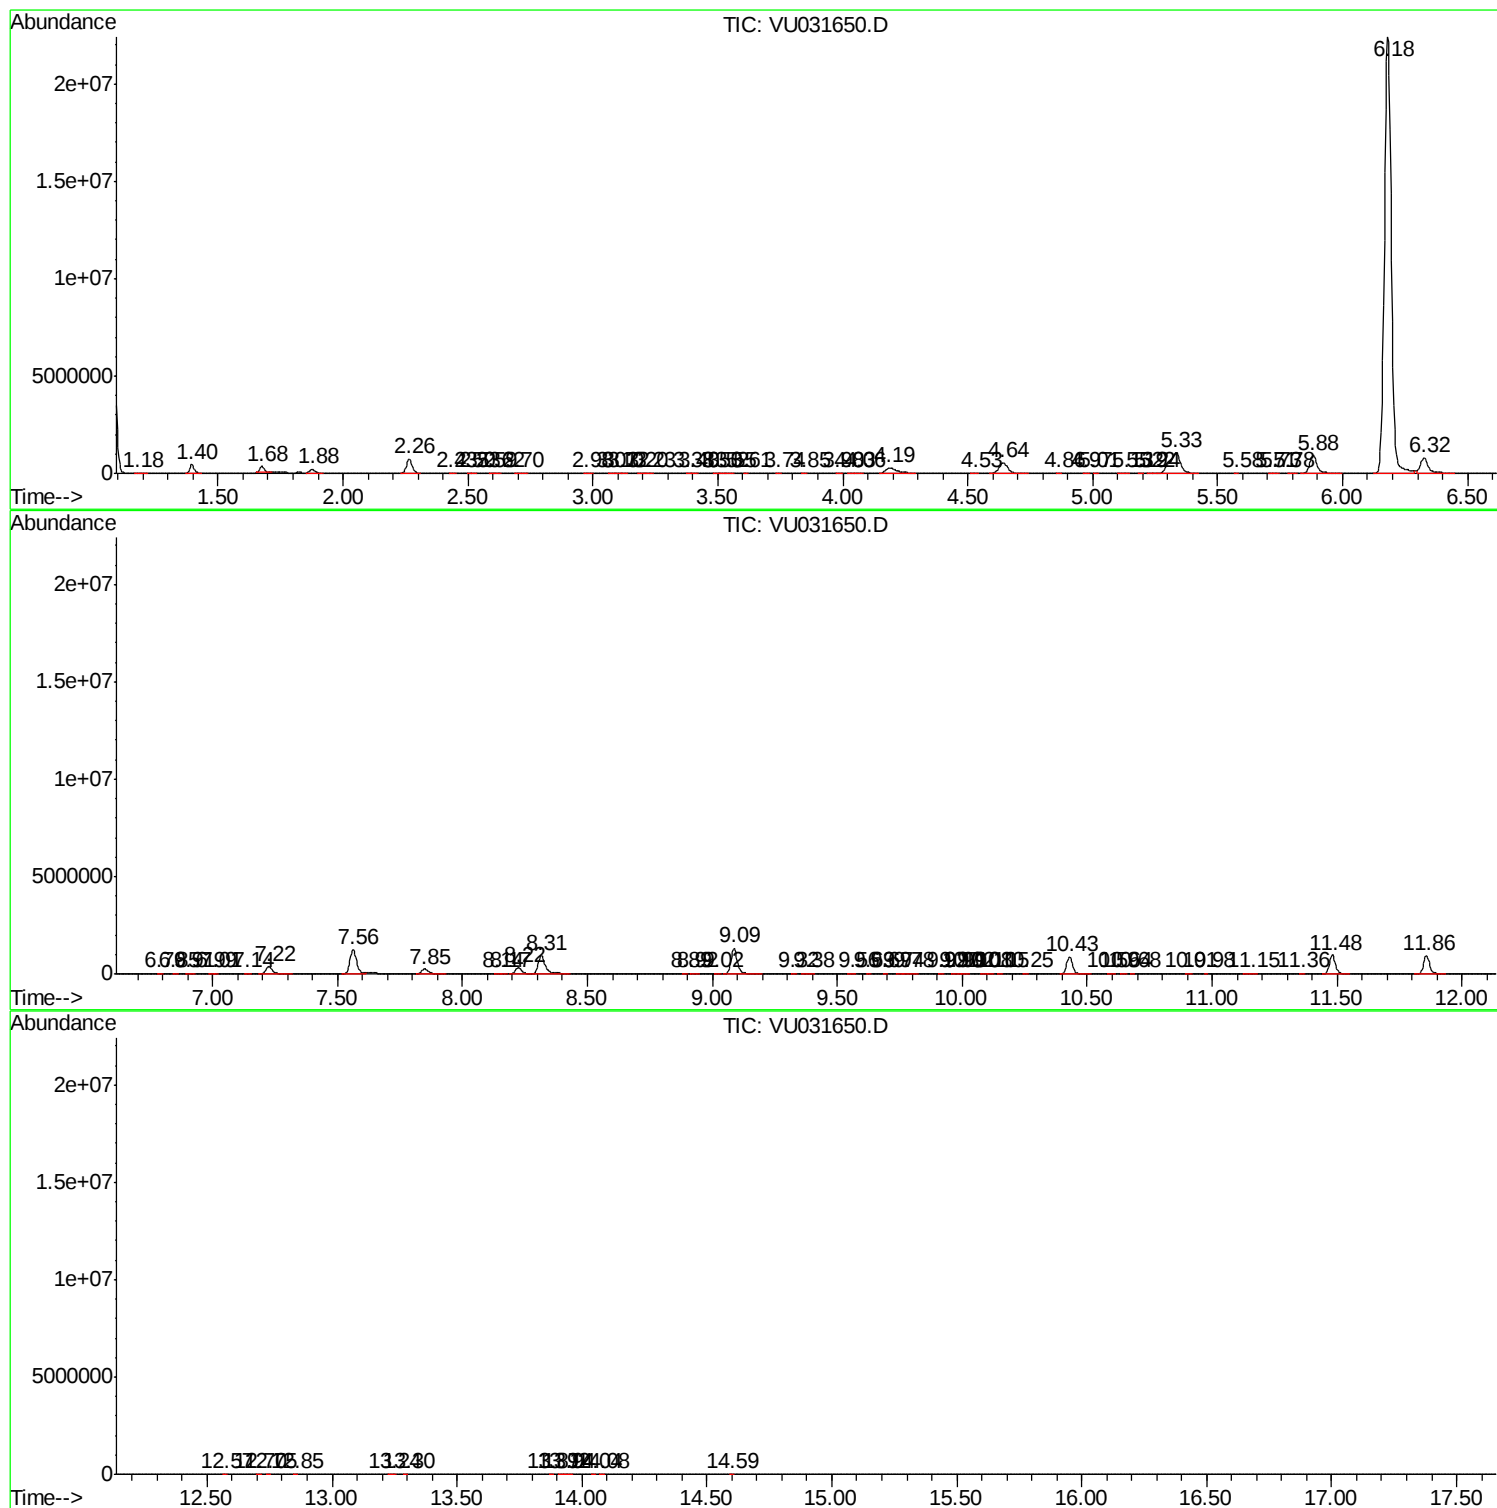

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031650.D
Acq On : 30 Apr 2019 21:32
Operator : JC/SP
Sample : K2593-17 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU043019\
Data File : VU031650.D
Acq On : 30 Apr 2019 21:32
Operator : JC/SP
Sample : K2593-17 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc