

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
 Data File : VU031652.D
 Acq On : 30 Apr 2019 22:19
 Operator : JC/SP
 Sample : K2593-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rBV	14046	11965	0.02%	0.016%
2	1.396	87	95	107	rBV	441968	492593	0.95%	0.646%
3	1.679	175	183	194	rBV	348204	439839	0.85%	0.577%
4	1.878	237	245	259	rVB	231160	325583	0.63%	0.427%
5	2.267	355	366	380	rVB	748532	1136330	2.19%	1.490%
6	2.434	416	418	421	rBV3	1466	905	0.00%	0.001%
7	2.463	425	427	431	rVB4	1633	908	0.00%	0.001%
8	2.486	431	434	437	rBV2	1760	1271	0.00%	0.002%
9	2.601	465	470	475	rBV3	1930	1834	0.00%	0.002%
10	2.701	489	501	508	rBV4	11141	19201	0.04%	0.025%
11	2.785	524	527	529	rBV3	940	743	0.00%	0.001%
12	2.823	536	539	543	rVB3	1162	812	0.00%	0.001%
13	2.852	543	548	551	rBV4	1662	1649	0.00%	0.002%
14	2.929	566	572	574	rBV3	1198	1082	0.00%	0.001%
15	2.981	583	588	591	rBV3	2680	2240	0.00%	0.003%
16	3.093	618	623	627	rBV6	1100	1100	0.00%	0.001%
17	3.180	646	650	653	rBV	2049	1899	0.00%	0.002%
18	3.225	661	664	667	rVB3	1772	1146	0.00%	0.002%
19	3.357	701	705	711	rVB3	1187	1309	0.00%	0.002%
20	3.428	722	727	731	rVB4	1259	1279	0.00%	0.002%
21	3.447	731	733	736	rVB3	1438	842	0.00%	0.001%
22	3.476	736	742	743	rBV3	1377	1017	0.00%	0.001%
23	3.521	752	756	763	rVB4	1251	1466	0.00%	0.002%
24	3.582	773	775	783	rVB4	1186	1237	0.00%	0.002%
25	3.614	783	785	789	rBV2	1266	1133	0.00%	0.001%
26	3.640	789	793	798	rVB5	1614	1532	0.00%	0.002%
27	3.666	798	801	805	rVB2	1624	1142	0.00%	0.001%
28	3.691	805	809	812	rBV	1365	1315	0.00%	0.002%
29	3.894	869	872	878	rVB4	977	1015	0.00%	0.001%
30	3.929	878	883	886	rBV2	1405	1460	0.00%	0.002%
31	3.990	899	902	907	rBV2	1070	1077	0.00%	0.001%
32	4.190	951	964	996	rBV2	261109	880290	1.69%	1.154%
33	4.640	1088	1104	1134	rBV	528163	1264603	2.43%	1.658%
34	4.887	1173	1181	1182	rBV5	2246	2439	0.00%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
 Data File : VU031652.D
 Acq On : 30 Apr 2019 22:19
 Operator : JC/SP
 Sample : K2593-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.990	1210	1213	1218	rBV8	1318	1082	0.00%	0.001%
36	5.122	1249	1254	1257	rBV4	2754	3023	0.01%	0.004%
37	5.209	1276	1281	1284	rVB4	1082	867	0.00%	0.001%
38	5.334	1296	1320	1351	rBV2	1074484	3220611	6.20%	4.222%
39	5.675	1422	1426	1429	rBV2	2113	1511	0.00%	0.002%
40	5.691	1429	1431	1436	rVB3	1450	983	0.00%	0.001%
41	5.756	1446	1451	1455	rBV6	958	1139	0.00%	0.001%
42	5.881	1477	1490	1517	rBV	890144	1816979	3.50%	2.382%
43	6.183	1565	1584	1617	rBV	26883394	51985909	100.00%	68.158%
44	6.325	1619	1628	1663	rVB	773942	1710002	3.29%	2.242%
45	6.739	1754	1757	1760	rBV4	1655	1084	0.00%	0.001%
46	6.926	1809	1815	1820	rBV8	1995	2443	0.00%	0.003%
47	7.128	1873	1878	1880	rBV3	1349	1289	0.00%	0.002%
48	7.164	1884	1889	1891	rBV4	1062	1043	0.00%	0.001%
49	7.225	1896	1908	1933	rBV	359586	670604	1.29%	0.879%
50	7.376	1953	1955	1960	rVB4	1212	761	0.00%	0.001%
51	7.563	2000	2013	2028	rBV	1233581	2207673	4.25%	2.894%
52	7.849	2092	2102	2130	rBV	231394	424510	0.82%	0.557%
53	8.074	2162	2172	2181	rBV10	4035	7716	0.01%	0.010%
54	8.145	2191	2194	2197	rVB3	1922	1298	0.00%	0.002%
55	8.161	2197	2199	2202	rBV2	1024	801	0.00%	0.001%
56	8.225	2206	2219	2236	rBV	469456	830337	1.60%	1.089%
57	8.315	2236	2247	2288	rVB2	880614	1820171	3.50%	2.386%
58	8.675	2356	2359	2362	rVB3	1981	1316	0.00%	0.002%
59	8.743	2378	2380	2383	rVB	1174	765	0.00%	0.001%
60	8.765	2383	2387	2389	rBV4	810	749	0.00%	0.001%
61	8.849	2410	2413	2419	rVB4	1615	1569	0.00%	0.002%
62	8.993	2451	2458	2462	rVB7	1935	2404	0.00%	0.003%
63	9.087	2474	2487	2509	rBV	1296014	2232319	4.29%	2.927%
64	9.334	2561	2564	2566	rBV4	1858	1310	0.00%	0.002%
65	9.376	2570	2577	2579	rBV3	10074	11617	0.02%	0.015%
66	9.427	2591	2593	2598	rVB5	1666	1294	0.00%	0.002%
67	9.505	2615	2617	2623	rVB5	915	760	0.00%	0.001%
68	9.530	2623	2625	2634	rVB7	1605	2273	0.00%	0.003%
69	9.620	2647	2653	2655	rBV2	1770	1665	0.00%	0.002%
70	9.736	2682	2689	2692	rBV5	2025	2221	0.00%	0.003%
71	9.755	2692	2695	2696	rVV3	1462	775	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
 Data File : VU031652.D
 Acq On : 30 Apr 2019 22:19
 Operator : JC/SP
 Sample : K2593-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.781	2697	2703	2713	rVB4	6693	10846	0.02%	0.014%
73	9.971	2760	2762	2767	rVV4	870	752	0.00%	0.001%
74	10.080	2792	2796	2799	rBV3	1307	1115	0.00%	0.001%
75	10.116	2804	2807	2809	rBV3	1091	763	0.00%	0.001%
76	10.161	2819	2821	2824	rBV2	1431	924	0.00%	0.001%
77	10.276	2855	2857	2864	rVB5	1188	940	0.00%	0.001%
78	10.431	2890	2905	2930	rBV	870332	1425540	2.74%	1.869%
79	10.685	2976	2984	2988	rBV8	3714	5076	0.01%	0.007%
80	10.919	3053	3057	3062	rVB2	1444	1100	0.00%	0.001%
81	10.945	3062	3065	3071	rBV5	2312	2907	0.01%	0.004%
82	10.977	3071	3075	3078	rBV4	1767	1549	0.00%	0.002%
83	11.154	3121	3130	3137	rBV6	6270	10043	0.02%	0.013%
84	11.218	3147	3150	3157	rBV3	2034	2144	0.00%	0.003%
85	11.283	3167	3170	3174	rBV2	874	857	0.00%	0.001%
86	11.341	3185	3188	3198	rVB7	1561	2254	0.00%	0.003%
87	11.386	3198	3202	3207	rBV3	928	895	0.00%	0.001%
88	11.482	3215	3232	3252	rBV	986677	1596461	3.07%	2.093%
89	11.855	3336	3348	3370	rBV	982772	1618212	3.11%	2.122%
90	12.173	3445	3447	3452	rVB4	1920	1139	0.00%	0.001%
91	12.241	3465	3468	3470	rBV3	1255	908	0.00%	0.001%
92	12.440	3527	3530	3533	rBV3	1795	1289	0.00%	0.002%
93	12.755	3626	3628	3630	rBV	1281	832	0.00%	0.001%
94	12.829	3648	3651	3657	rBV5	1617	1549	0.00%	0.002%
95	12.890	3664	3670	3673	rBV5	1523	1564	0.00%	0.002%
96	13.331	3804	3807	3810	rBV	1470	743	0.00%	0.001%
97	13.440	3839	3841	3847	rVB4	2242	1700	0.00%	0.002%
98	14.051	4028	4031	4035	rBV5	1257	1093	0.00%	0.001%
99	14.176	4067	4070	4074	rBV3	1878	1659	0.00%	0.002%
100	14.205	4077	4079	4082	rBV2	1410	956	0.00%	0.001%


Sum of corrected areas: 76272939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
Data File : VU031652.D
Acq On : 30 Apr 2019 22:19
Operator : JC/SP
Sample : K2593-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

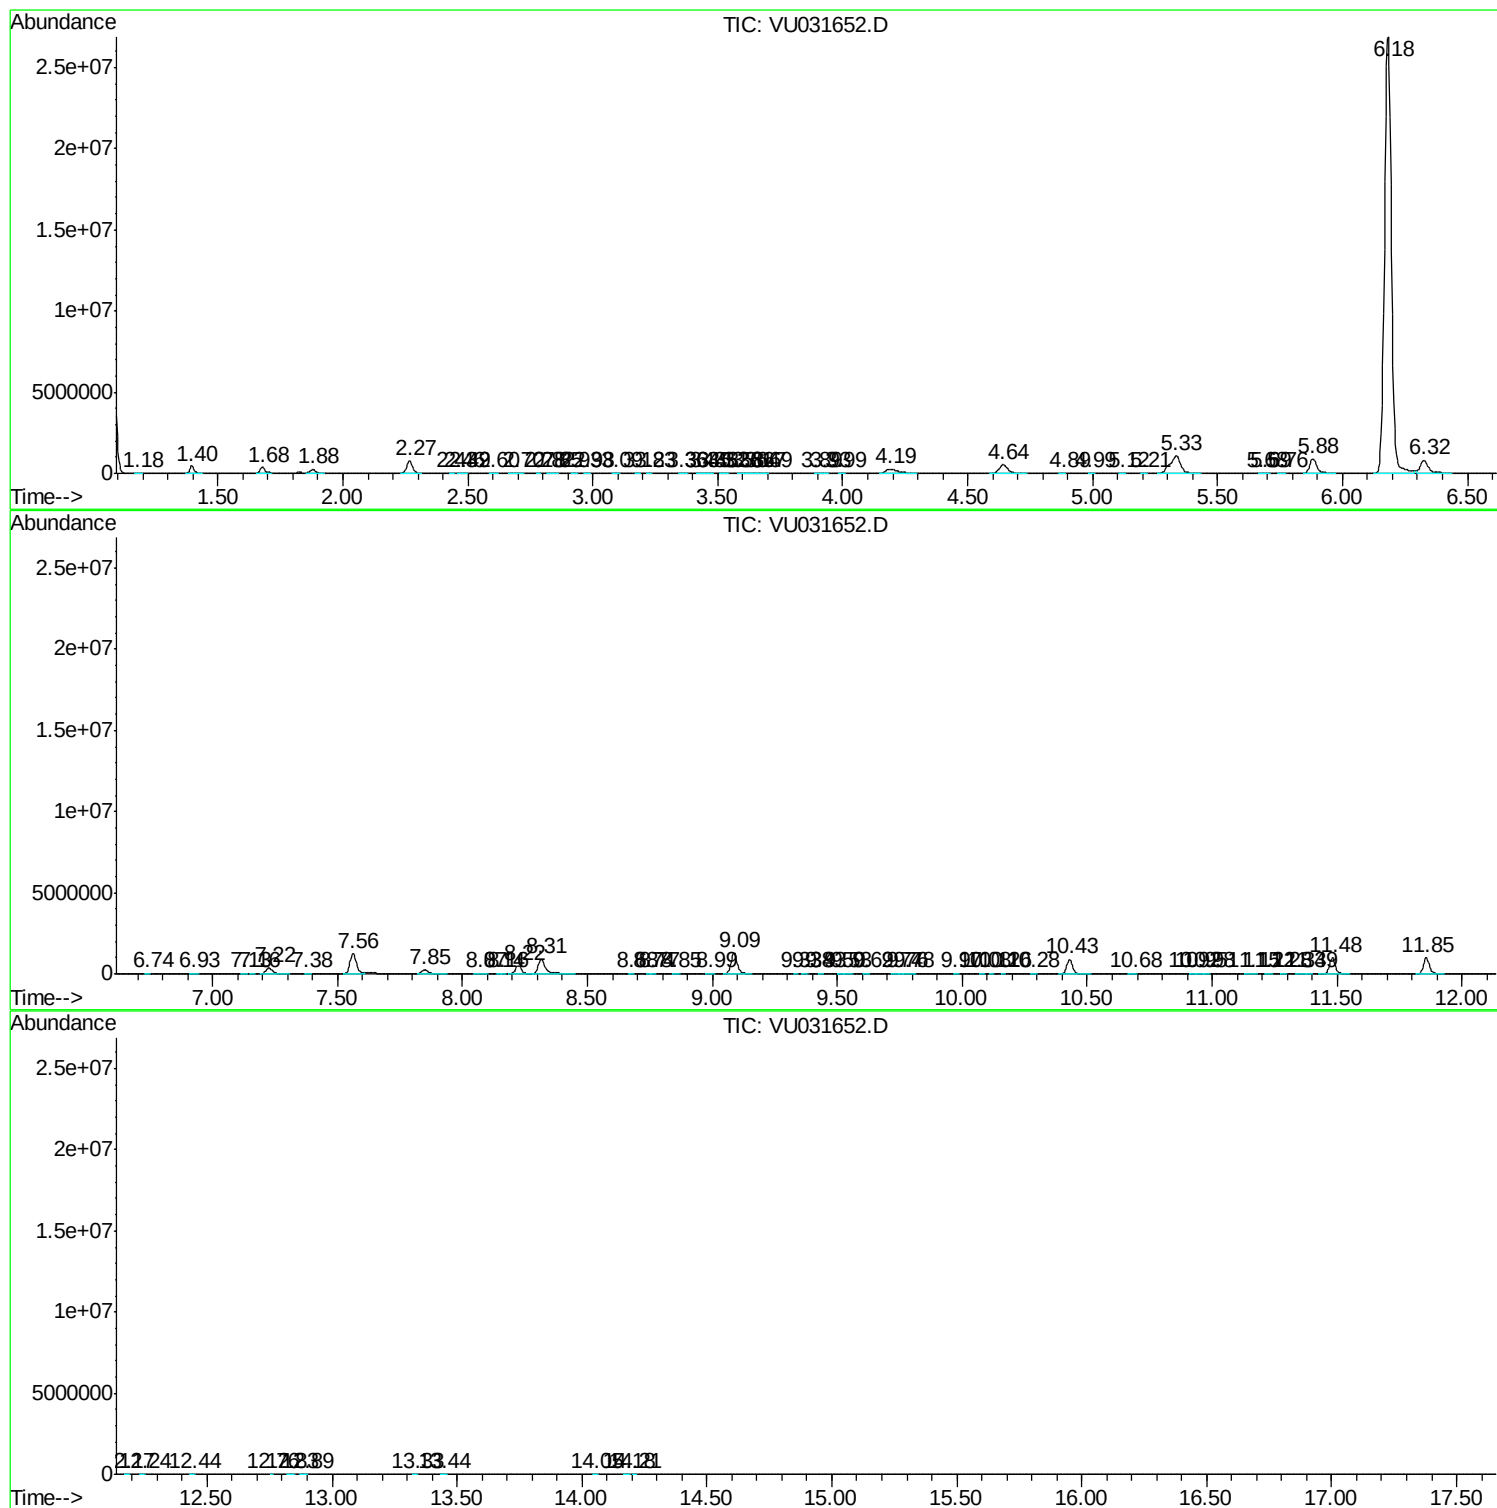

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
Data File : VU031652.D
Acq On : 30 Apr 2019 22:19
Operator : JC/SP
Sample : K2593-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
Data File : VU031652.D
Acq On : 30 Apr 2019 22:19
Operator : JC/SP
Sample : K2593-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc