


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043019\
 Data File : VU031624.D
 Acq On : 30 Apr 2019 11:11
 Operator : JC/SP
 Sample : BFB34
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Wed May 01 04:42:38 2019

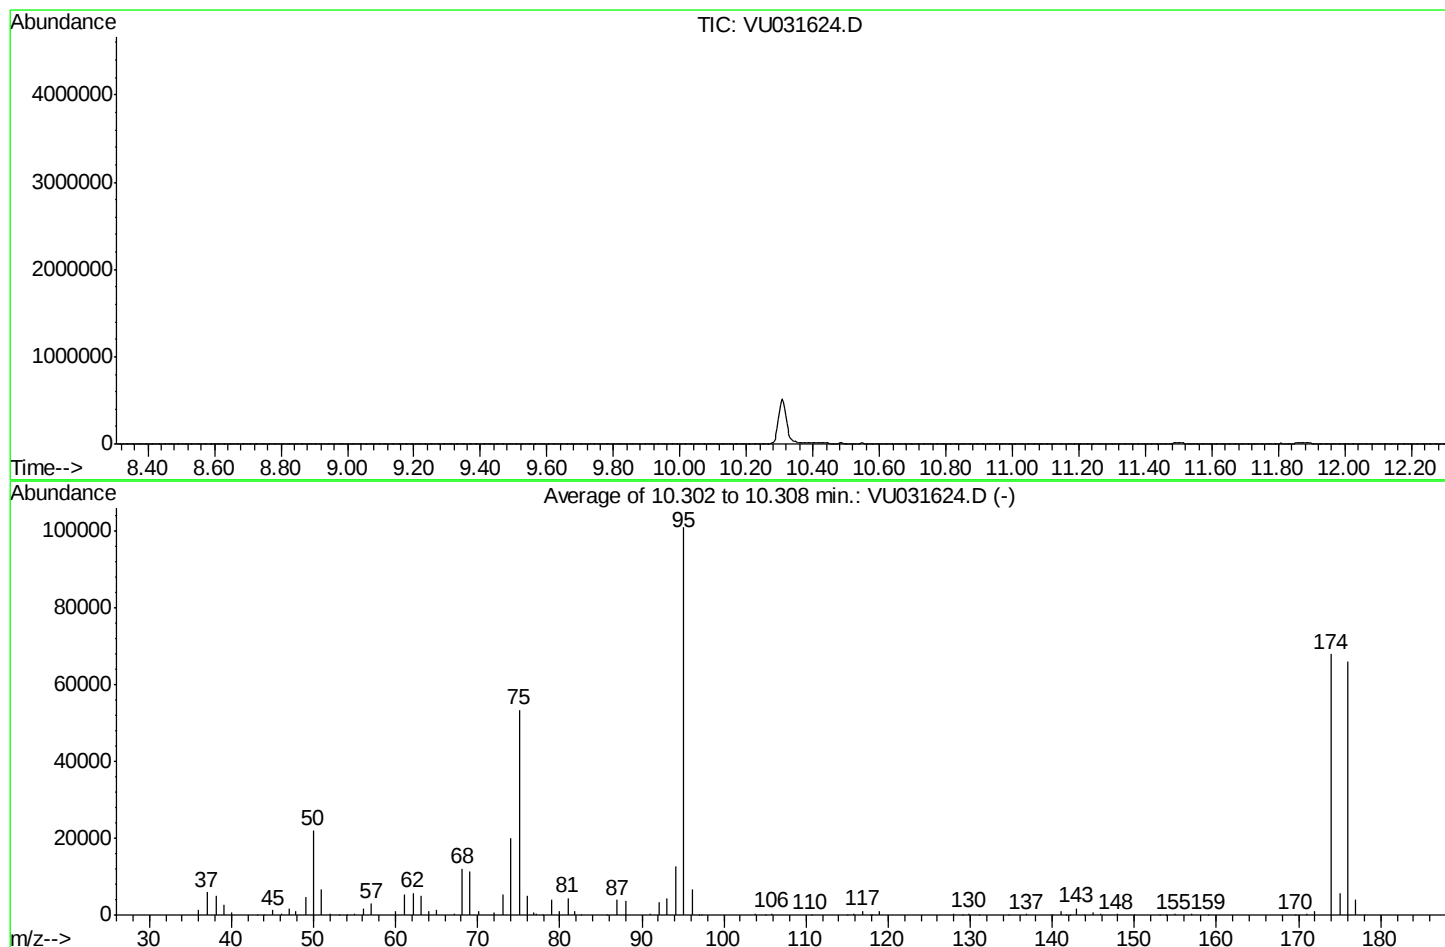

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	21837	PASS
75	95	30	80	53.0	53421	PASS
95	95	100	100	100.0	100869	PASS
96	95	5	9	6.6	6682	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.2	67818	PASS
175	174	5	9	8.3	5602	PASS
176	174	95	101	97.1	65885	PASS
177	176	5	9	5.9	3881	PASS

Scan 2854 (10.266 min): VU031624.D
BFB34

m/z	Abundance
40.00	3934.0
44.00	1608.0
207.20	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
35.90	1119.0
37.00	5686.0
38.10	4208.0
39.10	2636.0
40.00	4345.0
44.00	1771.0
45.10	1024.0
46.00	185.0
47.10	1572.0
47.90	1032.0
49.00	4733.0
50.00	20536.0
51.00	6391.0
52.00	306.0
54.10	108.0
55.00	236.0
56.10	1443.0
57.10	2693.0
60.10	935.0
61.00	5466.0
62.10	5482.0
63.10	4648.0
64.00	973.0
65.10	1500.0
67.10	487.0
68.10	11039.0
69.00	10238.0
70.10	1134.0
71.90	708.0
73.00	5161.0
74.10	18888.0
75.10	49824.0
76.00	4635.0
77.20	546.0
79.00	3429.0
79.90	775.0
81.00	3697.0
81.80	975.0
85.70	120.0
87.00	3663.0
88.00	3451.0
91.00	464.0
92.10	2945.0
93.00	3868.0
94.10	11891.0
95.10	94752.0
96.10	6376.0
96.90	208.0
103.90	251.0
105.00	138.0
105.90	382.0
115.10	100.0
115.90	393.0
116.90	1050.0
117.80	239.0
119.00	974.0
127.90	414.0
129.90	533.0
131.00	135.0
134.70	112.0
136.80	223.0
141.00	890.0
143.00	1634.0
145.00	645.0
146.00	188.0
147.90	230.0
149.90	121.0
154.90	275.0
157.00	164.0
159.00	109.0
170.90	223.0
172.00	879.0
174.00	61840.0
175.10	5054.0
176.00	58968.0
177.00	3556.0
178.00	134.0
207.00	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	1200.0
37.00	6181.0
38.10	5064.0
39.10	2818.0
40.00	4709.0
44.00	1602.0
45.00	1268.0
46.10	211.0
47.10	1828.0
47.90	1275.0
49.00	4819.0
50.00	22464.0
51.00	7041.0
52.00	288.0
54.10	132.0
54.90	248.0
56.00	1602.0
57.10	3031.0
60.00	1121.0
61.00	5315.0
62.10	6119.0
63.00	5113.0
64.10	1110.0
65.00	1465.0
67.10	473.0
68.10	12529.0
69.00	11910.0
70.00	948.0
71.90	701.0
73.10	5564.0
74.10	20432.0
75.10	54920.0
76.10	5196.0
76.90	680.0
79.00	3934.0
80.00	1019.0
81.00	4611.0
81.80	1019.0
82.60	180.0
87.00	3910.0
88.00	3852.0
91.00	528.0
92.10	3322.0
93.00	4296.0
94.10	12670.0
95.10	103944.0
96.10	6850.0
96.90	159.0
97.30	107.0
103.80	329.0
105.00	190.0
105.90	497.0
110.60	126.0
115.90	480.0
117.00	1089.0
118.00	217.0
118.90	1004.0
127.90	413.0
129.90	461.0
131.00	150.0
136.90	207.0
141.00	1050.0
141.70	115.0
142.20	124.0
143.00	1794.0
145.00	809.0
146.00	266.0
147.90	373.0
153.10	103.0
154.90	339.0
157.00	263.0
169.60	114.0
170.90	307.0
172.00	1060.0
174.00	69816.0
175.10	5714.0
176.00	67920.0
177.00	3972.0
178.00	165.0
207.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.10	1283.0
37.00	6115.0
38.10	5518.0
39.00	2818.0
40.00	4957.0
43.10	123.0
44.00	1499.0
45.00	1402.0
46.10	250.0
47.10	1808.0
47.90	1107.0
49.10	4552.0
50.00	22512.0
51.00	6821.0
52.10	218.0
53.10	130.0
54.00	120.0
55.00	307.0
56.00	1606.0
57.00	2948.0
60.00	1225.0
61.00	4922.0
62.10	5832.0
63.00	5298.0
64.10	1246.0
65.00	1306.0
67.10	391.0
68.10	12558.0
69.00	11815.0
70.00	720.0
72.00	700.0
73.10	5432.0
74.00	20328.0
75.10	55520.0
76.10	5297.0
76.90	875.0
77.90	323.0
79.00	4276.0
80.00	1262.0
81.00	4880.0
81.90	964.0
82.70	215.0
87.00	3975.0
88.00	4000.0
90.80	528.0
92.10	3290.0
93.00	4551.0
94.10	13195.0
95.10	103912.0
96.10	6822.0
96.90	105.0
103.80	376.0
105.00	190.0
105.90	551.0
110.60	161.0
115.80	502.0
117.00	934.0
118.00	322.0
118.90	868.0
127.90	362.0
129.00	103.0
129.90	380.0
131.10	120.0
137.00	222.0
140.00	136.0
141.00	966.0
141.70	134.0
143.00	1844.0
143.80	107.0
145.00	964.0
145.90	316.0
147.90	322.0
153.10	157.0
153.90	158.0
154.90	363.0
156.90	282.0
169.70	183.0
171.00	312.0
172.00	1073.0
174.00	71800.0
175.10	6040.0
176.00	70768.0
177.00	4117.0
178.00	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34