
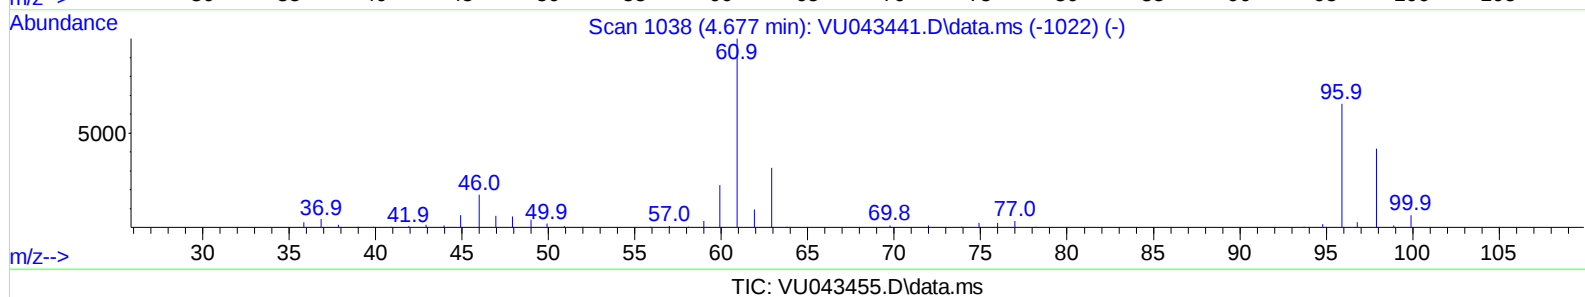
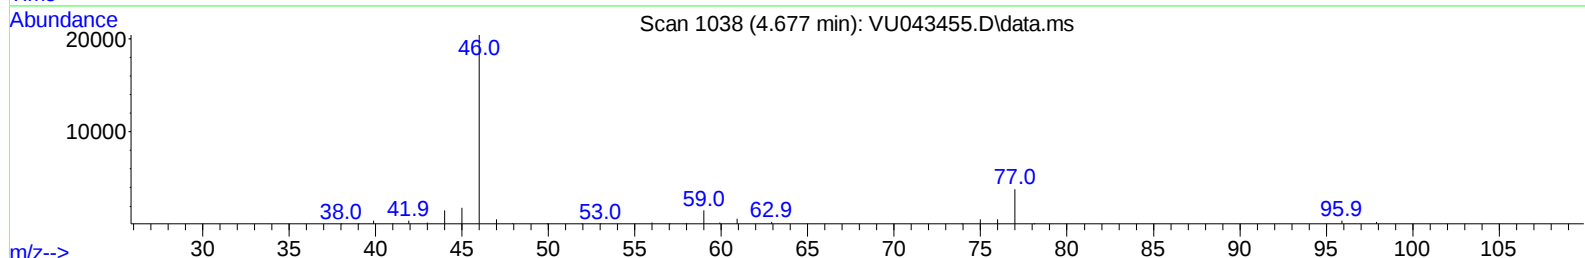


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
 Data File : VU043455.D
 Acq On : 30 Apr 2021 03:43
 Operator : SY/MD
 Sample : M2194-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Quant Time: May 03 08:10:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 30 08:34:29 2021
 Response via : Initial Calibration

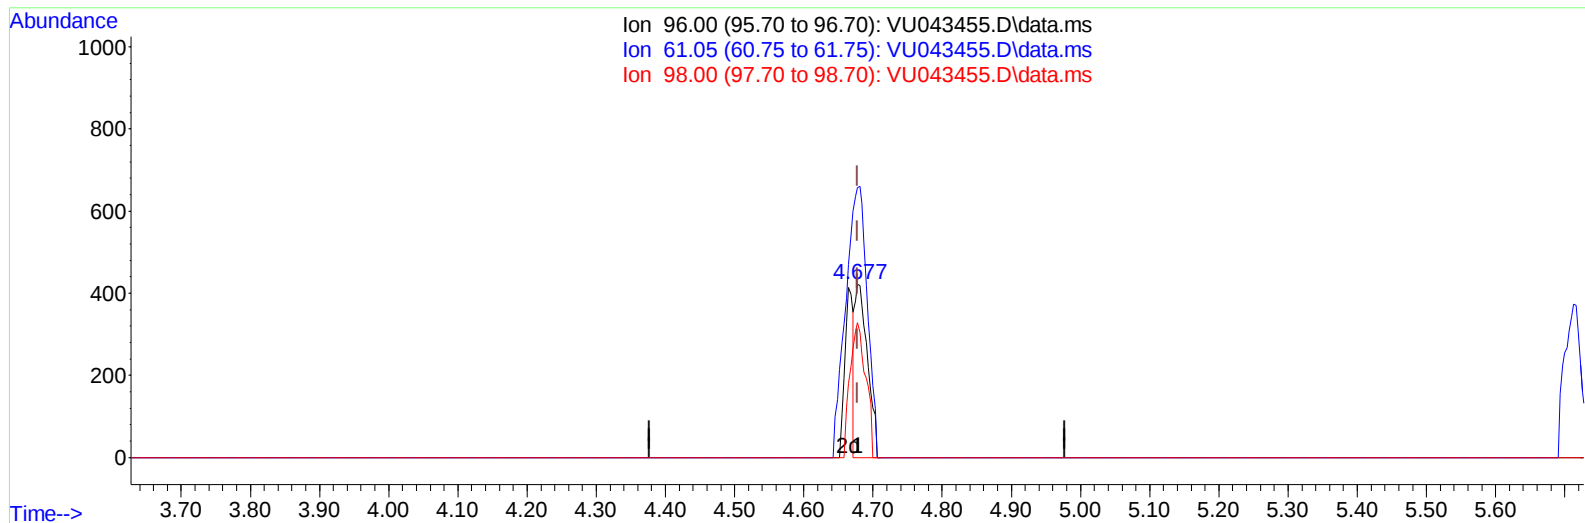

(22) cis-1,2-Dichloroethene (T)

4.677min (+ 0.000) 0.09 ug/L

response 539

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	124.90	155.69
98.00	68.10	77.73
0.00	0.00	0.00