

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
 Data File : VU043458.D
 Acq On : 30 Apr 2021 04:55
 Operator : SY/MD
 Sample : M2194-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YARR3

Quant Time: Apr 30 08:37:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 30 08:34:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	86831	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	88899	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	39856	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	18753	4.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.00%
7) Chloroethane-d5	1.919	69	19142	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.00%
11) 1,1-Dichloroethene-d2	2.575	65	11829	4.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.60%
20) 2-Butanone-d5	4.645	46	111922	57.79	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.58%
24) Chloroform-d	5.073	84	56304	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.710	65	36150	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.735	84	96556	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.700	67	35495	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.906	98	80775	3.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.00%
43) trans-1,3-Dichloroprop...	8.185	79	11537	3.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.20%
46) 2-Hexanone-d5	8.642	63	65584	43.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.76%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	29682	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.40%
66) 1,2-Dichlorobenzene-d4	12.201	152	31749	4.65	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.00%
Target Compounds						
33) Benzene	5.784	78	1488	0.06	ug/L	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
Data File : VU043458.D
Acq On : 30 Apr 2021 04:55
Operator : SY/MD
Sample : M2194-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YARR3

Quant Time: Apr 30 08:37:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 30 08:34:29 2021
Response via : Initial Calibration

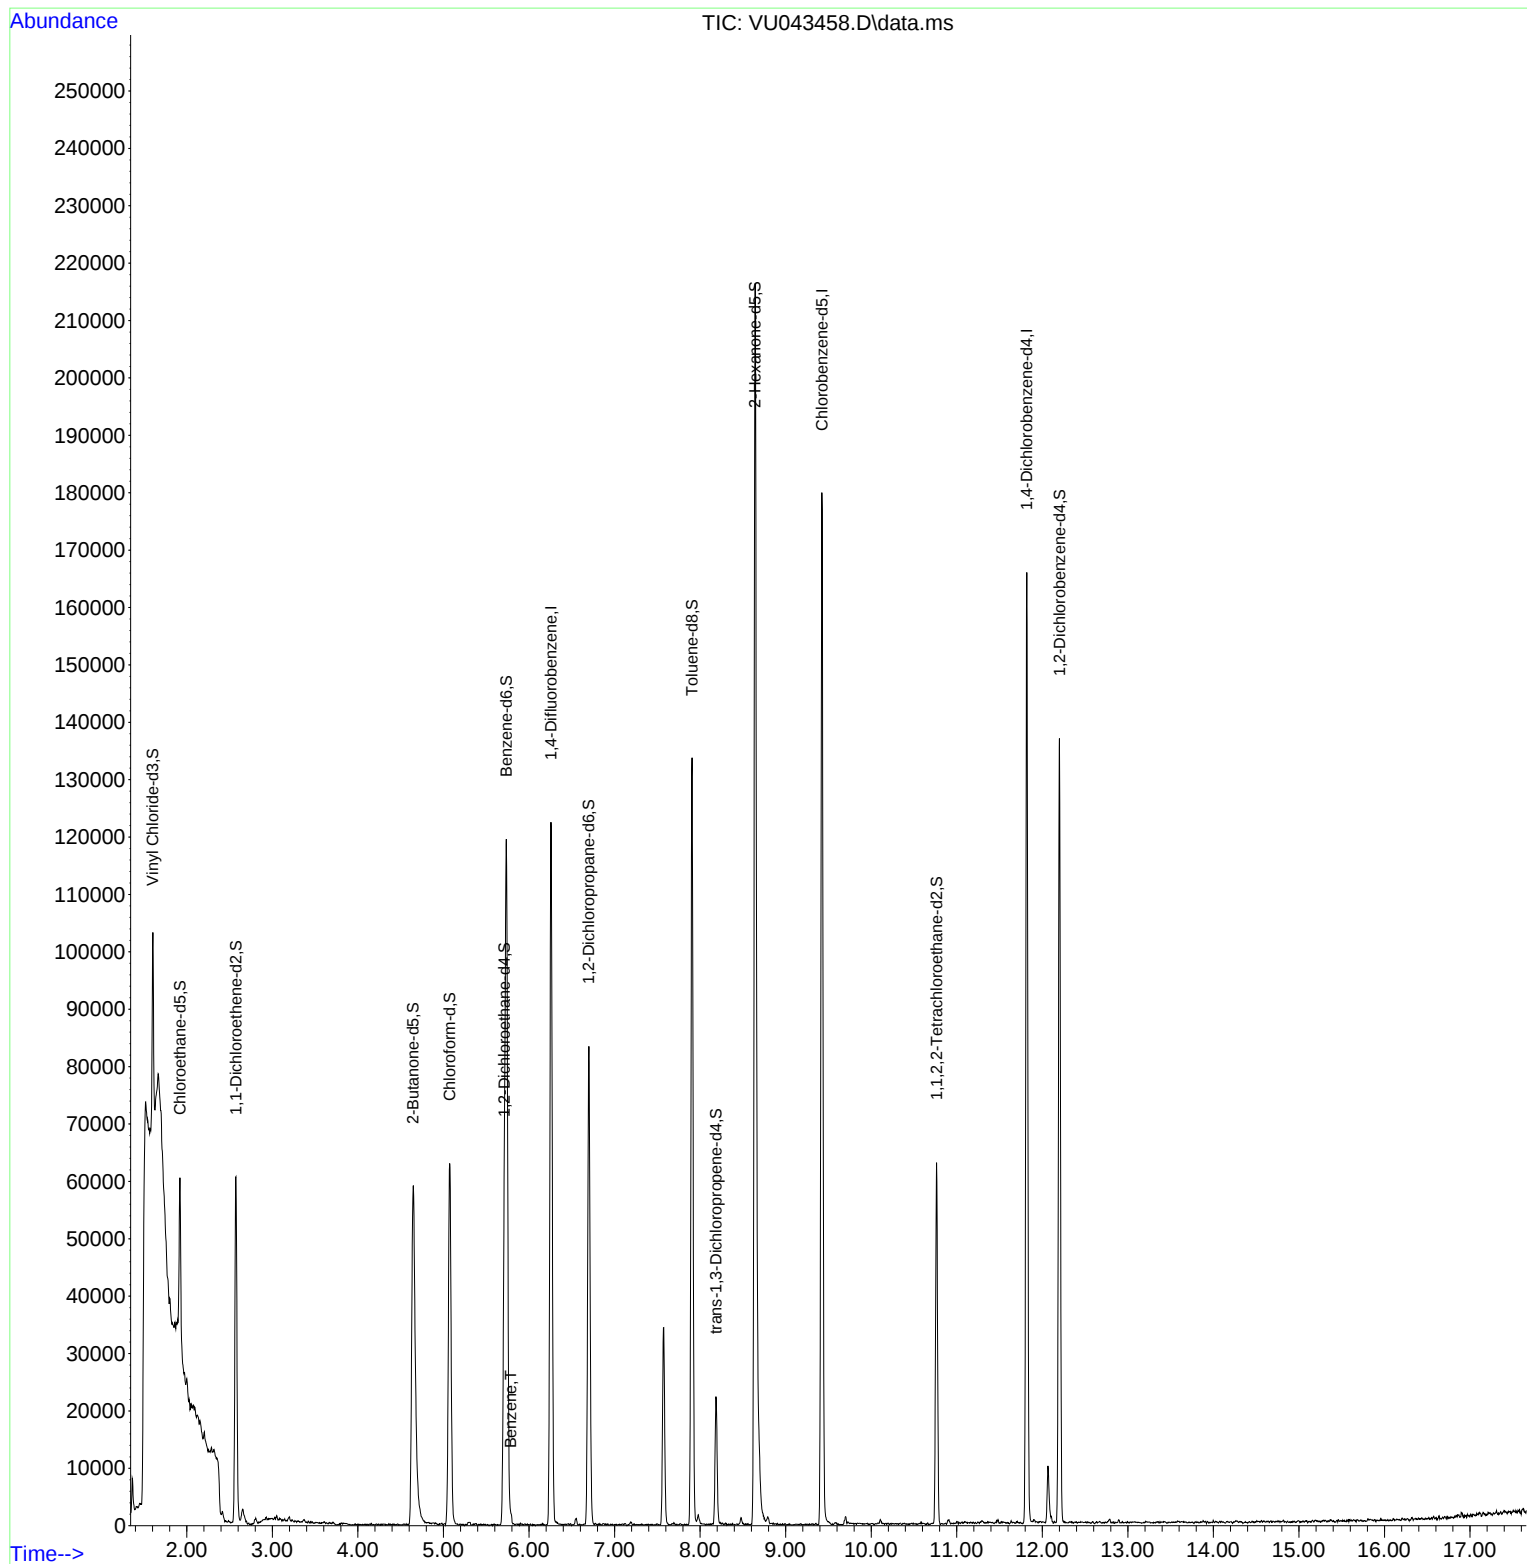

Abundance Scan 1382 (5.783 min): VU043441.D\data.ms (-1) #33

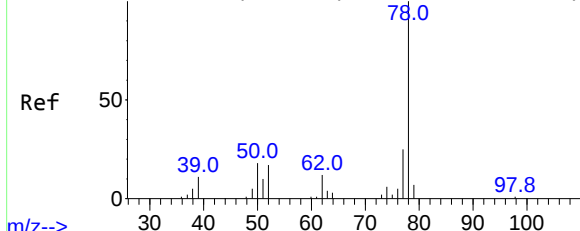


Benzene
Concen: 0.06 ug/L
RT: 5.784 min Scan# 1382
Delta R.T. 0.000 min
Lab File: VU043458.D
Acq: 30 Apr 2021 04:55

Instrument :
MSVOA_U
ClientSampleId :
YARR3

Tgt Ion: 78 Resp: 1488

Abundance Scan 1382 (5.784 min): VU043458.D\data.ms

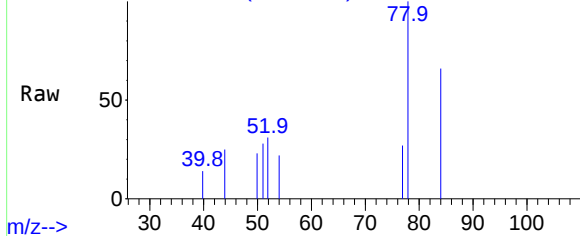

Abundance Scan 1382 (5.784 min): VU043458.D\data.ms (-1)

