

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
 Data File : VU043459.D
 Acq On : 30 Apr 2021 05:19
 Operator : SY/MD
 Sample : M2194-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YARR4

Quant Time: Apr 30 08:37:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 30 08:34:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	85196	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	86996	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	39458	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	19347	4.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.40%
7) Chloroethane-d5	1.919	69	19730	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.572	65	11884	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.80%
20) 2-Butanone-d5	4.642	46	113269	59.61	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.22%
24) Chloroform-d	5.073	84	55424	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.710	65	35705	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.735	84	96401	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
36) 1,2-Dichloropropane-d6	6.700	67	36017	5.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.20%
41) Toluene-d8	7.906	98	79309	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.40%
43) trans-1,3-Dichloroprop...	8.185	79	11062	3.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.60%
46) 2-Hexanone-d5	8.642	63	66367	44.86	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.72%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	29538	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
66) 1,2-Dichlorobenzene-d4	12.198	152	32373	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%
Target Compounds						
					Qvalue	
13) Acetone	2.652	43	2531	1.81	ug/L	81
33) Benzene	5.784	78	1496	0.06	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
Data File : VU043459.D
Acq On : 30 Apr 2021 05:19
Operator : SY/MD
Sample : M2194-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YARR4

Quant Time: Apr 30 08:37:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 30 08:34:29 2021
Response via : Initial Calibration




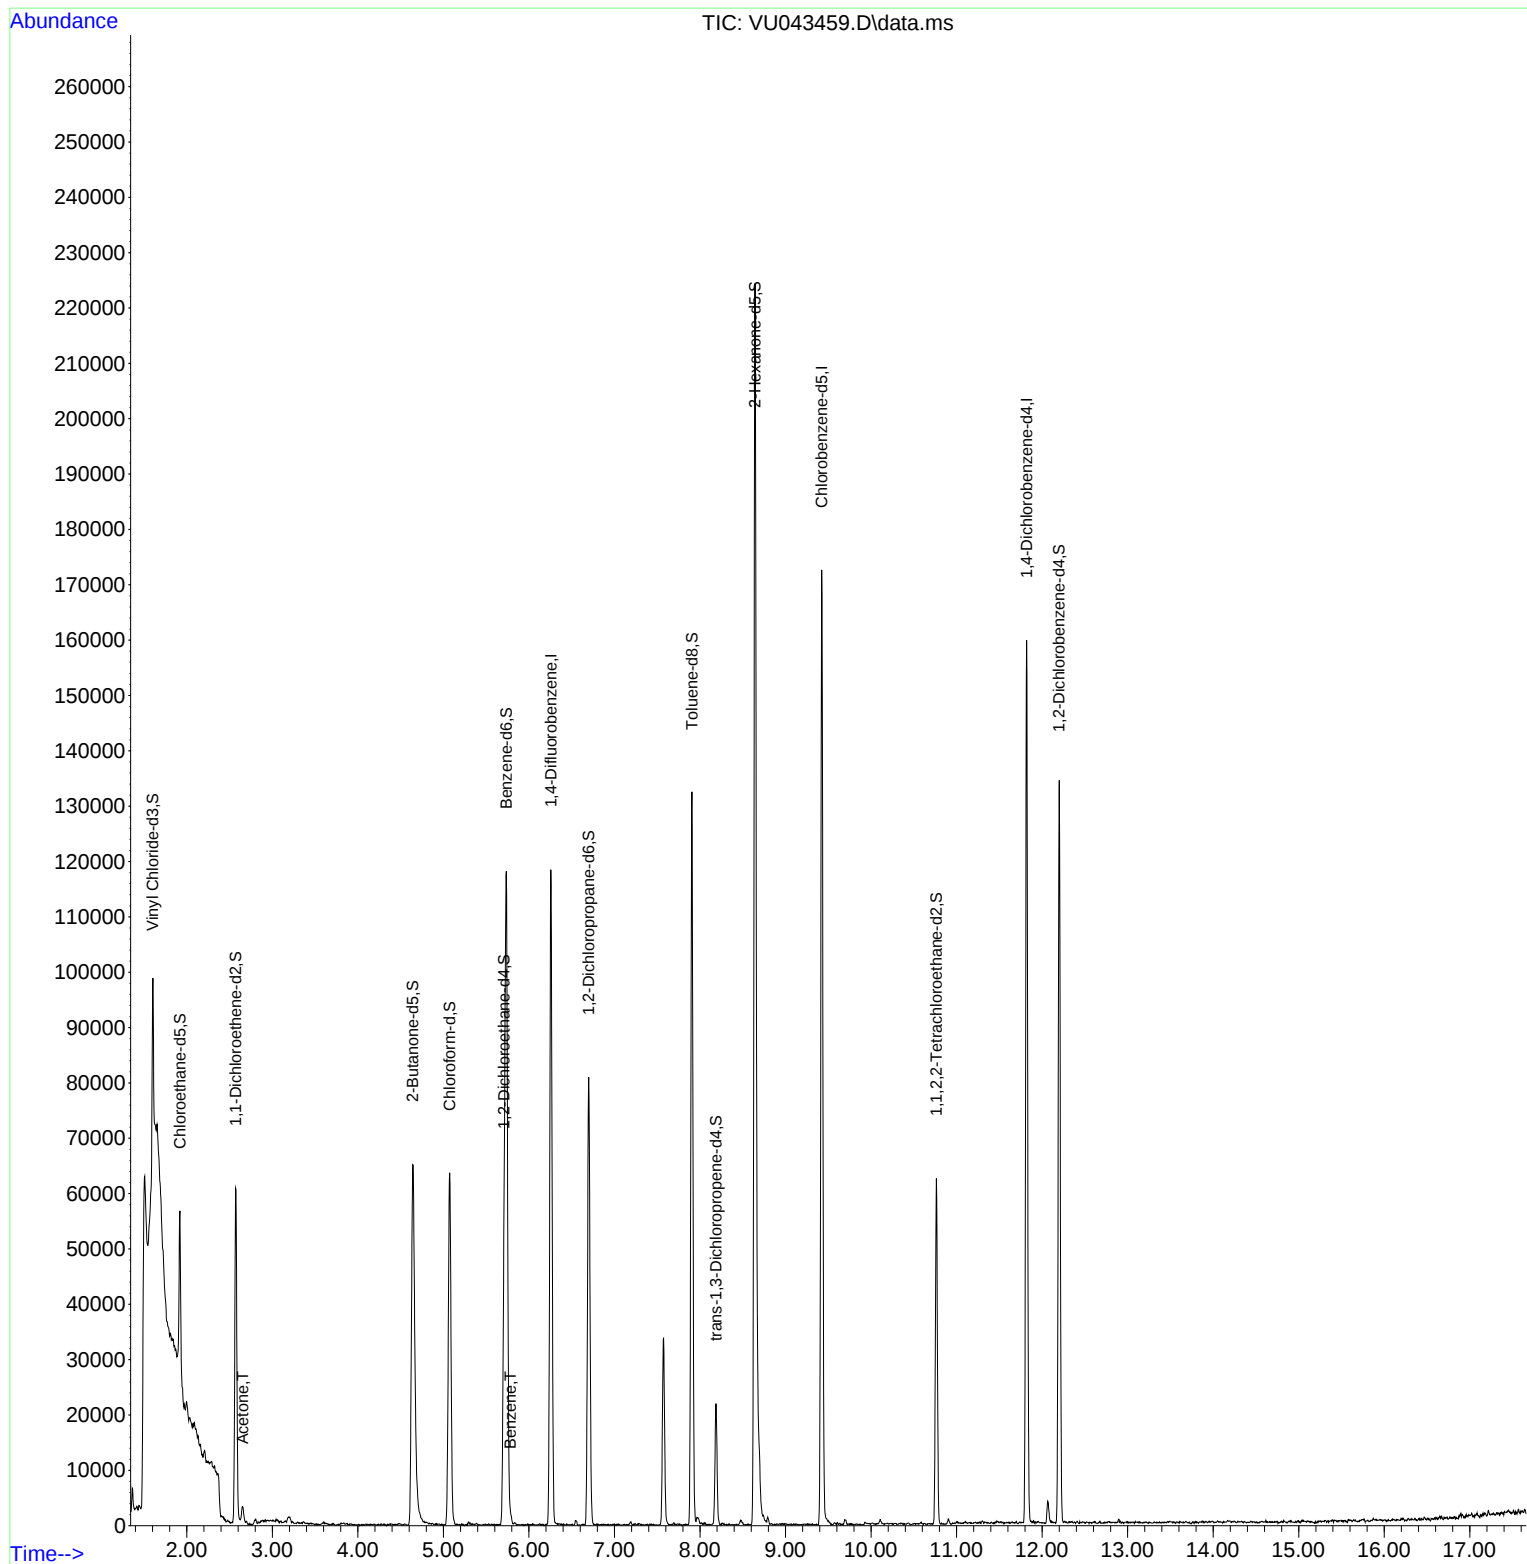


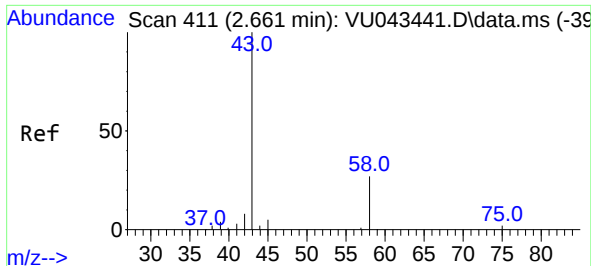

#13
Acetone
Concen: 1.81 ug/L
RT: 2.652 min Scan# 408
Delta R.T. -0.010 min
Lab File: VU043459.D
Acq: 30 Apr 2021 05:19

Instrument :
MSVOA_U
ClientSampleId :
YARR4

Tgt Ion: 43 Resp: 2531
Ion Ratio Lower Upper
43 100
58 19.8 0.0 25.0

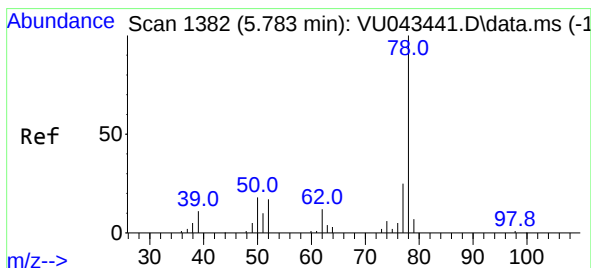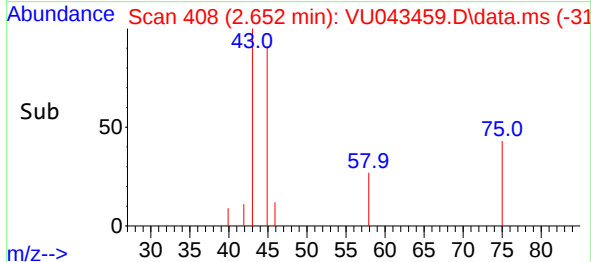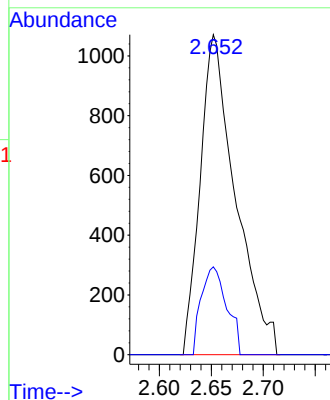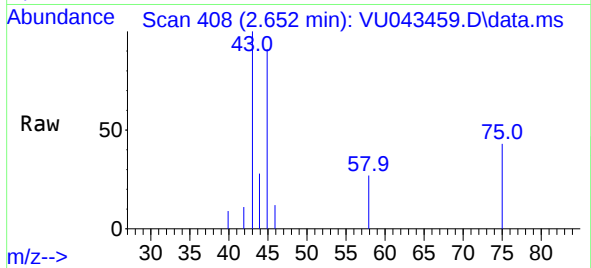

#33
Benzene
Concen: 0.06 ug/L
RT: 5.784 min Scan# 1382
Delta R.T. 0.000 min
Lab File: VU043459.D
Acq: 30 Apr 2021 05:19

Tgt Ion: 78 Resp: 1496

