


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
 Data File : VU043418.D
 Acq On : 29 Apr 2021 11:48
 Operator : SY/MD
 Sample : BFB38
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB138

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Apr 30 08:34:29 2021

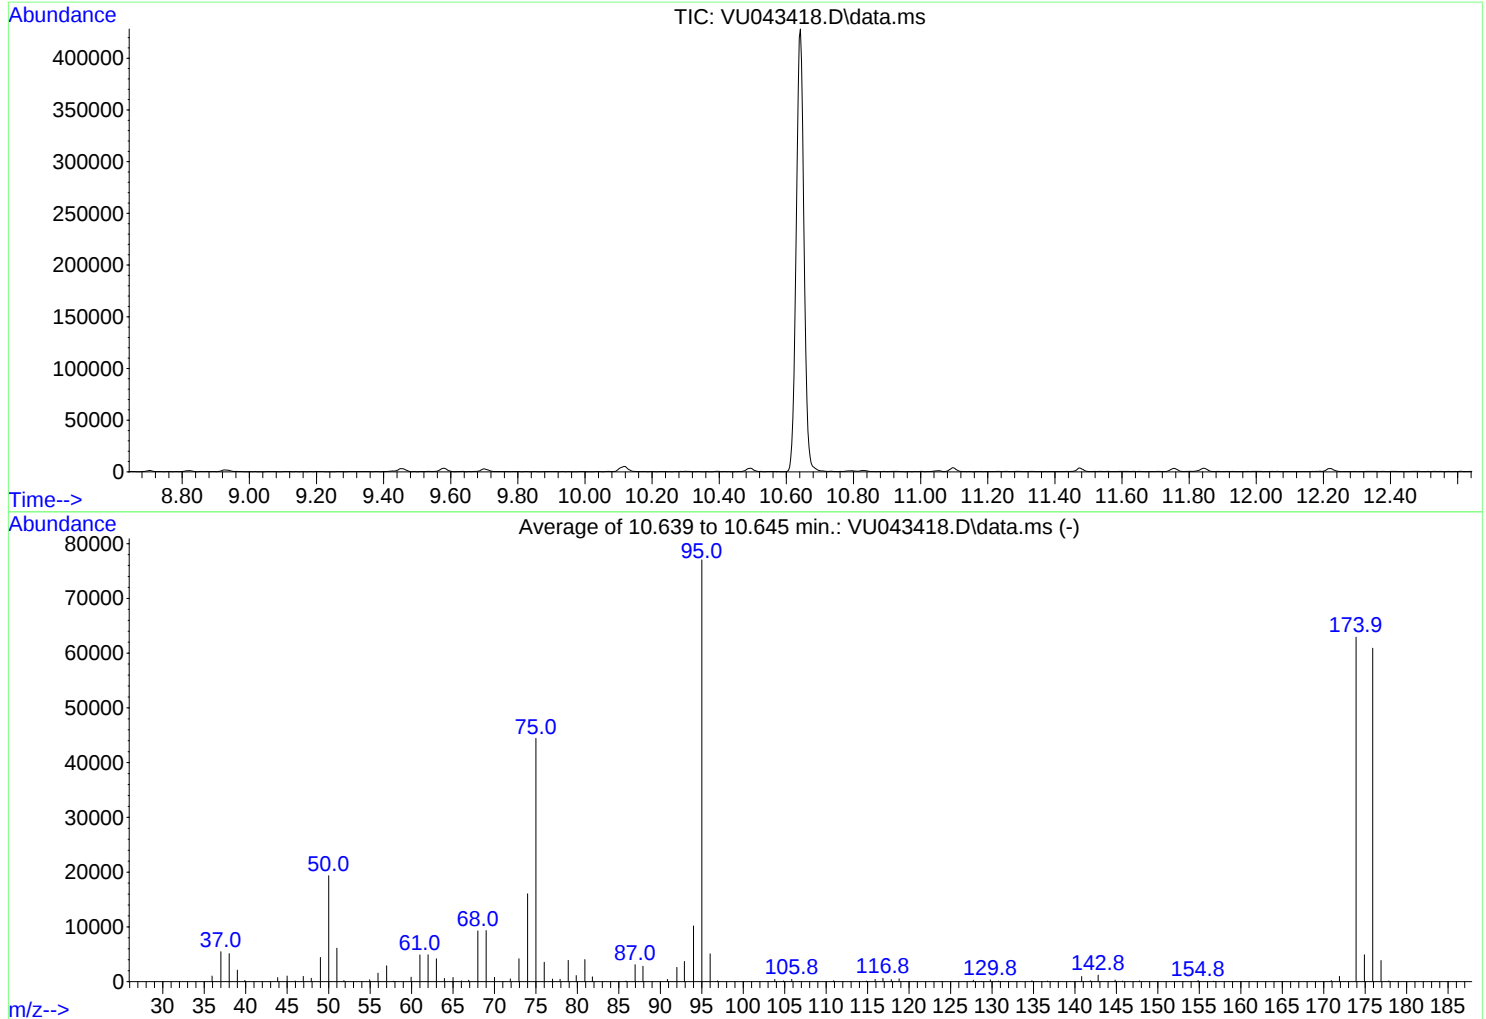

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	19339	PASS
75	95	30	80	57.6	44408	PASS
95	95	100	100	100.0	77040	PASS
96	95	5	9	6.6	5085	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.7	62928	PASS
175	174	5	9	7.8	4909	PASS
176	174	95	101	96.8	60915	PASS
177	176	5	9	6.3	3859	PASS

m/z	Abundance
43.80	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138

m/z	Abundance
35.90	1003.0
37.00	5168.0
38.00	4859.0
39.00	1981.0
39.90	195.0
43.90	849.0
45.00	991.0
46.00	122.0
46.90	916.0
47.90	592.0
49.00	4037.0
50.00	18216.0
51.00	5865.0
51.80	195.0
54.90	313.0
56.00	1471.0
57.00	2769.0
58.00	122.0
60.00	773.0
61.00	4528.0
62.00	4628.0
63.00	3893.0
63.90	603.0
65.00	689.0
66.00	149.0
66.90	256.0
68.00	8788.0
69.00	9024.0
70.00	716.0
71.90	455.0
72.90	4077.0
74.00	14964.0
75.00	42248.0
76.00	3296.0
77.00	415.0
77.90	433.0
78.90	3699.0
79.90	1036.0
80.90	3761.0
81.80	857.0
85.80	116.0
86.90	2826.0
87.90	2693.0
90.90	312.0
92.00	2545.0
92.90	3370.0
94.00	9870.0
95.00	73472.0
96.00	4783.0
96.90	113.0
103.80	426.0
104.90	123.0
105.80	431.0
110.90	142.0
114.80	113.0
115.90	404.0
116.90	617.0
117.80	343.0
118.80	471.0
123.80	101.0
127.70	249.0
129.80	287.0
130.80	114.0
134.90	174.0
136.80	114.0
140.80	974.0
141.80	130.0
142.80	1137.0
144.90	282.0
145.80	127.0
147.80	170.0
154.90	212.0
156.90	167.0
170.90	189.0
171.90	891.0
173.90	61576.0
174.90	4645.0
175.90	59208.0
176.90	3602.0
177.80	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138

m/z	Abundance
35.90	1018.0
37.00	5587.0
38.00	5260.0
39.00	2137.0
39.90	246.0
43.90	987.0
45.00	1072.0
46.00	127.0
46.90	983.0
47.90	655.0
49.00	4576.0
50.00	19928.0
51.00	6305.0
51.90	222.0
55.00	375.0
56.00	1607.0
57.00	2946.0
57.80	130.0
60.00	854.0
61.00	5025.0
62.00	5041.0
63.00	4356.0
64.00	631.0
65.00	781.0
66.00	158.0
66.90	271.0
68.00	9640.0
69.00	9616.0
70.00	800.0
71.90	518.0
72.90	4349.0
74.00	16680.0
75.00	45648.0
76.00	3614.0
77.00	481.0
77.90	474.0
78.90	4047.0
79.80	1124.0
80.90	4145.0
81.80	906.0
85.80	128.0
87.00	3158.0
87.90	2872.0
90.80	422.0
92.00	2668.0
92.90	3786.0
94.00	10485.0
95.00	79560.0
96.00	5243.0
96.90	147.0
103.80	398.0
104.90	143.0
105.90	439.0
110.90	194.0
112.90	115.0
114.90	130.0
115.90	449.0
116.90	621.0
117.90	393.0
118.80	540.0
123.90	105.0
127.80	278.0
128.70	106.0
129.80	336.0
130.80	121.0
134.80	195.0
136.70	110.0
140.80	936.0
141.90	168.0
142.80	1244.0
144.80	305.0
145.80	129.0
147.80	161.0
154.90	234.0
156.70	155.0
170.90	224.0
171.90	995.0
173.90	64872.0
174.90	5054.0
175.90	63144.0
176.90	3983.0
177.90	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138

m/z	Abundance
36.00	1016.0
37.00	5642.0
38.00	5271.0
39.00	2186.0
39.90	261.0
42.80	107.0
43.90	1038.0
45.00	1038.0
45.90	117.0
47.00	976.0
47.90	639.0
49.00	4609.0
50.00	19872.0
51.00	6155.0
51.90	206.0
55.00	380.0
55.90	1592.0
57.00	2949.0
57.80	127.0
59.90	839.0
61.00	5074.0
62.00	5041.0
63.00	4296.0
64.00	572.0
65.00	806.0
66.00	137.0
66.90	266.0
68.00	9385.0
69.00	9340.0
70.00	813.0
71.90	520.0
73.00	4142.0
74.00	16496.0
75.00	45328.0
76.00	3715.0
77.00	489.0
77.90	436.0
78.90	3926.0
79.80	1143.0
80.90	4165.0
81.80	888.0
85.90	127.0
87.00	3279.0
87.90	2902.0
90.80	490.0
92.00	2570.0
92.90	3862.0
94.00	10146.0
95.00	78088.0
96.00	5230.0
96.90	176.0
103.80	363.0
104.80	142.0
105.90	409.0
106.80	116.0
110.90	220.0
114.90	108.0
115.90	427.0
116.80	640.0
117.90	416.0
118.80	548.0
127.80	294.0
128.80	116.0
129.80	321.0
130.80	104.0
134.70	172.0
136.60	116.0
140.80	862.0
141.90	200.0
142.80	1233.0
144.80	297.0
145.70	130.0
147.80	149.0
154.80	232.0
156.70	145.0
170.90	221.0
171.90	1021.0
173.90	62336.0
174.90	5029.0
175.90	60392.0
176.90	3991.0
177.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138