


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043021\
Data File : VU043463.D
Acq On : 30 Apr 2021 08:56
Operator : SY/MD
Sample : BFB39
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB139

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 30 08:34:29 2021

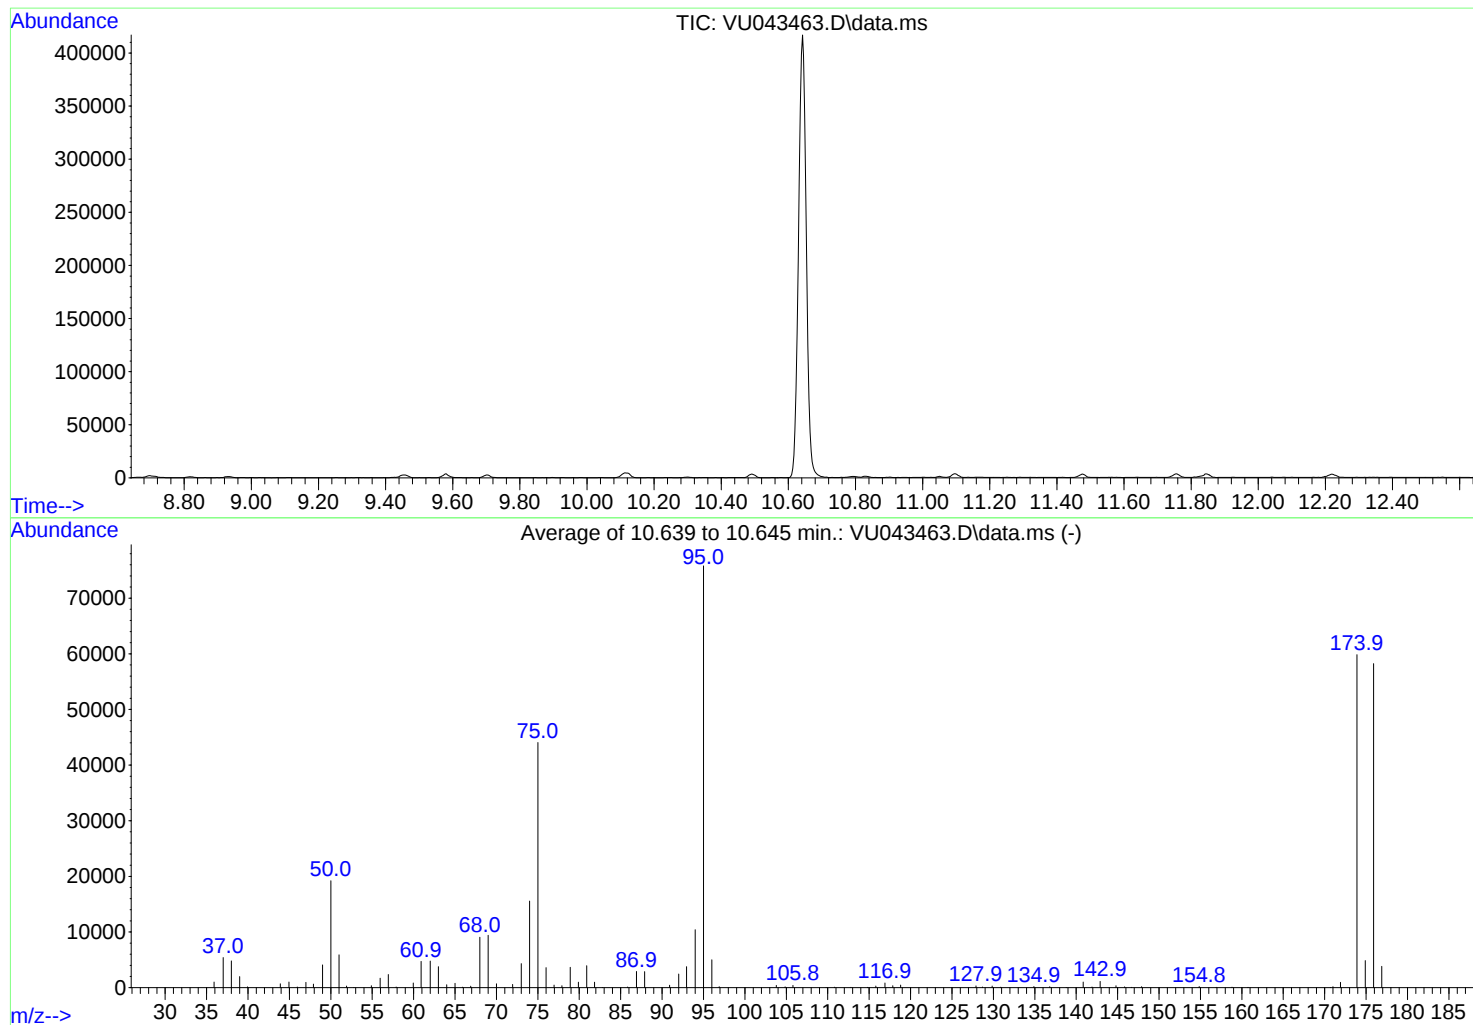

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.4	19221	PASS
75	95	30	80	58.1	44053	PASS
95	95	100	100	100.0	75811	PASS
96	95	5	9	6.6	5009	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.0	59853	PASS
175	174	5	9	8.1	4870	PASS
176	174	95	101	97.3	58224	PASS
177	176	5	9	6.6	3822	PASS

m/z	Abundance
35.90	1077.0
37.00	5461.0
38.00	4892.0
39.00	2087.0
39.90	146.0
43.90	860.0
45.00	982.0
46.00	151.0
47.00	946.0
47.90	650.0
49.00	4243.0
50.00	19056.0
51.00	5813.0
51.90	303.0
54.90	312.0
55.90	1609.0
57.00	2386.0
57.90	112.0
60.00	842.0
60.90	4752.0
62.00	4989.0
63.00	3892.0
64.00	577.0
65.00	885.0
66.80	293.0
68.00	9129.0
69.00	9105.0
70.00	729.0
71.90	558.0
73.00	4355.0
74.00	15334.0
75.00	43824.0
76.00	3728.0
76.90	452.0
77.90	338.0
78.90	3697.0
79.90	1037.0
80.90	4011.0
81.90	1020.0
85.80	119.0
86.90	2966.0
87.90	2662.0
90.90	410.0
92.00	2377.0
93.00	3932.0
94.00	10215.0
95.00	74736.0
96.00	5075.0
96.90	177.0
103.80	441.0
104.80	123.0
105.80	418.0
112.80	113.0
115.80	295.0
116.90	868.0
117.90	358.0
118.80	502.0
127.90	267.0
128.70	118.0
129.90	263.0
134.90	215.0
136.80	164.0
138.80	106.0
140.80	957.0
141.90	119.0
142.90	1117.0
144.80	357.0
145.80	132.0
147.90	166.0
154.80	198.0
156.90	118.0
160.70	100.0
170.70	141.0
171.00	140.0
171.90	998.0
173.90	57760.0
174.90	4721.0
175.90	56448.0
176.90	3787.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.00	957.0
37.00	5222.0
38.00	4570.0
39.00	1819.0
40.00	162.0
43.90	944.0
44.90	989.0
45.90	103.0
47.00	948.0
47.90	580.0
49.00	3822.0
50.00	18784.0
51.00	5805.0
51.90	270.0
54.90	331.0
56.00	1680.0
56.90	2273.0
57.90	130.0
59.90	823.0
60.90	4498.0
62.00	4386.0
63.00	3542.0
64.00	491.0
65.00	670.0
65.90	128.0
67.00	226.0
68.00	8727.0
69.00	9409.0
70.00	615.0
72.00	588.0
73.00	4126.0
74.00	15232.0
75.00	42928.0
76.00	3384.0
77.00	446.0
77.90	332.0
78.90	3495.0
79.90	906.0
80.90	3787.0
81.80	918.0
82.80	121.0
85.90	140.0
86.90	2766.0
87.90	3059.0
90.90	420.0
92.00	2394.0
92.90	3467.0
94.00	10270.0
95.00	74480.0
96.00	4779.0
96.90	152.0
103.80	371.0
104.90	174.0
105.80	392.0
110.80	132.0
114.80	116.0
115.80	302.0
116.90	766.0
117.80	331.0
118.80	432.0
127.90	350.0
128.70	118.0
129.80	327.0
130.90	132.0
134.90	202.0
136.80	148.0
140.90	1038.0
141.90	115.0
142.90	1130.0
144.80	342.0
145.90	147.0
146.70	100.0
147.90	181.0
154.90	189.0
158.80	137.0
160.80	100.0
171.00	190.0
171.90	900.0
173.90	60152.0
174.90	4848.0
175.90	58256.0
176.90	3773.0
178.00	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
43.90	233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	1012.0
37.00	5551.0
38.00	4977.0
39.00	2053.0
40.00	146.0
43.90	943.0
44.90	1033.0
45.90	128.0
47.00	949.0
47.90	651.0
49.00	4191.0
50.00	19824.0
51.00	6047.0
51.90	298.0
52.80	105.0
54.90	358.0
55.90	1778.0
56.90	2409.0
57.90	120.0
60.00	846.0
60.90	4895.0
62.00	4959.0
63.00	3898.0
64.00	533.0
65.00	793.0
65.90	100.0
66.90	256.0
68.00	9340.0
69.00	9690.0
70.00	728.0
71.90	623.0
73.00	4482.0
74.00	16106.0
75.00	45408.0
76.00	3691.0
77.00	445.0
77.90	344.0
78.90	3738.0
79.90	1017.0
80.90	3996.0
81.80	1027.0
85.80	124.0
86.90	3016.0
87.90	2952.0
90.90	451.0
92.00	2576.0
93.00	3926.0
94.00	10765.0
95.00	78216.0
96.00	5172.0
96.90	178.0
103.80	427.0
104.80	157.0
105.80	438.0
109.80	119.0
110.80	119.0
112.80	105.0
114.80	107.0
115.80	313.0
116.90	874.0
117.80	351.0
118.80	453.0
127.90	335.0
128.70	110.0
129.80	316.0
130.90	131.0
134.90	229.0
136.80	171.0
140.90	1048.0
141.90	109.0
142.90	1144.0
144.80	360.0
145.80	140.0
146.70	100.0
147.90	188.0
154.90	212.0
156.90	101.0
158.80	132.0
171.00	178.0
171.90	995.0
173.90	61648.0
174.90	5041.0
175.90	59968.0
176.90	3905.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139