

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053992.D
 Acq On : 29 Apr 2023 17:39
 Operator : JC/MD
 Sample : 02565-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU053992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB	130149	154978	14.76%	1.975%
2	1.912	169	178	196	rBV	90780	123672	11.78%	1.576%
3	2.288	293	295	302	rVB2	555	498	0.05%	0.006%
4	2.565	369	381	402	rBV	226281	365828	34.83%	4.662%
5	2.793	446	452	458	rVB2	663	981	0.09%	0.013%
6	2.848	465	469	471	rBV	368	312	0.03%	0.004%
7	2.899	480	485	490	rBV2	355	356	0.03%	0.005%
8	2.948	495	500	503	rBV2	264	301	0.03%	0.004%
9	3.012	516	520	521	rBV	256	217	0.02%	0.003%
10	3.044	521	530	540	rVV4	2500	4256	0.41%	0.054%
11	3.176	566	571	573	rBV2	348	382	0.04%	0.005%
12	3.211	580	582	589	rVB	272	267	0.03%	0.003%
13	3.276	598	602	604	rBV	374	294	0.03%	0.004%
14	3.356	615	627	637	rBV5	778	1423	0.14%	0.018%
15	3.687	728	730	736	rVB2	358	287	0.03%	0.004%
16	3.735	740	745	746	rBV	217	207	0.02%	0.003%
17	3.796	759	764	767	rVB2	247	207	0.02%	0.003%
18	4.124	863	866	871	rVB2	427	345	0.03%	0.004%
19	4.173	877	881	888	rBV	264	395	0.04%	0.005%
20	4.292	914	918	921	rBV2	274	233	0.02%	0.003%
21	4.475	969	975	982	rVB2	432	657	0.06%	0.008%
22	4.517	983	988	992	rBV2	400	509	0.05%	0.006%
23	4.626	1007	1022	1053	rBV	70369	191448	18.23%	2.440%
24	5.057	1139	1156	1176	rBV	185142	408255	38.87%	5.203%
25	5.285	1222	1227	1231	rBV2	271	350	0.03%	0.004%
26	5.417	1265	1268	1272	rVB2	254	201	0.02%	0.003%
27	5.507	1290	1296	1298	rBV2	292	298	0.03%	0.004%
28	5.719	1338	1362	1395	rBV2	384604	1050208	100.00%	13.384%
29	5.947	1431	1433	1436	rBV2	369	270	0.03%	0.003%
30	5.973	1438	1441	1445	rVB2	313	239	0.02%	0.003%
31	5.996	1445	1448	1450	rBV	277	201	0.02%	0.003%
32	6.034	1456	1460	1468	rBV2	331	397	0.04%	0.005%
33	6.111	1480	1484	1488	rVB3	369	378	0.04%	0.005%
34	6.243	1510	1525	1548	rBV	349832	667209	63.53%	8.503%
35	6.526	1605	1613	1614	rBV4	2121	2650	0.25%	0.034%
36	6.600	1630	1636	1640	rBV	309	389	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053992.D
 Acq On : 29 Apr 2023 17:39
 Operator : JC/MD
 Sample : 02565-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.684	1648	1662	1683	rBV	240124	470557	44.81%	5.997%
38	6.796	1694	1697	1711	rVB6	997	1560	0.15%	0.020%
39	6.918	1730	1735	1737	rBV2	238	210	0.02%	0.003%
40	7.176	1809	1815	1817	rBV2	322	354	0.03%	0.005%
41	7.189	1817	1819	1822	rVB2	353	226	0.02%	0.003%
42	7.205	1822	1824	1828	rBV3	383	299	0.03%	0.004%
43	7.510	1913	1919	1922	rBV2	285	257	0.02%	0.003%
44	7.562	1922	1935	1953	rBV	131477	234309	22.31%	2.986%
45	7.700	1974	1978	1983	rVB3	486	464	0.04%	0.006%
46	7.726	1983	1986	1989	rBV2	198	205	0.02%	0.003%
47	7.803	2005	2010	2014	rVV3	339	379	0.04%	0.005%
48	7.893	2025	2038	2055	rBV	474604	831728	79.20%	10.600%
49	8.079	2094	2096	2101	rVB	503	387	0.04%	0.005%
50	8.111	2101	2106	2109	rBV2	243	268	0.03%	0.003%
51	8.176	2113	2126	2149	rBV2	91063	160449	15.28%	2.045%
52	8.436	2205	2207	2211	rVB2	286	204	0.02%	0.003%
53	8.462	2212	2215	2218	rVB2	347	194	0.02%	0.002%
54	8.549	2235	2242	2253	rBV4	3111	4945	0.47%	0.063%
55	8.629	2255	2267	2300	rBV	226126	428679	40.82%	5.463%
56	8.851	2333	2336	2340	rBV2	255	229	0.02%	0.003%
57	8.922	2355	2358	2362	rBV2	293	251	0.02%	0.003%
58	9.041	2392	2395	2398	rVB2	241	195	0.02%	0.002%
59	9.195	2439	2443	2445	rBV2	293	237	0.02%	0.003%
60	9.237	2453	2456	2459	rBV2	281	238	0.02%	0.003%
61	9.410	2498	2510	2550	rBV	458652	773877	73.69%	9.862%
62	9.568	2556	2559	2563	rVB	410	297	0.03%	0.004%
63	9.613	2570	2573	2578	rBV2	240	232	0.02%	0.003%
64	9.684	2591	2595	2596	rBV2	403	264	0.03%	0.003%
65	9.690	2596	2597	2605	rVB3	745	731	0.07%	0.009%
66	9.828	2637	2640	2646	rBV2	172	209	0.02%	0.003%
67	9.877	2651	2655	2660	rVB2	292	318	0.03%	0.004%
68	9.912	2661	2666	2670	rVB2	337	349	0.03%	0.004%
69	10.105	2723	2726	2728	rVV2	634	359	0.03%	0.005%
70	10.121	2728	2731	2734	rVB3	641	448	0.04%	0.006%
71	10.288	2779	2783	2785	rBV2	284	197	0.02%	0.003%
72	10.478	2838	2842	2848	rVB4	786	877	0.08%	0.011%
73	10.751	2914	2927	2946	rBV	293237	478413	45.55%	6.097%
74	11.285	3087	3093	3096	rBB	332	289	0.03%	0.004%
75	11.465	3145	3149	3152	rBV2	533	513	0.05%	0.007%
76	11.552	3172	3176	3181	rVB	273	272	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053992.D
 Acq On : 29 Apr 2023 17:39
 Operator : JC/MD
 Sample : 02565-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.667	3207	3212	3213	rBV	282	261	0.02%	0.003%
78	11.709	3221	3225	3228	rBV2	299	259	0.02%	0.003%
79	11.745	3229	3236	3243	rBV3	1800	1967	0.19%	0.025%
80	11.806	3243	3255	3273	rBV	462280	729941	69.50%	9.302%
81	12.012	3315	3319	3323	rVB3	465	417	0.04%	0.005%
82	12.050	3327	3331	3337	rBV2	311	382	0.04%	0.005%
83	12.188	3361	3374	3390	rBV	448540	720090	68.57%	9.177%
84	12.330	3415	3418	3421	rVB3	290	219	0.02%	0.003%
85	12.433	3443	3450	3455	rBV2	380	458	0.04%	0.006%
86	12.458	3455	3458	3459	rBV2	354	198	0.02%	0.003%
87	13.053	3639	3643	3647	rVB2	594	454	0.04%	0.006%
88	13.230	3688	3698	3703	rVB4	1398	2103	0.20%	0.027%
89	13.336	3726	3731	3736	rBV2	348	384	0.04%	0.005%
90	13.423	3754	3758	3763	rBV3	296	276	0.03%	0.004%
91	13.516	3785	3787	3790	rBV2	323	196	0.02%	0.002%
92	13.732	3851	3854	3859	rVB2	432	325	0.03%	0.004%
93	13.841	3881	3888	3896	rBV4	3268	4805	0.46%	0.061%
94	14.089	3957	3965	3967	rBV5	2790	3002	0.29%	0.038%
95	14.220	4003	4006	4008	rBV2	459	347	0.03%	0.004%
96	14.330	4030	4040	4048	rBV4	3386	5255	0.50%	0.067%
97	14.426	4067	4070	4072	rBV2	297	205	0.02%	0.003%
98	15.281	4333	4336	4340	rBV2	529	462	0.04%	0.006%
99	16.050	4572	4575	4578	rBV2	863	595	0.06%	0.008%
100	16.169	4610	4612	4615	rBV4	830	598	0.06%	0.008%


Sum of corrected areas: 7846766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053992.D
Acq On : 29 Apr 2023 17:39
Operator : JC/MD
Sample : 02565-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

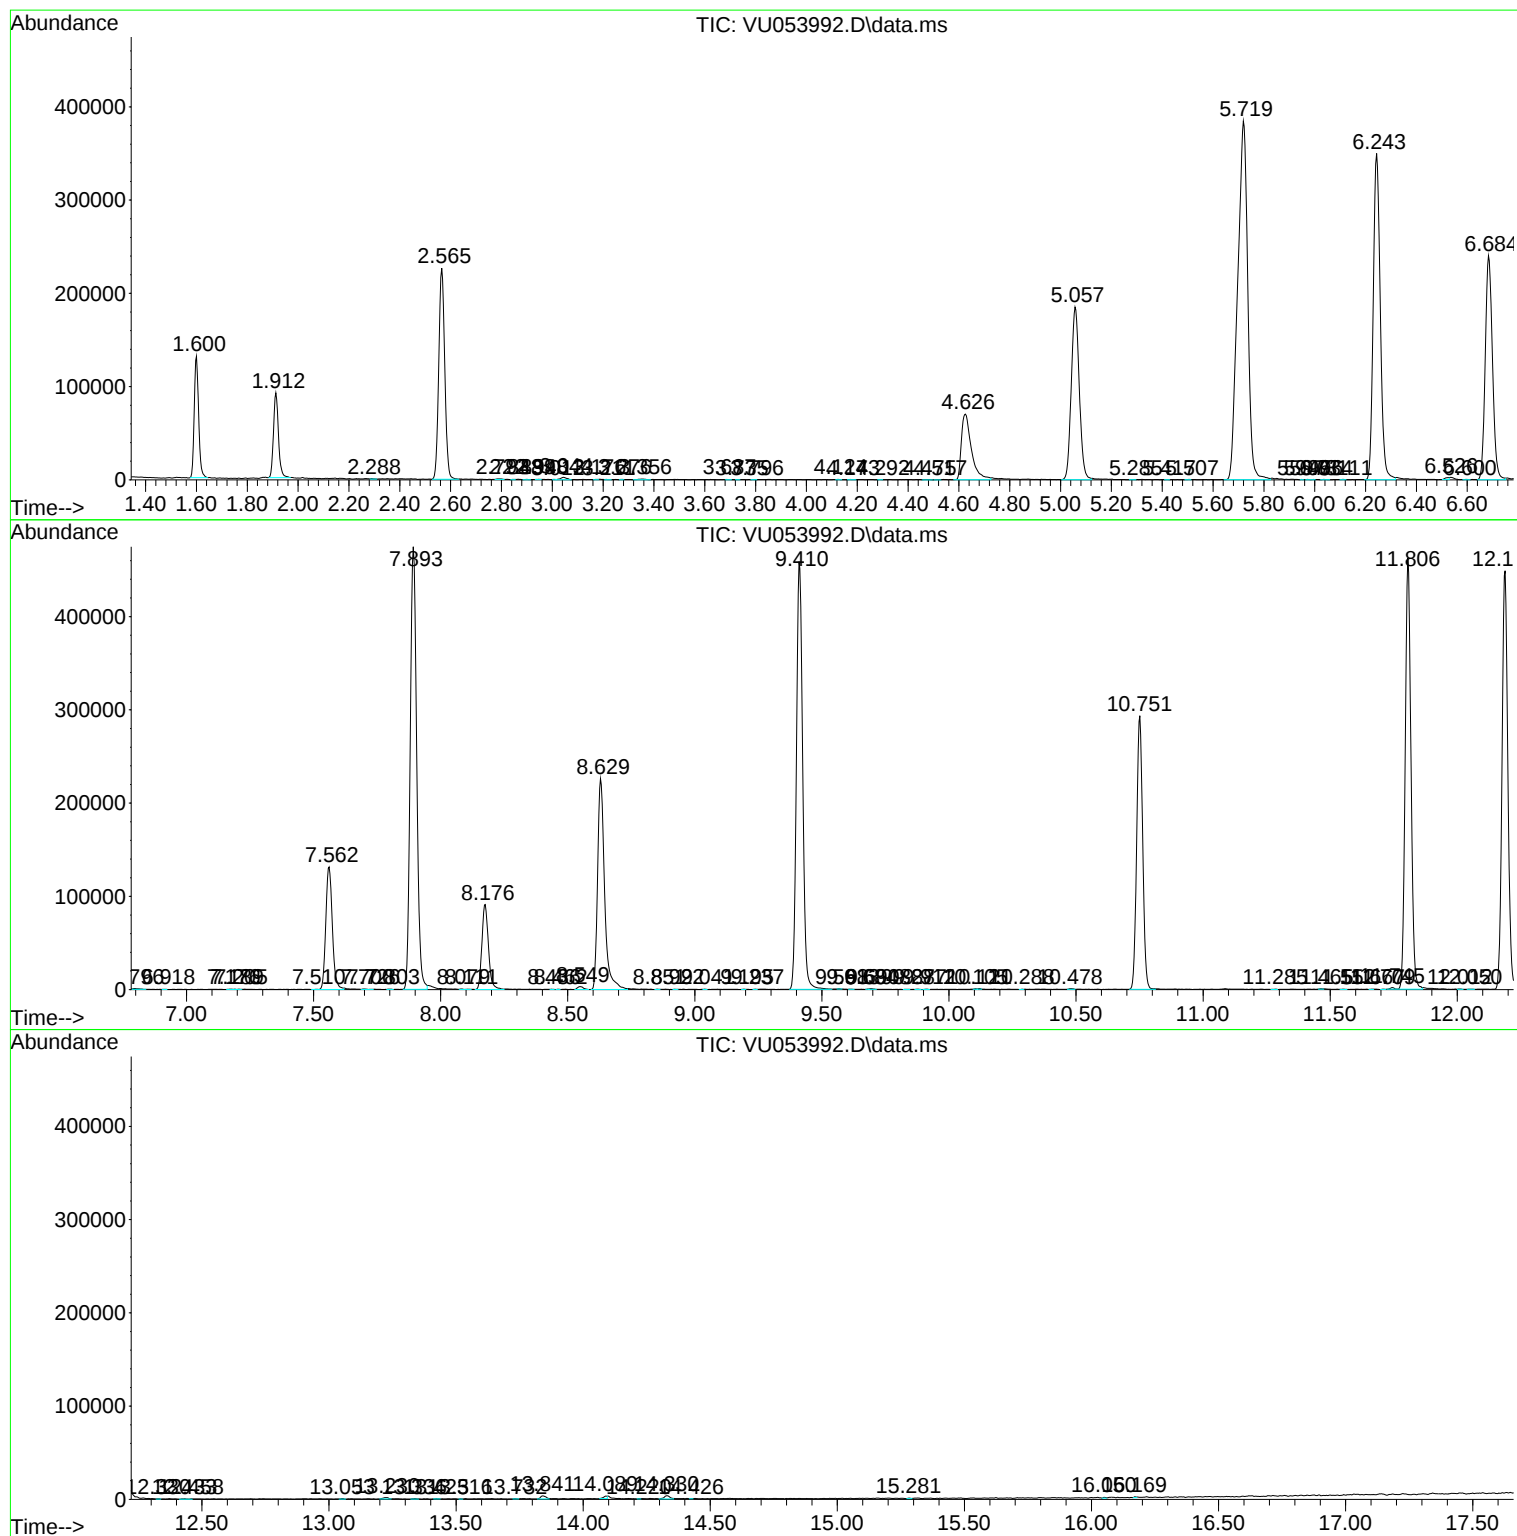

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053992.D
Acq On : 29 Apr 2023 17:39
Operator : JC/MD
Sample : 02565-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053992.D
Acq On : 29 Apr 2023 17:39
Operator : JC/MD
Sample : 02565-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc