

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053993.D
 Acq On : 29 Apr 2023 18:03
 Operator : JC/MD
 Sample : 02565-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU053993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rVB	124631	150170	14.82%	1.958%
2	1.912	169	178	193	rBV	87570	118411	11.69%	1.544%
3	2.105	234	238	239	rBV	495	391	0.04%	0.005%
4	2.285	292	294	297	rBV	404	261	0.03%	0.003%
5	2.565	368	381	399	rBV	215068	350871	34.64%	4.575%
6	3.051	522	532	539	rVV3	1185	2178	0.22%	0.028%
7	3.086	539	543	547	rVB2	307	332	0.03%	0.004%
8	3.356	625	627	632	rVB2	601	399	0.04%	0.005%
9	3.526	674	680	684	rBV2	292	371	0.04%	0.005%
10	3.587	697	699	706	rVB	272	209	0.02%	0.003%
11	3.890	790	793	796	rVV2	296	223	0.02%	0.003%
12	4.009	825	830	833	rBV	158	207	0.02%	0.003%
13	4.067	844	848	851	rBV	264	209	0.02%	0.003%
14	4.263	906	909	915	rVB2	300	344	0.03%	0.004%
15	4.337	927	932	939	rVB2	243	292	0.03%	0.004%
16	4.449	963	967	970	rVB2	212	204	0.02%	0.003%
17	4.497	977	982	984	rBV	202	201	0.02%	0.003%
18	4.530	989	992	996	rBV2	391	283	0.03%	0.004%
19	4.623	1005	1021	1060	rBV	72053	196357	19.38%	2.560%
20	5.057	1140	1156	1177	rBV	181218	396493	39.14%	5.170%
21	5.719	1341	1362	1394	rBV2	369736	1013006	100.00%	13.210%
22	5.928	1423	1427	1431	rBV3	345	374	0.04%	0.005%
23	6.012	1448	1453	1457	rBV2	344	287	0.03%	0.004%
24	6.243	1511	1525	1555	rBV	346921	668144	65.96%	8.713%
25	6.456	1588	1591	1594	rVB	338	268	0.03%	0.003%
26	6.484	1598	1600	1603	rVB	288	204	0.02%	0.003%
27	6.533	1606	1615	1625	rVB8	2913	5467	0.54%	0.071%
28	6.684	1648	1662	1685	rBV	231327	453397	44.76%	5.912%
29	6.787	1692	1694	1697	rVB3	561	262	0.03%	0.003%
30	6.877	1718	1722	1726	rBV2	268	278	0.03%	0.004%
31	6.954	1744	1746	1750	rVB	305	219	0.02%	0.003%
32	7.185	1814	1818	1820	rBV	482	359	0.04%	0.005%
33	7.404	1883	1886	1892	rBV2	209	198	0.02%	0.003%
34	7.475	1905	1908	1913	rVB2	214	212	0.02%	0.003%
35	7.562	1923	1935	1953	rBV	126230	224636	22.18%	2.929%
36	7.703	1972	1979	1983	rVV4	387	517	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053993.D
 Acq On : 29 Apr 2023 18:03
 Operator : JC/MD
 Sample : 02565-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	7.790	2002	2006	2009	rBV2	395	379	0.04%	0.005%
38	7.828	2015	2018	2021	rBV2	241	212	0.02%	0.003%
39	7.893	2025	2038	2064	rBV	460198	802439	79.21%	10.464%
40	8.086	2093	2098	2105	rVB3	356	577	0.06%	0.008%
41	8.172	2112	2125	2151	rBV	87152	152738	15.08%	1.992%
42	8.346	2175	2179	2181	rBV	300	225	0.02%	0.003%
43	8.488	2218	2223	2227	rBV2	314	319	0.03%	0.004%
44	8.510	2227	2230	2233	rBV	234	206	0.02%	0.003%
45	8.552	2235	2243	2253	rVB5	3206	4607	0.45%	0.060%
46	8.629	2253	2267	2297	rBV2	216666	420720	41.53%	5.486%
47	8.867	2338	2341	2343	rBV	329	212	0.02%	0.003%
48	8.896	2346	2350	2353	rVB	353	252	0.02%	0.003%
49	9.150	2422	2429	2434	rVB	319	399	0.04%	0.005%
50	9.259	2458	2463	2467	rVB	301	310	0.03%	0.004%
51	9.282	2467	2470	2474	rVB	422	347	0.03%	0.005%
52	9.343	2485	2489	2494	rBV2	224	239	0.02%	0.003%
53	9.410	2497	2510	2537	rBV	458570	769782	75.99%	10.038%
54	9.562	2554	2557	2559	rBV	686	531	0.05%	0.007%
55	9.690	2594	2597	2604	rVB4	722	892	0.09%	0.012%
56	9.870	2649	2653	2657	rBV2	220	219	0.02%	0.003%
57	9.938	2671	2674	2678	rBV2	269	277	0.03%	0.004%
58	9.979	2684	2687	2691	rBV2	224	200	0.02%	0.003%
59	10.012	2693	2697	2704	rVB2	353	410	0.04%	0.005%
60	10.044	2704	2707	2710	rBV	296	242	0.02%	0.003%
61	10.205	2752	2757	2759	rBV2	307	284	0.03%	0.004%
62	10.250	2769	2771	2775	rVB2	264	198	0.02%	0.003%
63	10.298	2782	2786	2791	rVB2	306	273	0.03%	0.004%
64	10.484	2839	2844	2847	rBV2	407	415	0.04%	0.005%
65	10.520	2850	2855	2859	rBV2	242	253	0.02%	0.003%
66	10.674	2900	2903	2907	rBV2	311	246	0.02%	0.003%
67	10.751	2915	2927	2945	rBV	285821	464139	45.82%	6.052%
68	10.873	2961	2965	2966	rBV	296	219	0.02%	0.003%
69	11.015	3006	3009	3014	rVB2	255	251	0.02%	0.003%
70	11.082	3026	3030	3034	rBV2	391	294	0.03%	0.004%
71	11.169	3052	3057	3062	rBV2	374	365	0.04%	0.005%
72	11.359	3112	3116	3118	rBV2	208	220	0.02%	0.003%
73	11.475	3145	3152	3158	rBV3	757	1096	0.11%	0.014%
74	11.568	3178	3181	3185	rVB	267	203	0.02%	0.003%
75	11.606	3188	3193	3194	rBV	354	290	0.03%	0.004%
76	11.738	3230	3234	3243	rBV5	1271	1743	0.17%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053993.D
 Acq On : 29 Apr 2023 18:03
 Operator : JC/MD
 Sample : 02565-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.806	3243	3255	3274	rBV	463482	735715	72.63%	9.594%
78	11.967	3303	3305	3309	rVB2	308	228	0.02%	0.003%
79	12.188	3361	3374	3396	rBV	427616	701308	69.23%	9.145%
80	12.372	3429	3431	3436	rVB2	387	268	0.03%	0.003%
81	12.606	3500	3504	3507	rVB2	283	249	0.02%	0.003%
82	12.648	3512	3517	3518	rBV2	244	197	0.02%	0.003%
83	12.838	3571	3576	3578	rBV	353	329	0.03%	0.004%
84	12.922	3600	3602	3607	rVB	340	261	0.03%	0.003%
85	12.960	3611	3614	3617	rBV	319	210	0.02%	0.003%
86	13.015	3628	3631	3635	rVB2	276	237	0.02%	0.003%
87	13.224	3690	3696	3703	rVB4	1084	1653	0.16%	0.022%
88	13.269	3706	3710	3712	rBV2	344	270	0.03%	0.004%
89	13.304	3718	3721	3724	rBV2	311	210	0.02%	0.003%
90	13.423	3755	3758	3766	rVV3	421	529	0.05%	0.007%
91	13.513	3782	3786	3788	rBV	283	249	0.02%	0.003%
92	13.848	3883	3890	3897	rVB4	1610	2541	0.25%	0.033%
93	14.024	3943	3945	3952	rVB3	514	501	0.05%	0.007%
94	14.063	3952	3957	3958	rBV	437	326	0.03%	0.004%
95	14.095	3961	3967	3978	rVB3	2855	4266	0.42%	0.056%
96	14.192	3995	3997	4002	rBV2	291	298	0.03%	0.004%
97	14.330	4033	4040	4049	rVB4	2661	4024	0.40%	0.052%
98	14.558	4108	4111	4112	rBV4	441	218	0.02%	0.003%
99	15.381	4365	4367	4374	rVB2	723	492	0.05%	0.006%
100	15.420	4374	4379	4384	rBV3	514	725	0.07%	0.009%




Sum of corrected areas: 7668761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053993.D
Acq On : 29 Apr 2023 18:03
Operator : JC/MD
Sample : 02565-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

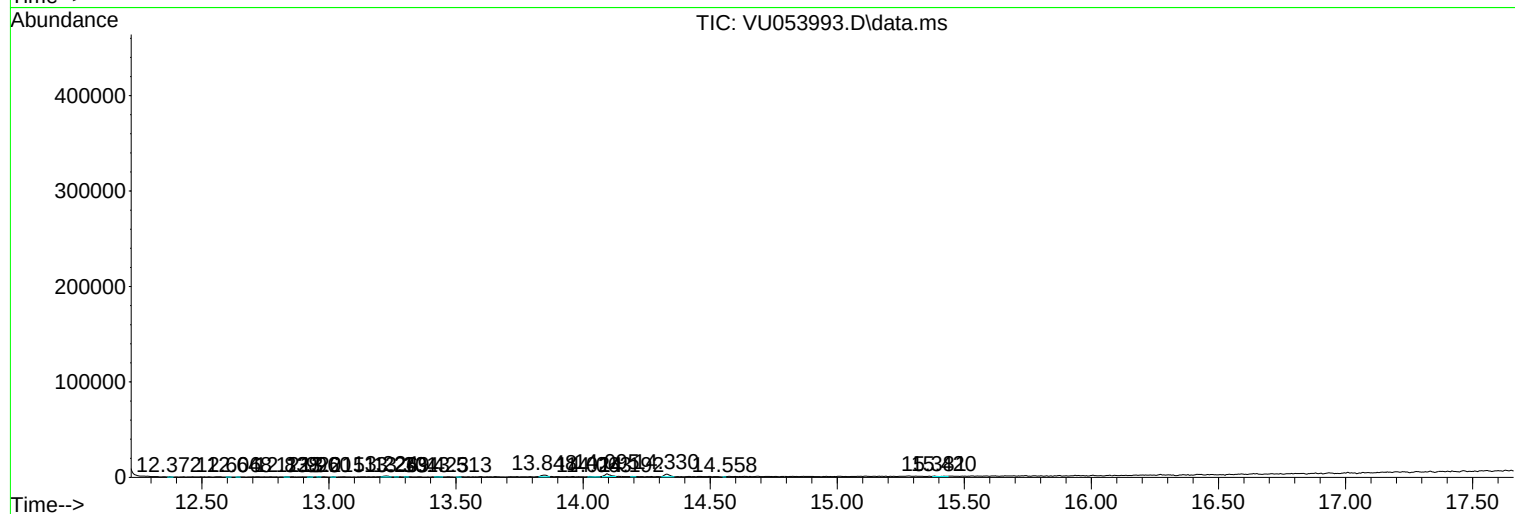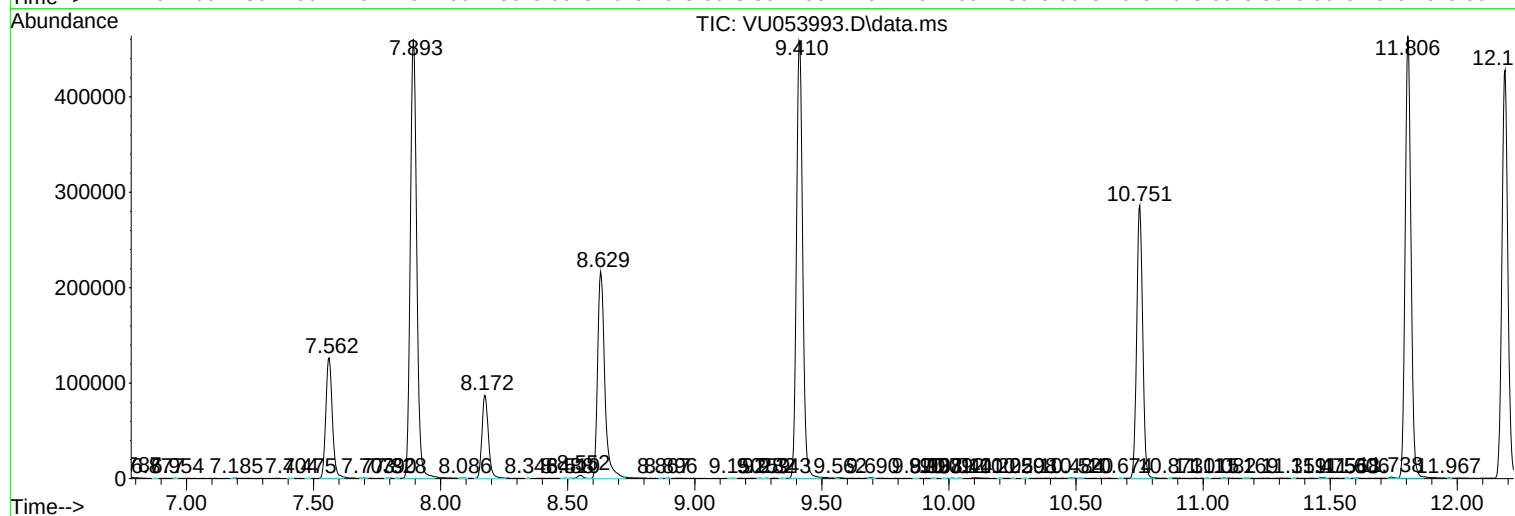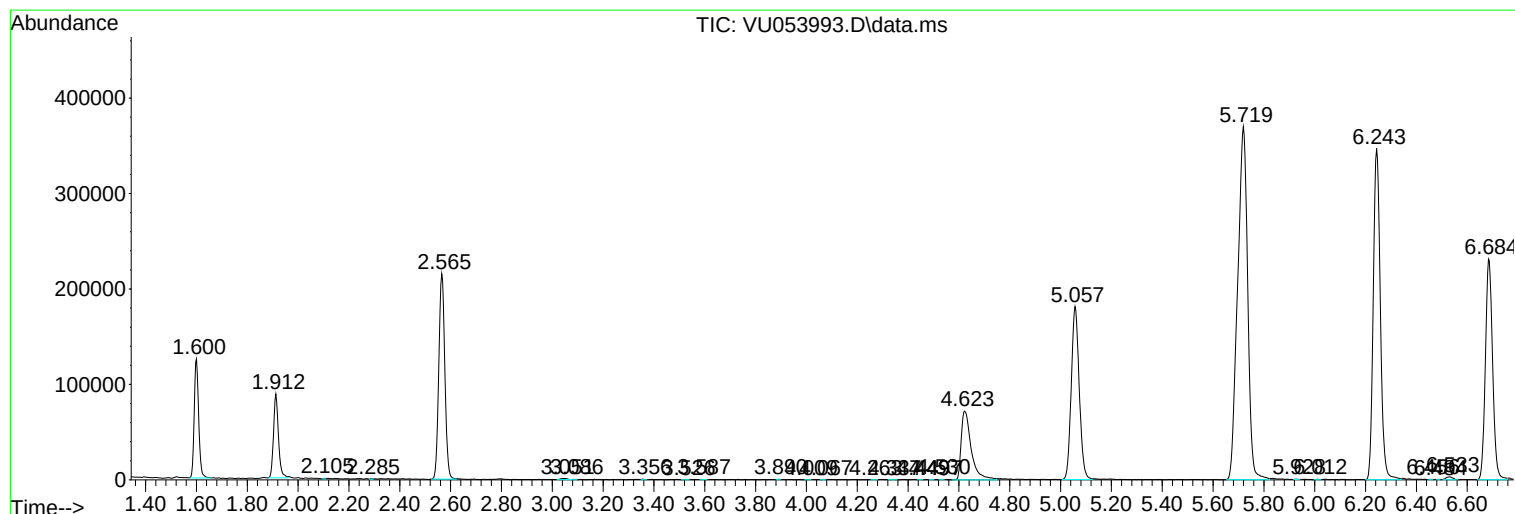

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053993.D
Acq On : 29 Apr 2023 18:03
Operator : JC/MD
Sample : 02565-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053993.D
Acq On : 29 Apr 2023 18:03
Operator : JC/MD
Sample : 02565-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc