

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053995.D
 Acq On : 29 Apr 2023 18:50
 Operator : JC/MD
 Sample : 02565-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU053995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	96	rBV	124890	150295	14.40%	1.919%
2	1.912	170	178	195	rVB	88296	118540	11.36%	1.513%
3	2.565	368	381	398	rBV	221916	363655	34.84%	4.642%
4	2.707	423	425	429	rVB	304	149	0.01%	0.002%
5	2.842	463	467	471	rVB2	293	223	0.02%	0.003%
6	2.861	471	473	475	rBV	244	154	0.01%	0.002%
7	3.044	523	530	538	rVB2	1136	1899	0.18%	0.024%
8	3.108	545	550	553	rBV2	225	210	0.02%	0.003%
9	3.186	571	574	578	rBV2	271	155	0.01%	0.002%
10	3.205	578	580	583	rBV2	219	160	0.02%	0.002%
11	3.247	590	593	595	rBV	329	152	0.01%	0.002%
12	3.385	633	636	639	rBV2	208	145	0.01%	0.002%
13	3.607	702	705	708	rBV	308	261	0.03%	0.003%
14	3.761	750	753	758	rBV2	167	132	0.01%	0.002%
15	3.790	758	762	765	rBV2	245	188	0.02%	0.002%
16	3.845	777	779	785	rVB2	260	246	0.02%	0.003%
17	3.964	814	816	820	rVB	233	139	0.01%	0.002%
18	3.999	824	827	831	rVB	171	160	0.02%	0.002%
19	4.025	831	835	837	rBV	252	201	0.02%	0.003%
20	4.076	848	851	852	rBV	210	117	0.01%	0.001%
21	4.137	867	870	872	rBV2	242	163	0.02%	0.002%
22	4.166	872	879	889	rBV2	240	563	0.05%	0.007%
23	4.343	931	934	936	rBV2	235	168	0.02%	0.002%
24	4.462	969	971	976	rBV2	170	149	0.01%	0.002%
25	4.514	983	987	990	rVB2	263	208	0.02%	0.003%
26	4.536	990	994	997	rBV	203	115	0.01%	0.001%
27	4.623	1009	1021	1054	rBV	75236	198860	19.05%	2.539%
28	4.944	1118	1121	1123	rBV	256	146	0.01%	0.002%
29	4.996	1134	1137	1141	rBV2	232	192	0.02%	0.002%
30	5.057	1141	1156	1180	rBV	187124	411220	39.40%	5.250%
31	5.247	1213	1215	1219	rVB3	333	211	0.02%	0.003%
32	5.427	1267	1271	1276	rBV2	203	262	0.03%	0.003%
33	5.465	1280	1283	1285	rBV	155	132	0.01%	0.002%
34	5.584	1316	1320	1323	rVB2	231	176	0.02%	0.002%
35	5.616	1323	1330	1333	rBV2	252	364	0.03%	0.005%
36	5.719	1340	1362	1384	rBV2	386855	1043829	100.00%	13.325%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053995.D
 Acq On : 29 Apr 2023 18:50
 Operator : JC/MD
 Sample : 02565-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.034	1457	1460	1462	rVB2	331	137	0.01%	0.002%
38	6.086	1472	1476	1479	rBV	291	259	0.02%	0.003%
39	6.243	1511	1525	1547	rBV	348889	660195	63.25%	8.428%
40	6.478	1594	1598	1600	rBV	300	203	0.02%	0.003%
41	6.530	1605	1614	1623	rVB7	3064	5733	0.55%	0.073%
42	6.565	1623	1625	1629	rVB3	283	163	0.02%	0.002%
43	6.684	1648	1662	1682	rBV	236370	465450	44.59%	5.942%
44	6.835	1708	1709	1713	rVB2	320	189	0.02%	0.002%
45	6.890	1721	1726	1727	rBV	166	167	0.02%	0.002%
46	6.948	1741	1744	1747	rBV2	272	154	0.01%	0.002%
47	6.989	1752	1757	1759	rBV	262	270	0.03%	0.003%
48	7.063	1776	1780	1785	rVB	244	171	0.02%	0.002%
49	7.092	1785	1789	1794	rBV2	218	253	0.02%	0.003%
50	7.160	1804	1810	1813	rVB2	327	369	0.04%	0.005%
51	7.195	1813	1821	1824	rBV2	593	726	0.07%	0.009%
52	7.243	1833	1836	1841	rBV2	213	183	0.02%	0.002%
53	7.304	1852	1855	1857	rBV	172	145	0.01%	0.002%
54	7.337	1861	1865	1871	rBV2	164	175	0.02%	0.002%
55	7.433	1889	1895	1896	rBV	185	138	0.01%	0.002%
56	7.491	1911	1913	1915	rBV2	396	186	0.02%	0.002%
57	7.562	1923	1935	1952	rBV	132480	234269	22.44%	2.991%
58	7.738	1988	1990	1992	rBV	168	119	0.01%	0.002%
59	7.783	2001	2004	2009	rVB	249	143	0.01%	0.002%
60	7.803	2009	2010	2016	rVB2	262	141	0.01%	0.002%
61	7.835	2017	2020	2023	rVB2	221	169	0.02%	0.002%
62	7.893	2023	2038	2071	rBV	481406	836768	80.16%	10.682%
63	8.131	2108	2112	2113	rBV	333	181	0.02%	0.002%
64	8.176	2115	2126	2145	rVV	92078	157354	15.07%	2.009%
65	8.430	2202	2205	2209	rBV	268	187	0.02%	0.002%
66	8.504	2223	2228	2235	rBV2	274	384	0.04%	0.005%
67	8.549	2235	2242	2253	rVB6	2371	3860	0.37%	0.049%
68	8.629	2253	2267	2298	rBV	235551	440914	42.24%	5.629%
69	8.922	2353	2358	2361	rVB2	264	256	0.02%	0.003%
70	8.951	2361	2367	2369	rBV2	305	378	0.04%	0.005%
71	9.082	2405	2408	2412	rVB2	238	212	0.02%	0.003%
72	9.269	2460	2466	2469	rBV2	229	302	0.03%	0.004%
73	9.330	2480	2485	2490	rVB2	230	252	0.02%	0.003%
74	9.410	2496	2510	2542	rBV	456497	770387	73.80%	9.835%
75	9.645	2580	2583	2584	rBV	258	143	0.01%	0.002%
76	9.841	2641	2644	2647	rBV2	293	187	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053995.D
 Acq On : 29 Apr 2023 18:50
 Operator : JC/MD
 Sample : 02565-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	9.922	2665	2669	2672	rBV	178	199	0.02%	0.003%
78	10.147	2736	2739	2742	rBV2	236	130	0.01%	0.002%
79	10.259	2771	2774	2777	rBV	203	173	0.02%	0.002%
80	10.430	2824	2827	2829	rBV	166	130	0.01%	0.002%
81	10.574	2870	2872	2875	rBV	225	155	0.01%	0.002%
82	10.751	2909	2927	2944	rBV	295520	484440	46.41%	6.184%
83	10.873	2962	2965	2967	rBV2	211	141	0.01%	0.002%
84	11.012	3005	3008	3010	rBV2	192	131	0.01%	0.002%
85	11.060	3021	3023	3029	rBV	222	268	0.03%	0.003%
86	11.166	3052	3056	3057	rBV	232	159	0.02%	0.002%
87	11.201	3065	3067	3072	rVB2	259	217	0.02%	0.003%
88	11.378	3117	3122	3128	rBV	244	390	0.04%	0.005%
89	11.465	3146	3149	3151	rBV	492	388	0.04%	0.005%
90	11.504	3158	3161	3165	rBV2	245	273	0.03%	0.003%
91	11.745	3230	3236	3243	rBV4	1252	1668	0.16%	0.021%
92	11.806	3243	3255	3279	rBV	463783	737046	70.61%	9.409%
93	12.105	3343	3348	3350	rBV2	323	294	0.03%	0.004%
94	12.188	3360	3374	3391	rBV	444698	729694	69.91%	9.315%
95	12.632	3508	3512	3515	rBV2	349	267	0.03%	0.003%
96	12.716	3534	3538	3544	rBV2	247	351	0.03%	0.004%
97	12.886	3589	3591	3595	rBV2	310	254	0.02%	0.003%
98	13.159	3674	3676	3678	rBV	245	150	0.01%	0.002%
99	13.192	3683	3686	3688	rBV	255	198	0.02%	0.003%
100	13.513	3781	3786	3789	rBV2	588	574	0.05%	0.007%




Sum of corrected areas: 7833501

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053995.D
Acq On : 29 Apr 2023 18:50
Operator : JC/MD
Sample : 02565-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

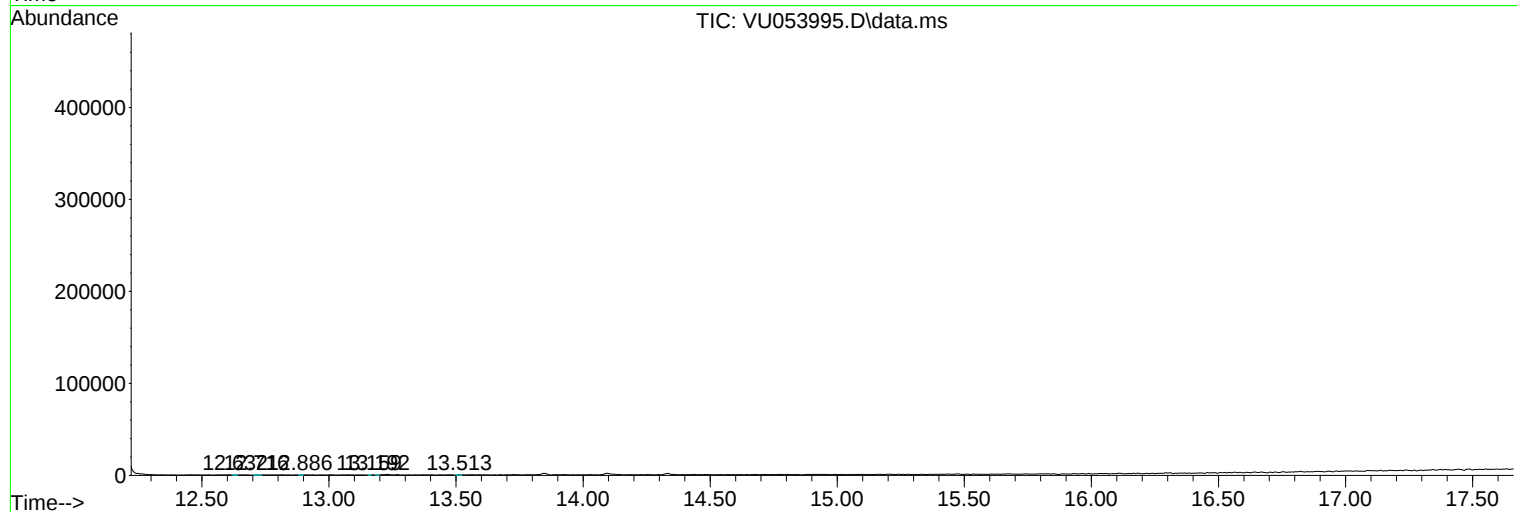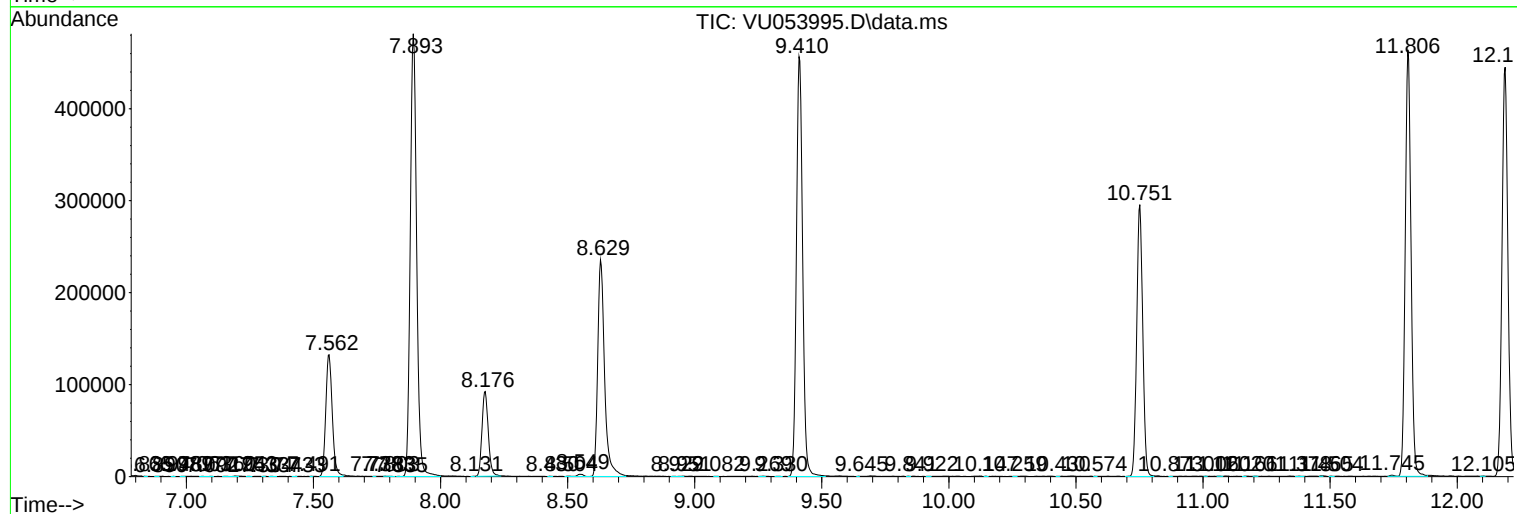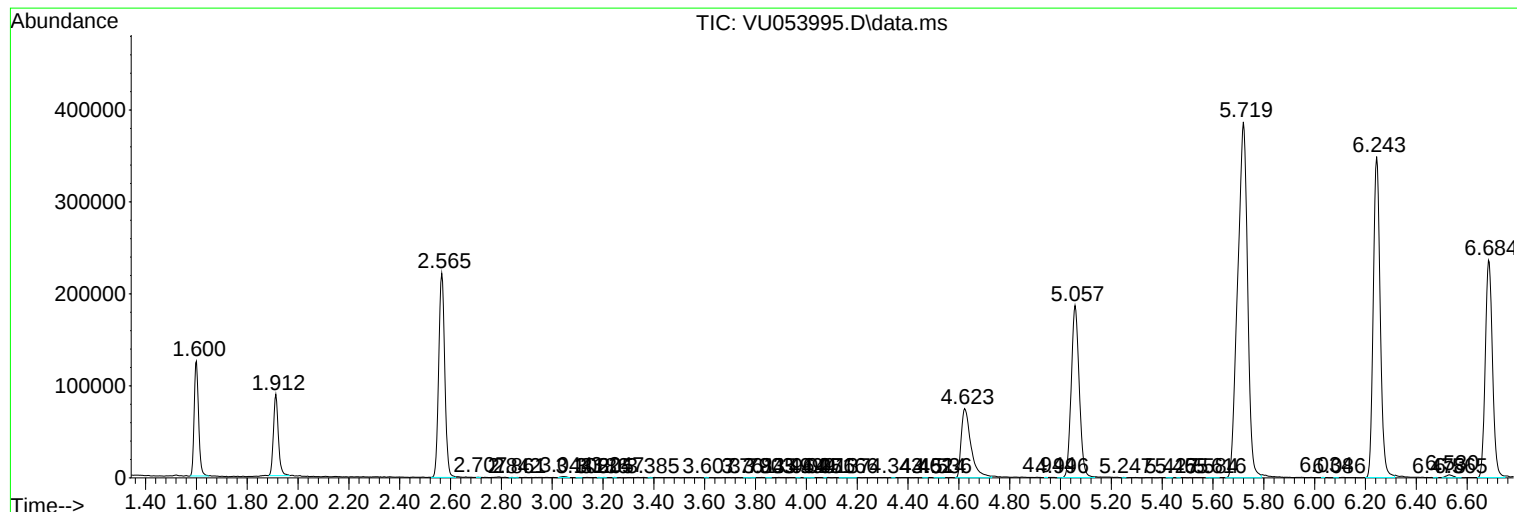

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053995.D
Acq On : 29 Apr 2023 18:50
Operator : JC/MD
Sample : 02565-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053995.D
Acq On : 29 Apr 2023 18:50
Operator : JC/MD
Sample : 02565-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------