

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053997.D
 Acq On : 29 Apr 2023 19:36
 Operator : JC/MD
 Sample : 02565-07 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU053997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	106	rVB	122438	148189	14.88%	1.985%
2	1.913	170	178	197	rVB	85856	116726	11.72%	1.564%
3	2.565	369	381	400	rBV	213995	346283	34.77%	4.639%
4	2.697	418	422	426	rBV3	472	482	0.05%	0.006%
5	3.044	522	530	539	rBV6	1554	2997	0.30%	0.040%
6	3.176	567	571	573	rBV2	441	399	0.04%	0.005%
7	3.234	587	589	592	rVB	211	113	0.01%	0.002%
8	3.462	652	660	665	rBV2	457	544	0.05%	0.007%
9	3.514	672	676	680	rBV2	303	297	0.03%	0.004%
10	3.610	704	706	712	rVB2	324	198	0.02%	0.003%
11	3.797	761	764	765	rBV	149	71	0.01%	0.001%
12	3.838	774	777	780	rBV	189	142	0.01%	0.002%
13	3.871	784	787	789	rBV	177	119	0.01%	0.002%
14	3.961	809	815	820	rVB2	285	396	0.04%	0.005%
15	3.986	820	823	826	rBV	205	198	0.02%	0.003%
16	4.002	826	828	829	rBV	189	51	0.01%	0.001%
17	4.096	854	857	859	rBV2	178	137	0.01%	0.002%
18	4.195	885	888	891	rVB	198	125	0.01%	0.002%
19	4.228	896	898	901	rVB	328	174	0.02%	0.002%
20	4.247	902	904	905	rBV	190	81	0.01%	0.001%
21	4.282	912	915	919	rVB	200	149	0.01%	0.002%
22	4.308	922	923	926	rBV	144	54	0.01%	0.001%
23	4.356	935	938	941	rBV2	253	191	0.02%	0.003%
24	4.430	959	961	963	rBV	115	59	0.01%	0.001%
25	4.501	979	983	986	rBV2	342	382	0.04%	0.005%
26	4.555	998	1000	1001	rBV2	132	56	0.01%	0.001%
27	4.623	1010	1021	1053	rBV	68660	180155	18.09%	2.413%
28	5.057	1140	1156	1181	rBV	176668	388755	39.03%	5.208%
29	5.295	1228	1230	1233	rBV2	144	118	0.01%	0.002%
30	5.356	1246	1249	1253	rBV2	219	192	0.02%	0.003%
31	5.417	1266	1268	1269	rBV2	187	83	0.01%	0.001%
32	5.472	1283	1285	1288	rVB	196	119	0.01%	0.002%
33	5.488	1288	1290	1294	rBV	208	161	0.02%	0.002%
34	5.562	1311	1313	1315	rBV	242	157	0.02%	0.002%
35	5.719	1341	1362	1387	rBV2	367753	996028	100.00%	13.343%
36	6.147	1493	1495	1497	rVB	171	67	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053997.D
 Acq On : 29 Apr 2023 19:36
 Operator : JC/MD
 Sample : 02565-07 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.163	1497	1500	1503	rBV3	270	191	0.02%	0.003%
38	6.244	1512	1525	1553	rBV	336625	644772	64.73%	8.637%
39	6.411	1573	1577	1579	rBV	392	351	0.04%	0.005%
40	6.523	1605	1612	1623	rVB6	2247	4284	0.43%	0.057%
41	6.684	1648	1662	1686	rBV	227581	449336	45.11%	6.019%
42	6.851	1711	1714	1718	rBV2	192	140	0.01%	0.002%
43	6.938	1738	1741	1746	rVB2	252	215	0.02%	0.003%
44	7.028	1766	1769	1772	rBV2	189	153	0.02%	0.002%
45	7.067	1779	1781	1784	rBV	183	125	0.01%	0.002%
46	7.083	1784	1786	1790	rBV	233	142	0.01%	0.002%
47	7.131	1799	1801	1803	rVB	189	79	0.01%	0.001%
48	7.160	1803	1810	1812	rBV	240	317	0.03%	0.004%
49	7.269	1842	1844	1847	rVB2	187	99	0.01%	0.001%
50	7.369	1872	1875	1879	rVB	452	355	0.04%	0.005%
51	7.391	1879	1882	1885	rBV	426	382	0.04%	0.005%
52	7.559	1923	1934	1961	rVB2	122456	219043	21.99%	2.934%
53	7.739	1988	1990	1992	rBV	209	82	0.01%	0.001%
54	7.829	2015	2018	2019	rBV	152	86	0.01%	0.001%
55	7.893	2024	2038	2059	rBV	452583	795359	79.85%	10.654%
56	8.173	2113	2125	2146	rBV	86944	150483	15.11%	2.016%
57	8.359	2180	2183	2188	rBV2	249	274	0.03%	0.004%
58	8.552	2236	2243	2249	rBV6	2348	3257	0.33%	0.044%
59	8.629	2255	2267	2300	rBV	210917	399627	40.12%	5.353%
60	8.938	2360	2363	2367	rBV	206	179	0.02%	0.002%
61	8.973	2372	2374	2376	rBV	192	97	0.01%	0.001%
62	9.253	2459	2461	2463	rVB	228	114	0.01%	0.002%
63	9.411	2497	2510	2539	rBV	448553	750521	75.35%	10.054%
64	9.610	2570	2572	2574	rBV	171	74	0.01%	0.001%
65	9.809	2632	2634	2636	rBV	233	105	0.01%	0.001%
66	9.845	2641	2645	2646	rBV	224	145	0.01%	0.002%
67	9.903	2661	2663	2666	rVB	249	117	0.01%	0.002%
68	10.076	2715	2717	2719	rBV2	183	118	0.01%	0.002%
69	10.157	2739	2742	2744	rBV	202	138	0.01%	0.002%
70	10.700	2908	2911	2914	rBV2	373	355	0.04%	0.005%
71	10.751	2915	2927	2945	rVV	279802	453524	45.53%	6.075%
72	10.928	2979	2982	2987	rBV2	304	271	0.03%	0.004%
73	10.954	2987	2990	2994	rVB2	341	257	0.03%	0.003%
74	11.806	3243	3255	3279	rBV	451016	712291	71.51%	9.542%
75	12.189	3360	3374	3393	rBV	416153	692949	69.57%	9.283%
76	12.880	3586	3589	3591	rBV	398	214	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053997.D
Acq On : 29 Apr 2023 19:36
Operator : JC/MD
Sample : 02565-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis




Sum of corrected areas: 7465069

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053997.D
Acq On : 29 Apr 2023 19:36
Operator : JC/MD
Sample : 02565-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

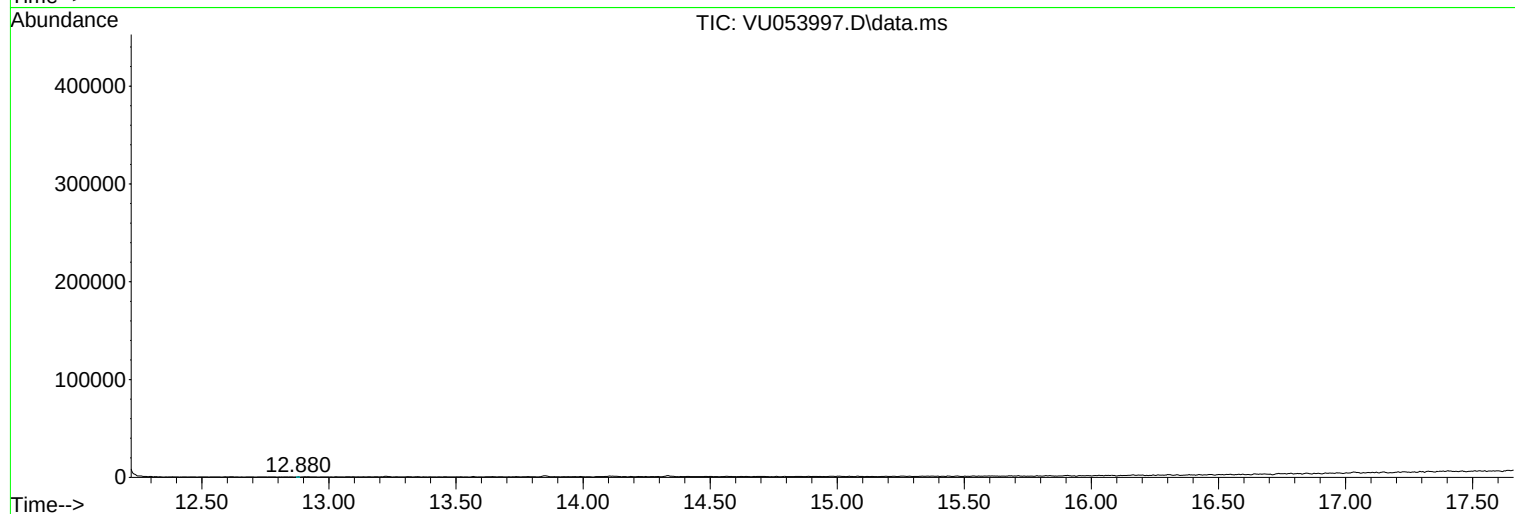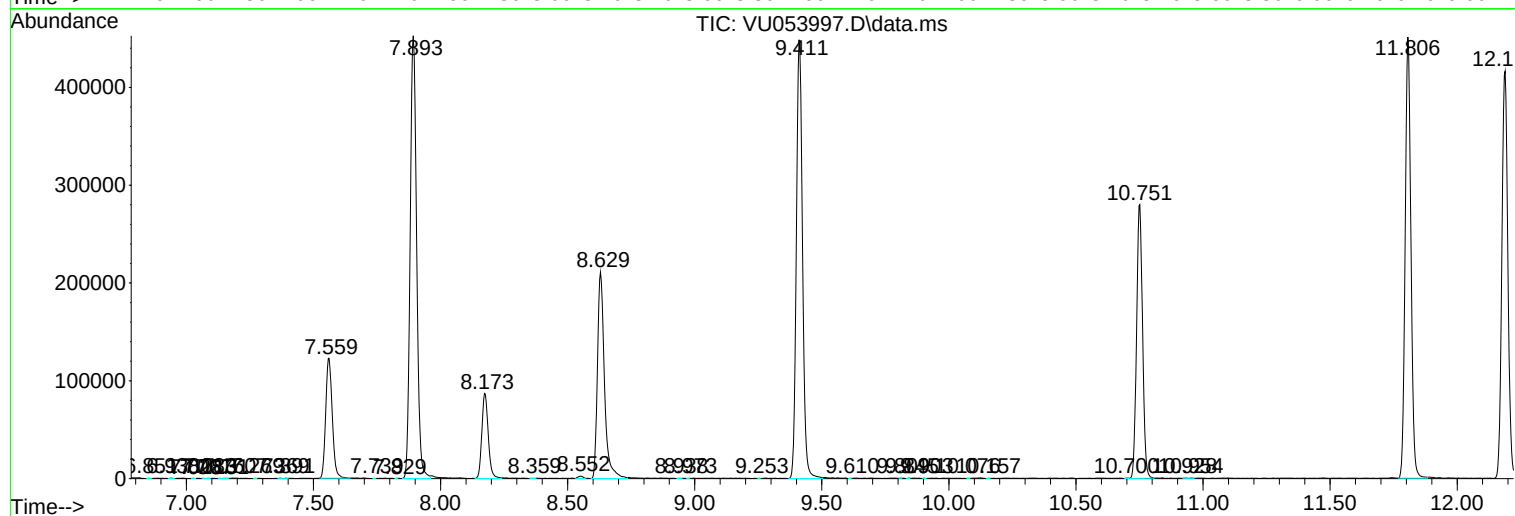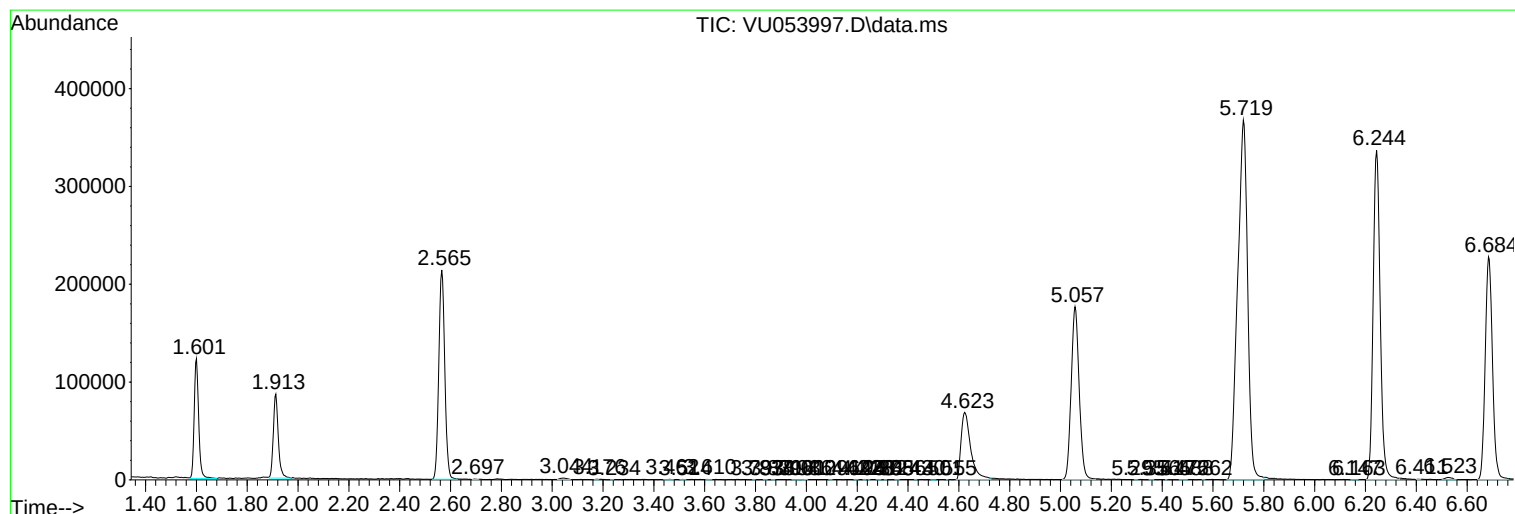

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053997.D
Acq On : 29 Apr 2023 19:36
Operator : JC/MD
Sample : 02565-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053997.D
Acq On : 29 Apr 2023 19:36
Operator : JC/MD
Sample : 02565-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc