

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053998.D
 Acq On : 29 Apr 2023 20:00
 Operator : JC/MD
 Sample : 02565-08 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU053998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB	121069	146803	14.55%	1.946%
2	1.816	146	148	151	rBV	787	464	0.05%	0.006%
3	1.912	169	178	195	rBV	87154	116798	11.57%	1.548%
4	2.565	366	381	404	rVB	214765	353490	35.03%	4.685%
5	2.710	421	426	427	rBV	346	259	0.03%	0.003%
6	2.784	442	449	451	rBV2	527	550	0.05%	0.007%
7	2.842	465	467	470	rBV	277	199	0.02%	0.003%
8	2.970	503	507	510	rBV2	333	268	0.03%	0.004%
9	3.015	517	521	524	rBV3	348	273	0.03%	0.004%
10	3.038	524	528	529	rBV2	683	556	0.06%	0.007%
11	3.141	556	560	564	rBV2	277	229	0.02%	0.003%
12	3.166	564	568	571	rVB3	299	218	0.02%	0.003%
13	3.250	591	594	599	rBV2	201	230	0.02%	0.003%
14	3.363	624	629	632	rBV2	249	317	0.03%	0.004%
15	3.539	681	684	689	rBV2	290	225	0.02%	0.003%
16	3.591	695	700	703	rBV	245	216	0.02%	0.003%
17	3.861	780	784	790	rVB2	250	238	0.02%	0.003%
18	3.896	790	795	797	rBV2	231	211	0.02%	0.003%
19	4.015	829	832	838	rBV2	253	251	0.02%	0.003%
20	4.154	870	875	877	rBV2	269	256	0.03%	0.003%
21	4.260	904	908	914	rVB2	269	302	0.03%	0.004%
22	4.363	937	940	942	rBV	305	200	0.02%	0.003%
23	4.424	955	959	964	rBV	161	224	0.02%	0.003%
24	4.527	988	991	993	rBV	244	193	0.02%	0.003%
25	4.581	1004	1008	1011	rBV2	230	226	0.02%	0.003%
26	4.626	1011	1022	1051	rBV2	67897	184599	18.29%	2.447%
27	5.057	1140	1156	1179	rBV	176810	394560	39.10%	5.229%
28	5.301	1228	1232	1234	rBV2	480	379	0.04%	0.005%
29	5.314	1234	1236	1239	rVV3	567	434	0.04%	0.006%
30	5.501	1289	1294	1299	rBV2	176	231	0.02%	0.003%
31	5.719	1341	1362	1391	rBV2	364246	1009102	100.00%	13.374%
32	6.044	1460	1463	1469	rVB2	229	217	0.02%	0.003%
33	6.243	1512	1525	1547	rBV	331897	634945	62.92%	8.415%
34	6.478	1596	1598	1603	rBV2	345	303	0.03%	0.004%
35	6.533	1603	1615	1628	rVB8	4708	9888	0.98%	0.131%
36	6.684	1648	1662	1693	rVV	231850	456848	45.27%	6.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053998.D
 Acq On : 29 Apr 2023 20:00
 Operator : JC/MD
 Sample : 02565-08 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.809	1695	1701	1709	rVB5	779	1097	0.11%	0.015%
38	6.899	1720	1729	1734	rBV2	254	500	0.05%	0.007%
39	7.025	1766	1768	1772	rVB	325	202	0.02%	0.003%
40	7.276	1840	1846	1854	rBV2	433	825	0.08%	0.011%
41	7.372	1872	1876	1883	rVV2	221	242	0.02%	0.003%
42	7.562	1922	1935	1963	rBV	126001	225429	22.34%	2.988%
43	7.893	2023	2038	2062	rBV	462143	802551	79.53%	10.637%
44	8.047	2082	2086	2089	rBV2	375	336	0.03%	0.004%
45	8.173	2114	2125	2144	rBV2	88602	150618	14.93%	1.996%
46	8.295	2160	2163	2168	rVB2	257	248	0.02%	0.003%
47	8.321	2168	2171	2173	rBV2	263	213	0.02%	0.003%
48	8.478	2217	2220	2228	rBV2	351	377	0.04%	0.005%
49	8.549	2235	2242	2251	rVB5	2166	3420	0.34%	0.045%
50	8.629	2256	2267	2298	rBV	221032	416455	41.27%	5.520%
51	8.784	2313	2315	2318	rVB	520	248	0.02%	0.003%
52	8.941	2360	2364	2367	rBV2	302	249	0.02%	0.003%
53	8.996	2377	2381	2385	rBV2	354	348	0.03%	0.005%
54	9.099	2404	2413	2418	rVB2	365	531	0.05%	0.007%
55	9.128	2418	2422	2423	rBV	307	215	0.02%	0.003%
56	9.321	2478	2482	2489	rVB	395	532	0.05%	0.007%
57	9.362	2489	2495	2498	rBV	448	414	0.04%	0.005%
58	9.411	2498	2510	2538	rBV	442524	742163	73.55%	9.836%
59	9.546	2549	2552	2555	rBV2	394	287	0.03%	0.004%
60	9.603	2567	2570	2571	rBV2	361	215	0.02%	0.003%
61	9.703	2592	2601	2605	rBV2	471	769	0.08%	0.010%
62	9.790	2624	2628	2632	rBV2	264	259	0.03%	0.003%
63	9.906	2659	2664	2667	rVB2	234	219	0.02%	0.003%
64	9.935	2670	2673	2678	rBV	250	202	0.02%	0.003%
65	10.102	2721	2725	2729	rVB2	336	269	0.03%	0.004%
66	10.124	2729	2732	2737	rVB2	394	273	0.03%	0.004%
67	10.449	2830	2833	2836	rBV2	259	240	0.02%	0.003%
68	10.587	2874	2876	2882	rVB	277	224	0.02%	0.003%
69	10.620	2882	2886	2889	rBV2	250	277	0.03%	0.004%
70	10.751	2911	2927	2947	rBV	287268	466865	46.27%	6.188%
71	11.037	3010	3016	3020	rVB2	221	266	0.03%	0.004%
72	11.079	3027	3029	3034	rVB2	340	294	0.03%	0.004%
73	11.401	3126	3129	3133	rVB	343	258	0.03%	0.003%
74	11.468	3147	3150	3152	rBV	333	231	0.02%	0.003%
75	11.500	3156	3160	3168	rBV2	312	422	0.04%	0.006%
76	11.581	3180	3185	3189	rBV2	314	367	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053998.D
 Acq On : 29 Apr 2023 20:00
 Operator : JC/MD
 Sample : 02565-08 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.738	3228	3234	3241	rVB5	906	1239	0.12%	0.016%
78	11.806	3241	3255	3277	rBV	447663	701146	69.48%	9.293%
79	12.144	3355	3360	3361	rBV2	510	367	0.04%	0.005%
80	12.189	3361	3374	3396	rVV	431055	700262	69.39%	9.281%
81	12.539	3478	3483	3485	rBV2	225	219	0.02%	0.003%
82	12.584	3494	3497	3500	rBV2	402	263	0.03%	0.003%
83	13.025	3629	3634	3637	rBV2	315	334	0.03%	0.004%
84	13.240	3698	3701	3706	rVB2	560	385	0.04%	0.005%
85	13.291	3713	3717	3722	rBV3	466	427	0.04%	0.006%
86	13.362	3736	3739	3744	rBV	250	196	0.02%	0.003%
87	13.494	3777	3780	3783	rBV	411	281	0.03%	0.004%
88	13.516	3783	3787	3793	rVV3	421	557	0.06%	0.007%
89	13.584	3806	3808	3811	rVB2	340	193	0.02%	0.003%
90	13.603	3811	3814	3816	rBV2	340	257	0.03%	0.003%
91	13.848	3885	3890	3896	rBV4	1002	1197	0.12%	0.016%
92	13.877	3896	3899	3902	rVV	347	247	0.02%	0.003%
93	14.047	3950	3952	3958	rVB3	566	431	0.04%	0.006%
94	14.330	4035	4040	4043	rBV4	998	996	0.10%	0.013%
95	14.539	4102	4105	4107	rBV2	314	222	0.02%	0.003%
96	14.565	4111	4113	4117	rBV	320	268	0.03%	0.004%
97	15.295	4338	4340	4343	rBV2	394	204	0.02%	0.003%
98	15.549	4416	4419	4425	rBV4	563	591	0.06%	0.008%
99	15.925	4532	4536	4540	rBV4	668	761	0.08%	0.010%
100	15.967	4547	4549	4552	rVB3	641	251	0.02%	0.003%


Sum of corrected areas: 7545146

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053998.D
Acq On : 29 Apr 2023 20:00
Operator : JC/MD
Sample : 02565-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

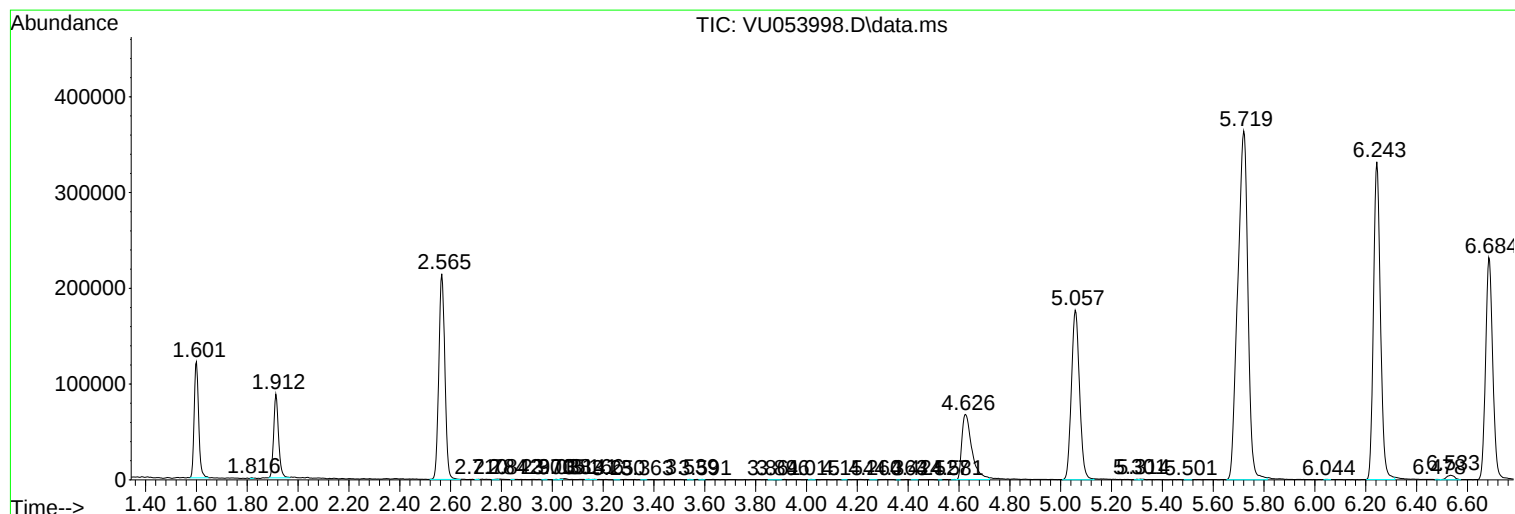

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053998.D
Acq On : 29 Apr 2023 20:00
Operator : JC/MD
Sample : 02565-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053998.D
Acq On : 29 Apr 2023 20:00
Operator : JC/MD
Sample : 02565-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc