

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053999.D
 Acq On : 29 Apr 2023 20:23
 Operator : JC/MD
 Sample : 02565-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU053999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	122060	145302	14.61%	1.959%
2	1.913	168	178	190	rBV	86831	115291	11.59%	1.554%
3	2.298	294	298	299	rBV2	296	224	0.02%	0.003%
4	2.478	351	354	356	rBV2	342	212	0.02%	0.003%
5	2.565	368	381	395	rBV	212262	344733	34.65%	4.648%
6	2.855	468	471	473	rBV2	378	250	0.03%	0.003%
7	3.041	523	529	538	rBV5	1376	2126	0.21%	0.029%
8	3.173	566	570	573	rBV2	400	317	0.03%	0.004%
9	3.282	601	604	609	rBV2	213	233	0.02%	0.003%
10	3.578	689	696	698	rBV2	213	225	0.02%	0.003%
11	3.613	703	707	709	rBV	288	231	0.02%	0.003%
12	3.752	745	750	752	rBV2	219	214	0.02%	0.003%
13	3.906	792	798	802	rBV2	235	215	0.02%	0.003%
14	4.019	831	833	842	rVB2	296	331	0.03%	0.004%
15	4.166	873	879	881	rBV2	274	258	0.03%	0.003%
16	4.240	897	902	904	rBV2	200	206	0.02%	0.003%
17	4.327	924	929	933	rVB2	250	318	0.03%	0.004%
18	4.623	1010	1021	1058	rBV	68388	184360	18.53%	2.486%
19	4.951	1118	1123	1125	rBV2	197	197	0.02%	0.003%
20	5.057	1133	1156	1177	rBV	176004	388848	39.09%	5.243%
21	5.154	1183	1186	1190	rVB3	373	242	0.02%	0.003%
22	5.388	1257	1259	1265	rVB2	434	429	0.04%	0.006%
23	5.417	1265	1268	1274	rBV2	360	475	0.05%	0.006%
24	5.491	1288	1291	1297	rVB	288	211	0.02%	0.003%
25	5.639	1333	1337	1341	rVB	274	244	0.02%	0.003%
26	5.719	1341	1362	1390	rBV2	363760	994850	100.00%	13.413%
27	6.096	1474	1479	1483	rBV2	257	287	0.03%	0.004%
28	6.244	1511	1525	1557	rBV	322890	620536	62.37%	8.366%
29	6.379	1564	1567	1571	rVB	511	309	0.03%	0.004%
30	6.481	1597	1599	1604	rBV3	323	308	0.03%	0.004%
31	6.530	1605	1614	1622	rVV9	2742	4482	0.45%	0.060%
32	6.684	1648	1662	1686	rBV	229280	449666	45.20%	6.063%
33	6.803	1696	1699	1704	rBV4	540	508	0.05%	0.007%
34	7.182	1811	1817	1819	rBV3	430	423	0.04%	0.006%
35	7.269	1840	1844	1847	rVB2	344	282	0.03%	0.004%
36	7.562	1922	1935	1962	rBV	123352	221753	22.29%	2.990%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053999.D
 Acq On : 29 Apr 2023 20:23
 Operator : JC/MD
 Sample : 02565-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	7.790	2002	2006	2013	rVB2	256	294	0.03%	0.004%
38	7.893	2025	2038	2058	rBV	453969	790687	79.48%	10.660%
39	8.173	2113	2125	2145	rBV	86518	149322	15.01%	2.013%
40	8.311	2165	2168	2172	rVB2	446	333	0.03%	0.004%
41	8.340	2173	2177	2178	rBV	418	249	0.03%	0.003%
42	8.462	2210	2215	2217	rBV3	296	310	0.03%	0.004%
43	8.546	2233	2241	2249	rVB7	2042	2998	0.30%	0.040%
44	8.629	2256	2267	2300	rBV	217857	410100	41.22%	5.529%
45	8.829	2326	2329	2335	rVB	332	243	0.02%	0.003%
46	8.858	2335	2338	2340	rBV2	303	191	0.02%	0.003%
47	8.874	2341	2343	2349	rVB2	389	229	0.02%	0.003%
48	8.919	2354	2357	2360	rBV	283	192	0.02%	0.003%
49	9.015	2383	2387	2393	rBV2	290	353	0.04%	0.005%
50	9.128	2416	2422	2427	rVB2	340	380	0.04%	0.005%
51	9.253	2458	2461	2470	rVB2	268	399	0.04%	0.005%
52	9.327	2482	2484	2491	rVB2	287	245	0.02%	0.003%
53	9.362	2491	2495	2498	rBV2	344	275	0.03%	0.004%
54	9.411	2498	2510	2539	rBV	430754	723727	72.75%	9.758%
55	9.925	2665	2670	2672	rBV2	297	313	0.03%	0.004%
56	10.102	2721	2725	2730	rVB2	211	213	0.02%	0.003%
57	10.234	2762	2766	2771	rBV	365	319	0.03%	0.004%
58	10.263	2771	2775	2778	rVV2	268	260	0.03%	0.004%
59	10.330	2792	2796	2800	rVB2	209	214	0.02%	0.003%
60	10.472	2837	2840	2844	rVV2	340	234	0.02%	0.003%
61	10.594	2874	2878	2880	rBV2	226	197	0.02%	0.003%
62	10.629	2887	2889	2897	rVB2	307	306	0.03%	0.004%
63	10.751	2914	2927	2945	rBV	286212	464334	46.67%	6.260%
64	10.919	2974	2979	2986	rVB2	189	306	0.03%	0.004%
65	11.070	3021	3026	3030	rBV2	219	331	0.03%	0.004%
66	11.099	3032	3035	3040	rVB2	434	307	0.03%	0.004%
67	11.234	3074	3077	3080	rBV2	311	260	0.03%	0.004%
68	11.279	3087	3091	3094	rBV2	343	289	0.03%	0.004%
69	11.513	3161	3164	3167	rBV	363	260	0.03%	0.004%
70	11.748	3232	3237	3243	rVB3	510	578	0.06%	0.008%
71	11.806	3243	3255	3273	rBV	428921	684302	68.78%	9.226%
72	11.989	3307	3312	3319	rBV2	293	450	0.05%	0.006%
73	12.028	3321	3324	3330	rVV2	186	201	0.02%	0.003%
74	12.189	3361	3374	3393	rBV	424583	691634	69.52%	9.325%
75	12.671	3520	3524	3527	rBV2	249	254	0.03%	0.003%
76	12.748	3545	3548	3554	rVB2	445	392	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU053999.D
 Acq On : 29 Apr 2023 20:23
 Operator : JC/MD
 Sample : 02565-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	12.877	3585	3588	3592	rVB2	308	287	0.03%	0.004%
78	12.902	3593	3596	3600	rBV	258	259	0.03%	0.003%
79	13.044	3634	3640	3643	rBV2	403	501	0.05%	0.007%
80	13.115	3659	3662	3665	rBV2	346	249	0.03%	0.003%
81	13.182	3681	3683	3691	rVB3	456	517	0.05%	0.007%
82	13.224	3691	3696	3697	rBV4	569	514	0.05%	0.007%
83	13.324	3721	3727	3731	rBV2	287	344	0.03%	0.005%
84	13.420	3754	3757	3759	rBV	343	220	0.02%	0.003%
85	13.520	3785	3788	3789	rBV2	272	192	0.02%	0.003%
86	13.613	3813	3817	3820	rBV2	366	245	0.02%	0.003%
87	13.729	3850	3853	3859	rBV3	354	386	0.04%	0.005%
88	13.771	3863	3866	3869	rVB2	422	255	0.03%	0.003%
89	13.844	3884	3889	3899	rBV4	925	1625	0.16%	0.022%
90	13.915	3907	3911	3914	rBV2	448	314	0.03%	0.004%
91	13.941	3917	3919	3922	rBV2	309	207	0.02%	0.003%
92	13.992	3930	3935	3938	rBV3	413	428	0.04%	0.006%
93	14.340	4036	4043	4048	rBV4	892	1316	0.13%	0.018%
94	14.410	4060	4065	4066	rBV2	337	283	0.03%	0.004%
95	14.430	4068	4071	4077	rVV2	474	428	0.04%	0.006%
96	14.475	4082	4085	4087	rBV2	299	200	0.02%	0.003%
97	14.568	4109	4114	4116	rBV2	506	482	0.05%	0.006%
98	14.918	4221	4223	4226	rBV2	400	266	0.03%	0.004%
99	15.732	4474	4476	4482	rVB3	723	566	0.06%	0.008%
100	16.574	4735	4738	4742	rBV5	1446	1411	0.14%	0.019%




Sum of corrected areas: 7417072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053999.D
Acq On : 29 Apr 2023 20:23
Operator : JC/MD
Sample : 02565-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

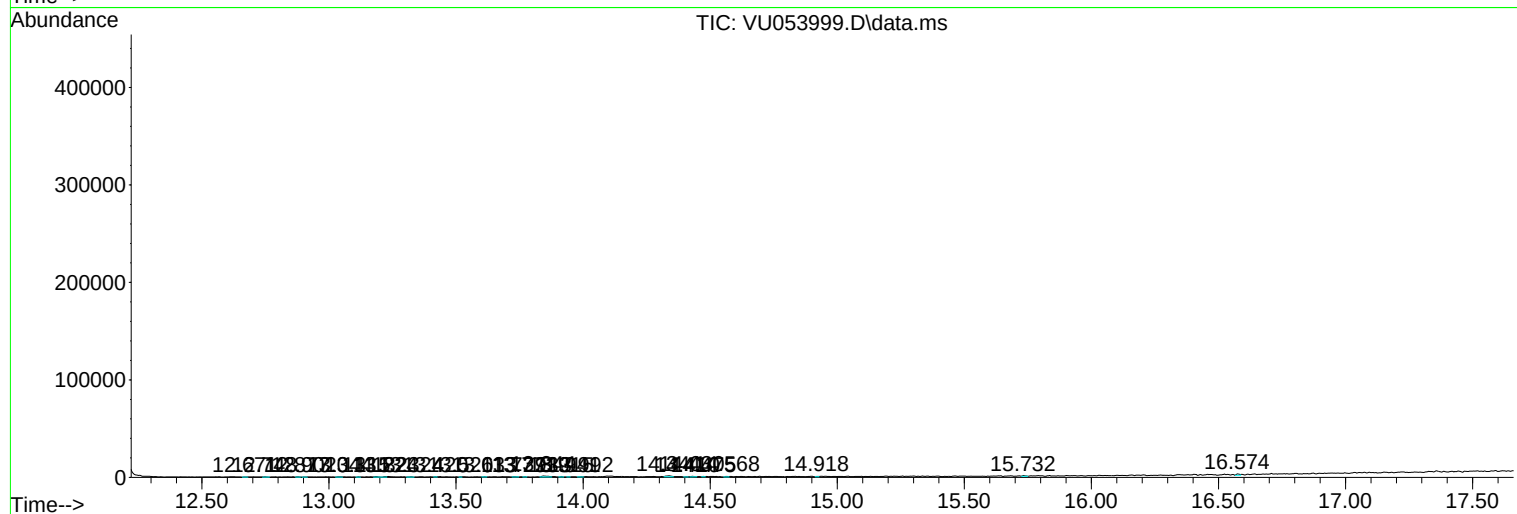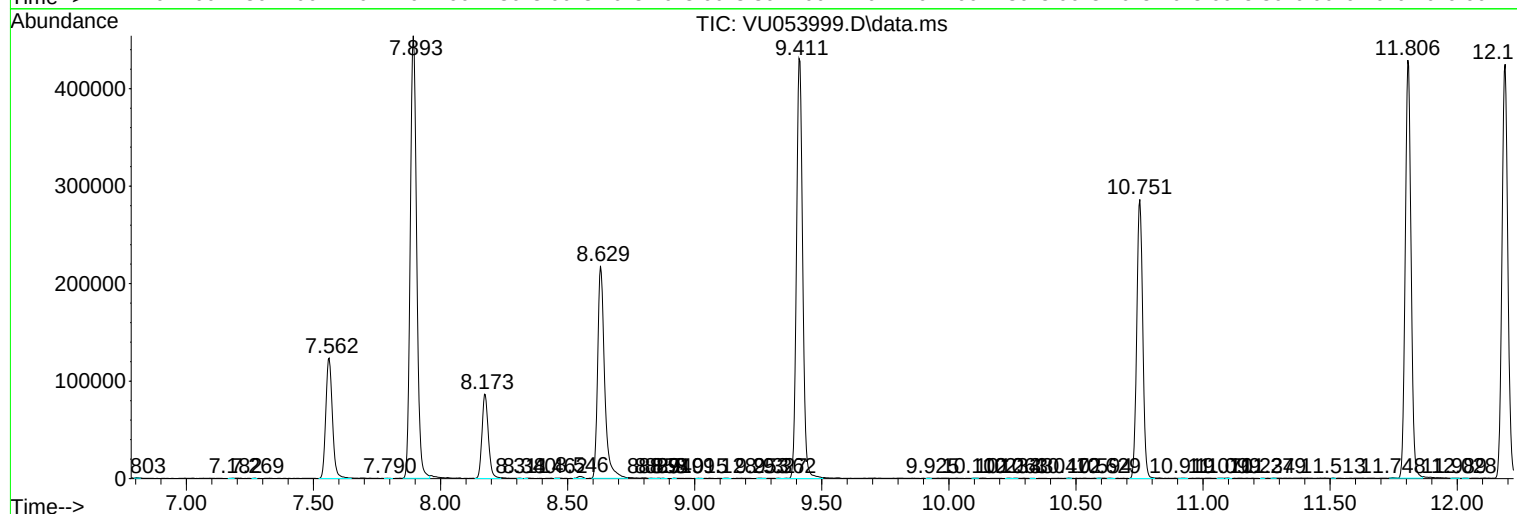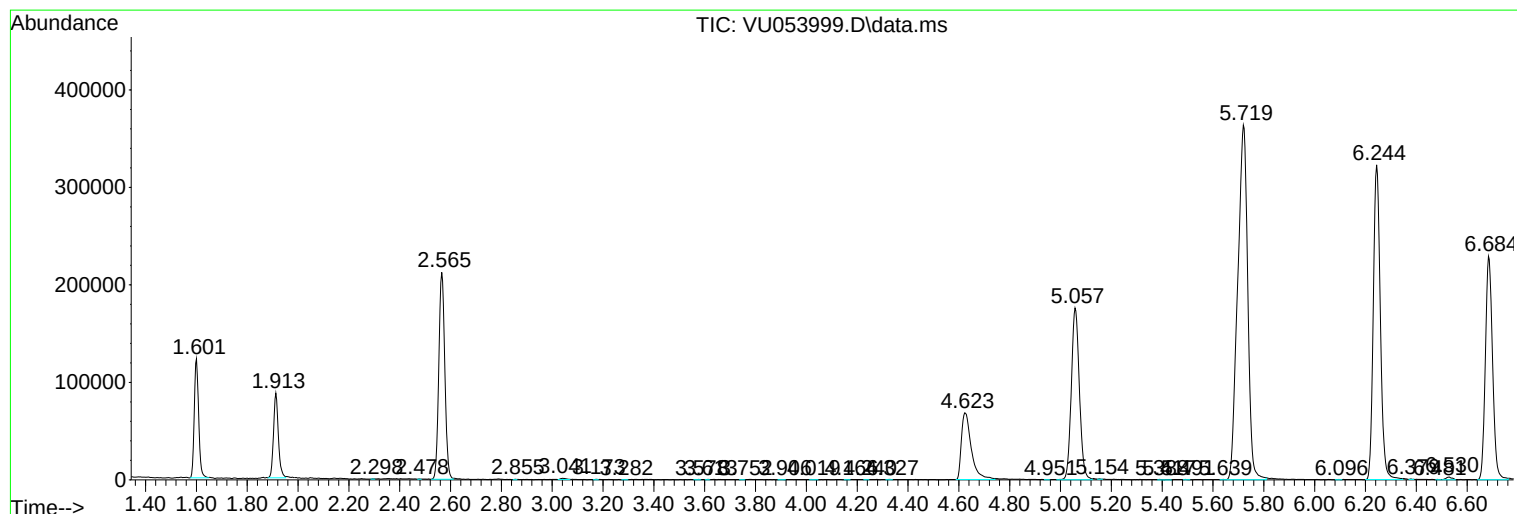

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053999.D
Acq On : 29 Apr 2023 20:23
Operator : JC/MD
Sample : 02565-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053999.D
Acq On : 29 Apr 2023 20:23
Operator : JC/MD
Sample : 02565-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------