

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU054010.D
 Acq On : 30 Apr 2023 00:42
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	100	rBV	169882	247232	13.39%	2.022%
2	1.906	169	176	193	rBV	96365	172171	9.32%	1.408%
3	2.549	363	376	393	rBV	387031	624713	33.83%	5.109%
4	2.871	473	476	478	rBV	255	186	0.01%	0.002%
5	2.887	479	481	484	rBV2	213	123	0.01%	0.001%
6	2.938	494	497	501	rBV	427	404	0.02%	0.003%
7	3.038	518	528	537	rBV4	2502	4886	0.26%	0.040%
8	3.176	567	571	576	rVB3	378	358	0.02%	0.003%
9	3.285	602	605	608	rBV	286	218	0.01%	0.002%
10	3.337	617	621	623	rBV	217	201	0.01%	0.002%
11	3.388	633	637	643	rBV2	234	254	0.01%	0.002%
12	3.530	678	681	685	rBV2	185	169	0.01%	0.001%
13	3.594	695	701	703	rBV2	387	388	0.02%	0.003%
14	3.642	713	716	717	rBV	206	141	0.01%	0.001%
15	3.678	724	727	731	rBV2	224	193	0.01%	0.002%
16	3.716	736	739	740	rBV	224	125	0.01%	0.001%
17	3.777	755	758	759	rBV	209	135	0.01%	0.001%
18	3.874	782	788	793	rBV3	323	445	0.02%	0.004%
19	3.957	811	814	817	rBV3	281	252	0.01%	0.002%
20	3.993	823	825	827	rBV	178	126	0.01%	0.001%
21	4.086	849	854	856	rBV	248	251	0.01%	0.002%
22	4.125	863	866	871	rBV2	217	172	0.01%	0.001%
23	4.150	871	874	877	rBV2	159	143	0.01%	0.001%
24	4.202	884	890	895	rBV2	234	242	0.01%	0.002%
25	4.260	905	908	912	rBV	236	158	0.01%	0.001%
26	4.411	953	955	958	rBV	228	155	0.01%	0.001%
27	4.430	958	961	966	rVV	214	239	0.01%	0.002%
28	4.459	967	970	974	rVB	260	162	0.01%	0.001%
29	4.523	986	990	995	rBV2	162	216	0.01%	0.002%
30	4.546	995	997	999	rBV2	215	136	0.01%	0.001%
31	4.633	1007	1024	1073	rBV	87824	336621	18.23%	2.753%
32	4.986	1129	1134	1138	rBV2	494	510	0.03%	0.004%
33	5.054	1138	1155	1186	rBV	312517	717526	38.85%	5.868%
34	5.398	1257	1262	1263	rBV	224	181	0.01%	0.001%
35	5.604	1318	1326	1328	rBV2	170	248	0.01%	0.002%
36	5.716	1339	1361	1386	rBV2	696469	1846857	100.00%	15.103%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU054010.D
 Acq On : 30 Apr 2023 00:42
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.977	1434	1442	1453	rBV6	1223	2701	0.15%	0.022%
38	6.080	1471	1474	1475	rBV	307	161	0.01%	0.001%
39	6.128	1486	1489	1495	rBV2	309	358	0.02%	0.003%
40	6.240	1511	1524	1549	rBV	316840	620472	33.60%	5.074%
41	6.523	1602	1612	1623	rBV6	5956	11493	0.62%	0.094%
42	6.607	1627	1638	1645	rBV4	2012	4019	0.22%	0.033%
43	6.684	1647	1662	1692	rVV	414641	825752	44.71%	6.753%
44	7.080	1781	1785	1788	rBV2	206	238	0.01%	0.002%
45	7.192	1812	1820	1823	rBV5	2262	2841	0.15%	0.023%
46	7.266	1841	1843	1847	rBV	210	172	0.01%	0.001%
47	7.298	1850	1853	1855	rVB	189	126	0.01%	0.001%
48	7.317	1855	1859	1862	rBV2	339	240	0.01%	0.002%
49	7.401	1881	1885	1887	rBV2	186	138	0.01%	0.001%
50	7.459	1900	1903	1907	rBV2	160	154	0.01%	0.001%
51	7.501	1913	1916	1918	rBV	154	128	0.01%	0.001%
52	7.559	1921	1934	1963	rVV	213319	410309	22.22%	3.355%
53	7.777	1999	2002	2008	rBV2	426	468	0.03%	0.004%
54	7.835	2017	2020	2024	rBV	219	172	0.01%	0.001%
55	7.893	2024	2038	2064	rBV	840048	1532716	82.99%	12.534%
56	8.176	2114	2126	2149	rBV	132436	287658	15.58%	2.352%
57	8.285	2157	2160	2167	rVB3	570	513	0.03%	0.004%
58	8.497	2223	2226	2228	rBV	168	120	0.01%	0.001%
59	8.549	2232	2242	2253	rVB7	2842	4395	0.24%	0.036%
60	8.655	2258	2275	2308	rBV	364017	765552	41.45%	6.261%
61	8.887	2343	2347	2349	rBV2	306	284	0.02%	0.002%
62	9.015	2385	2387	2391	rBV	296	169	0.01%	0.001%
63	9.054	2395	2399	2404	rBV	282	326	0.02%	0.003%
64	9.092	2409	2411	2414	rVB2	282	165	0.01%	0.001%
65	9.417	2492	2512	2541	rBV	396528	762706	41.30%	6.237%
66	9.568	2555	2559	2569	rVB3	757	1124	0.06%	0.009%
67	9.607	2569	2571	2573	rBV2	203	123	0.01%	0.001%
68	9.649	2582	2584	2587	rBV	245	185	0.01%	0.002%
69	9.745	2611	2614	2616	rBV2	308	157	0.01%	0.001%
70	9.867	2649	2652	2655	rBV	259	199	0.01%	0.002%
71	9.906	2659	2664	2666	rBV	169	163	0.01%	0.001%
72	10.044	2703	2707	2710	rBV2	203	193	0.01%	0.002%
73	10.086	2717	2720	2722	rBV	390	267	0.01%	0.002%
74	10.481	2840	2843	2845	rBV2	177	126	0.01%	0.001%
75	10.536	2855	2860	2863	rBV2	237	261	0.01%	0.002%
76	10.645	2891	2894	2895	rBV	405	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
 Data File : VU054010.D
 Acq On : 30 Apr 2023 00:42
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	10.684	2903	2906	2909	rVB2	197	159	0.01%	0.001%
78	10.758	2915	2929	2946	rBV	539627	876606	47.46%	7.169%
79	10.906	2972	2975	2980	rBV3	402	286	0.02%	0.002%
80	10.993	2997	3002	3003	rBV	185	162	0.01%	0.001%
81	11.028	3010	3013	3017	rBV	223	177	0.01%	0.001%
82	11.057	3019	3022	3026	rVB	342	255	0.01%	0.002%
83	11.086	3026	3031	3036	rBV2	492	601	0.03%	0.005%
84	11.115	3036	3040	3046	rVB2	824	694	0.04%	0.006%
85	11.150	3046	3051	3052	rBV2	231	197	0.01%	0.002%
86	11.308	3096	3100	3103	rBV3	552	436	0.02%	0.004%
87	11.485	3148	3155	3159	rBV3	525	637	0.03%	0.005%
88	11.616	3192	3196	3198	rBV2	291	290	0.02%	0.002%
89	11.658	3207	3209	3212	rBV2	213	170	0.01%	0.001%
90	11.739	3231	3234	3236	rBV2	334	233	0.01%	0.002%
91	11.809	3244	3256	3281	rBV	478388	750170	40.62%	6.135%
92	12.028	3321	3324	3326	rBV	241	166	0.01%	0.001%
93	12.189	3361	3374	3394	rBV	873502	1401067	75.86%	11.458%
94	12.375	3430	3432	3436	rVB	304	158	0.01%	0.001%
95	12.722	3537	3540	3544	rBV2	254	192	0.01%	0.002%
96	13.713	3846	3848	3849	rBV	405	179	0.01%	0.001%
97	13.774	3864	3867	3869	rBV2	350	216	0.01%	0.002%
98	13.796	3871	3874	3876	rBV2	336	275	0.01%	0.002%
99	14.092	3963	3966	3968	rBV3	514	373	0.02%	0.003%
100	15.176	4300	4303	4305	rBV2	599	406	0.02%	0.003%




Sum of corrected areas: 12228212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU054010.D
Acq On : 30 Apr 2023 00:42
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

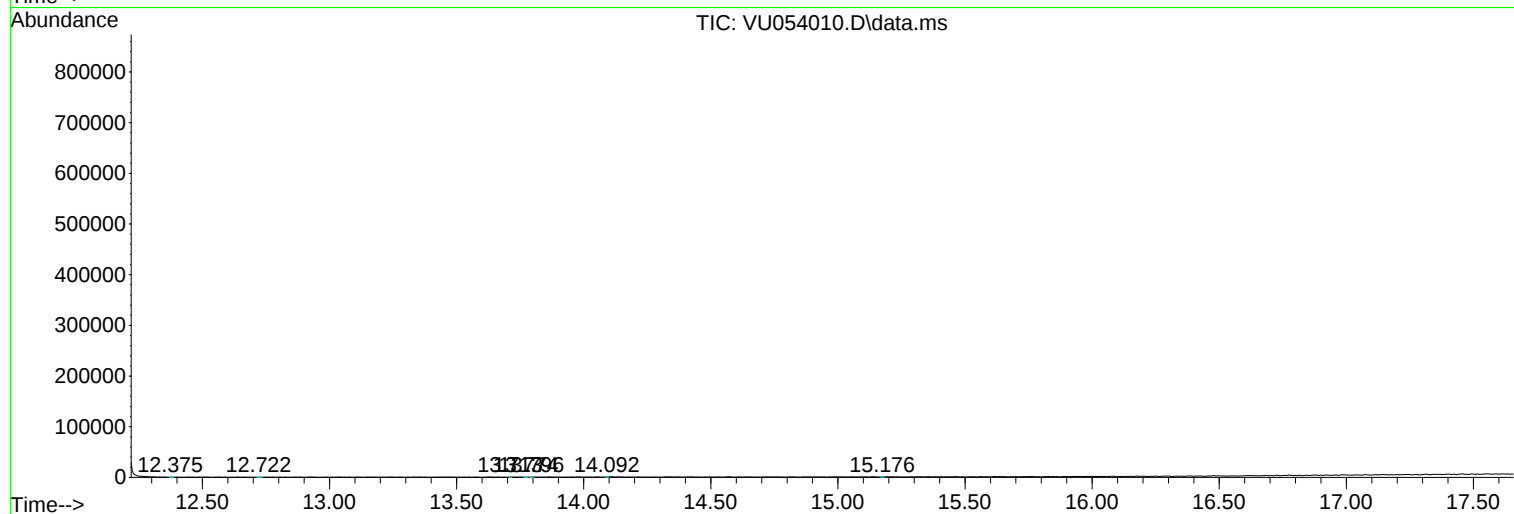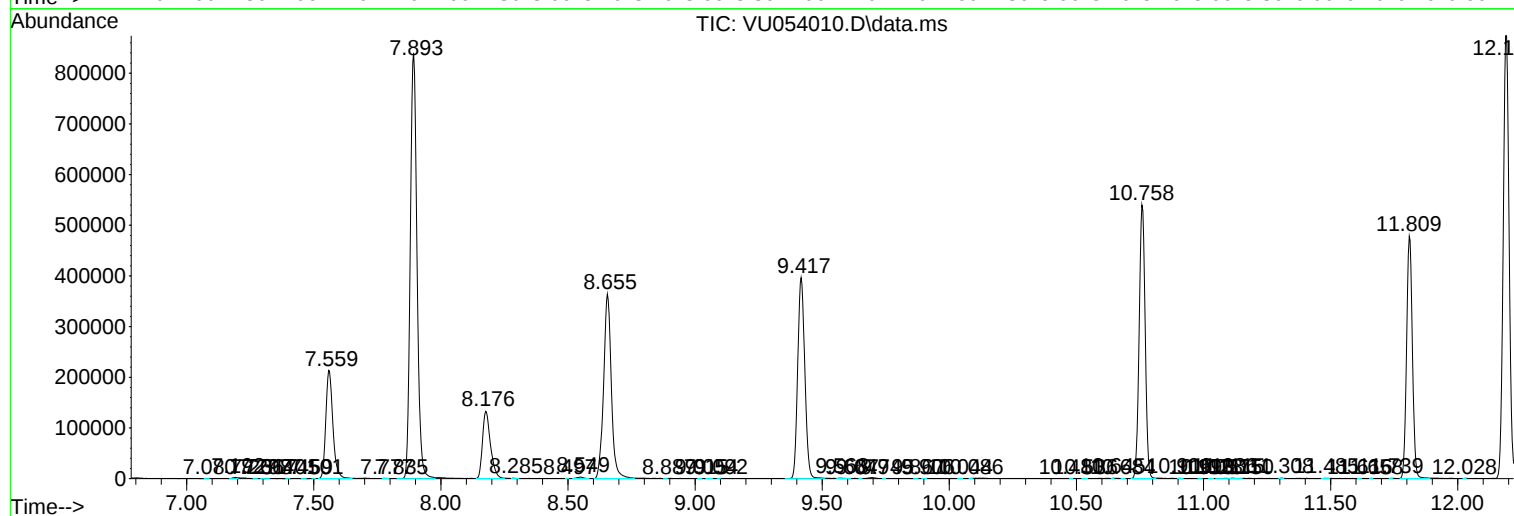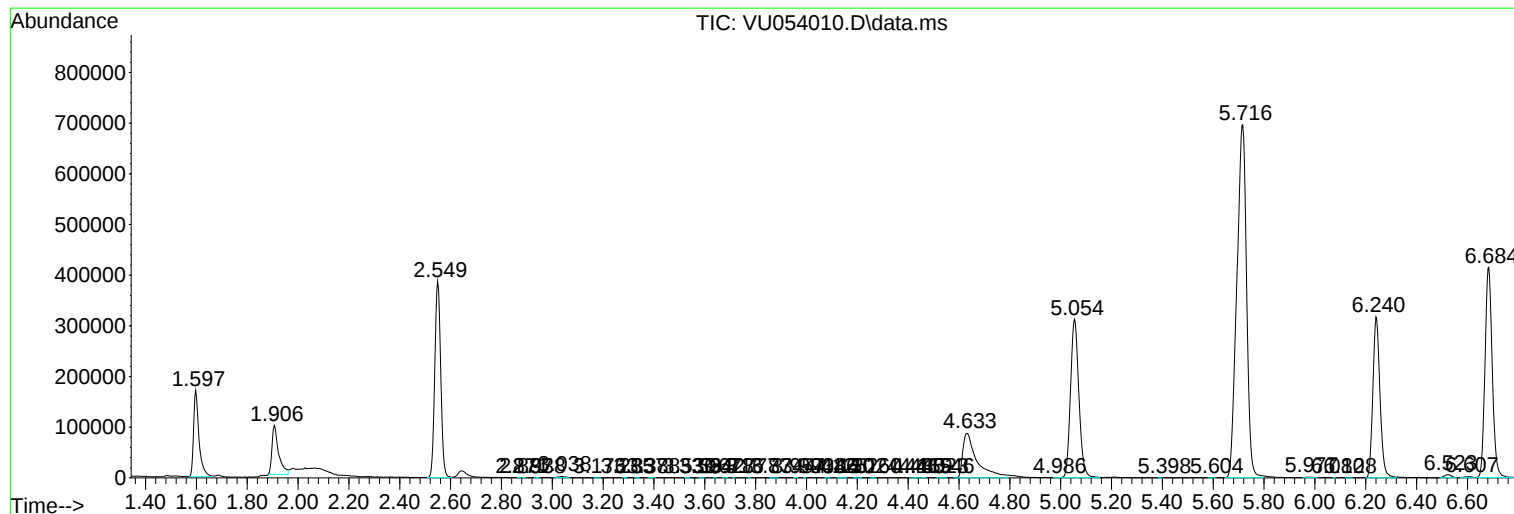

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU054010.D
Acq On : 30 Apr 2023 00:42
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU054010.D
Acq On : 30 Apr 2023 00:42
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc