


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043023\
Data File : VU053980.D
Acq On : 29 Apr 2023 12:20
Operator : JC/MD
Sample : BFB182
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB182

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis
Last Update : Tue May 02 05:29:54 2023

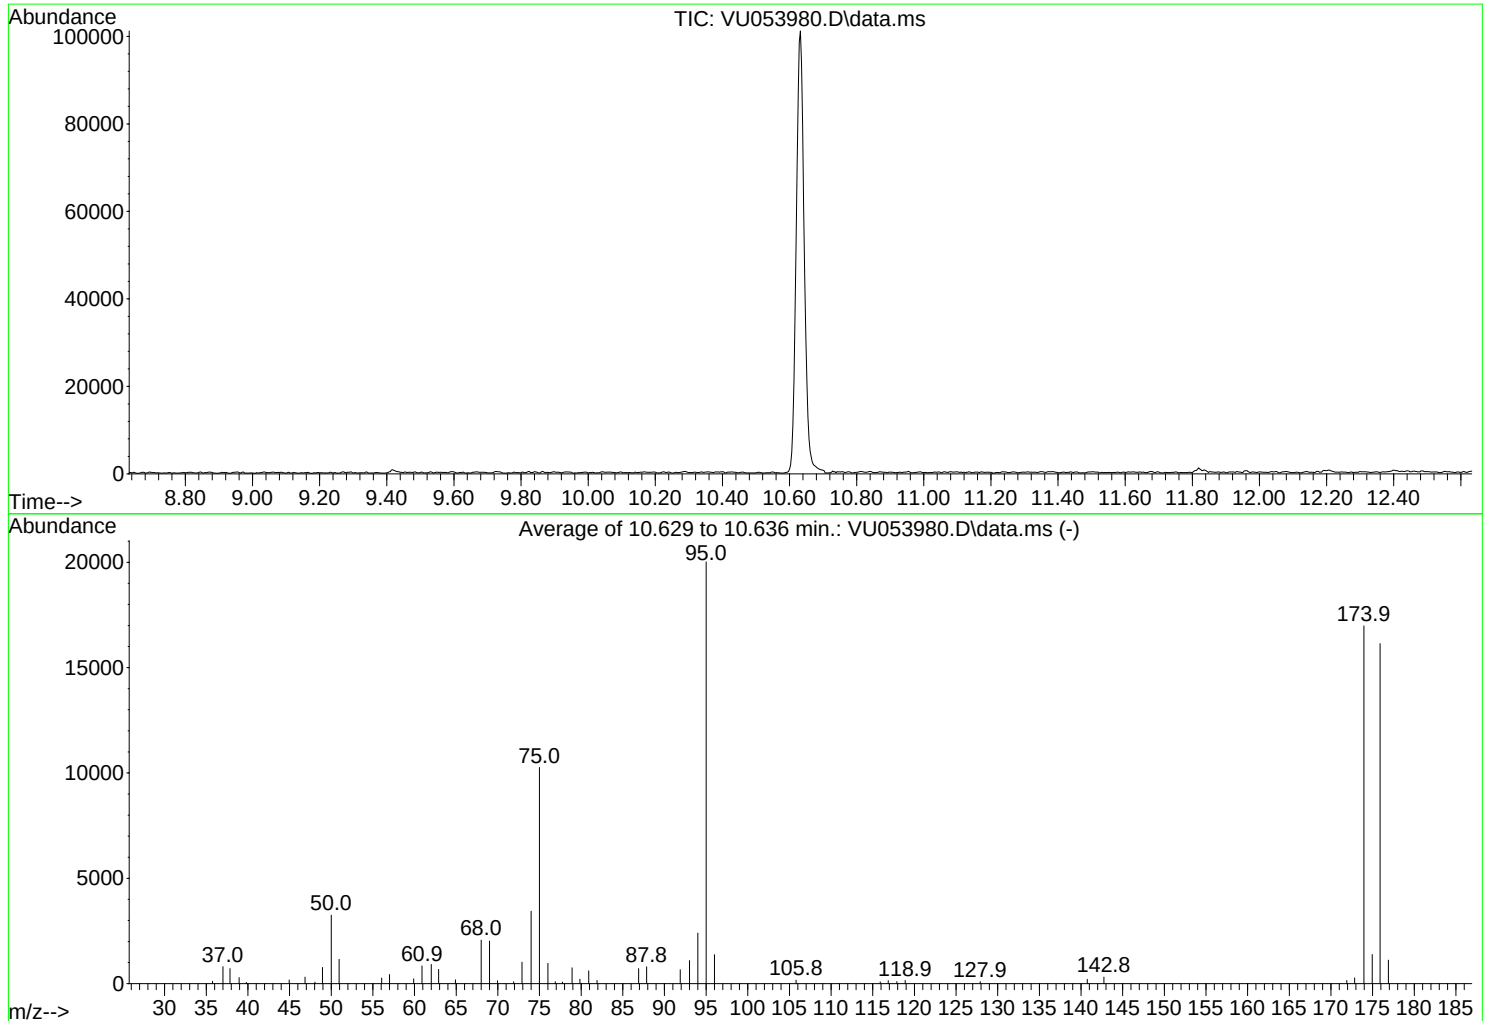

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	3247	PASS
75	95	30	80	51.2	10260	PASS
95	95	100	100	100.0	20021	PASS
96	95	5	9	6.9	1376	PASS
173	174	0.00	2	1.6	271	PASS
174	95	50	120	84.8	16979	PASS
175	174	5	9	8.1	1381	PASS
176	174	95	101	95.0	16136	PASS
177	176	5	9	6.9	1115	PASS

m/z	Abundance
39.80	107.0
43.90	300.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
35.80	111.0
37.00	787.0
37.90	706.0
38.90	355.0
39.90	167.0
44.00	343.0
45.00	166.0
46.80	317.0
48.00	118.0
48.90	799.0
50.00	3154.0
51.00	1255.0
56.00	269.0
57.00	463.0
59.90	201.0
60.90	893.0
62.00	899.0
62.90	766.0
65.00	147.0
68.00	2090.0
69.00	2090.0
70.00	111.0
71.90	136.0
72.90	1075.0
74.00	3503.0
75.00	10424.0
76.00	1010.0
77.70	137.0
78.90	750.0
79.90	196.0
80.90	660.0
81.90	188.0
86.90	669.0
87.80	813.0
91.90	632.0
93.00	1088.0
94.00	2405.0
95.00	20496.0
96.00	1533.0
105.80	149.0
115.90	129.0
116.80	157.0
118.90	146.0
140.70	212.0
142.70	232.0
171.80	147.0
172.90	262.0
174.00	16552.0
174.90	1442.0
175.90	16191.0
176.90	1127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
35.70	119.0
37.00	834.0
37.90	764.0
38.90	290.0
39.80	168.0
44.00	278.0
44.90	176.0
46.90	322.0
48.10	110.0
48.90	794.0
50.00	3298.0
51.00	1212.0
56.10	283.0
57.00	423.0
59.90	226.0
60.90	863.0
62.00	951.0
62.90	693.0
64.90	187.0
68.00	2144.0
69.00	2090.0
69.90	137.0
71.90	130.0
72.90	1049.0
74.00	3566.0
75.00	10541.0
76.00	983.0
76.90	115.0
77.80	100.0
78.90	774.0
79.80	217.0
80.90	633.0
81.90	156.0
86.90	725.0
87.90	805.0
91.90	697.0
93.00	1140.0
94.00	2502.0
95.00	20672.0
96.00	1382.0
105.80	174.0
115.90	129.0
116.80	137.0
117.90	146.0
118.90	152.0
127.90	119.0
140.70	213.0
142.70	326.0
171.90	151.0
172.80	286.0
173.90	17664.0
174.90	1397.0
175.90	16608.0
176.90	1147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
35.80	120.0
37.00	791.0
37.80	665.0
39.00	217.0
39.80	163.0
44.00	253.0
44.90	184.0
46.90	293.0
49.00	719.0
50.00	3288.0
50.90	1001.0
56.00	237.0
57.00	412.0
59.90	259.0
60.90	763.0
62.00	892.0
62.90	559.0
64.80	205.0
68.00	1967.0
69.00	1881.0
69.90	155.0
72.90	930.0
74.00	3255.0
75.00	9815.0
76.00	896.0
76.90	149.0
78.90	725.0
79.80	234.0
80.90	540.0
81.80	113.0
86.90	756.0
87.90	776.0
91.90	653.0
93.00	1048.0
94.00	2302.0
95.00	18896.0
96.00	1213.0
105.80	168.0
116.90	133.0
117.90	152.0
118.90	152.0
127.90	169.0
140.80	200.0
142.80	367.0
172.00	166.0
172.80	264.0
173.90	16720.0
175.00	1304.0
175.90	15610.0
176.90	1072.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182