


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050118\
 Data File : VU023544.D
 Acq On : 01 May 2018 09:44
 Operator : MD/SY
 Sample : BFB45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Title : VOC Analysis
 Last Update : Wed May 02 03:12:05 2018

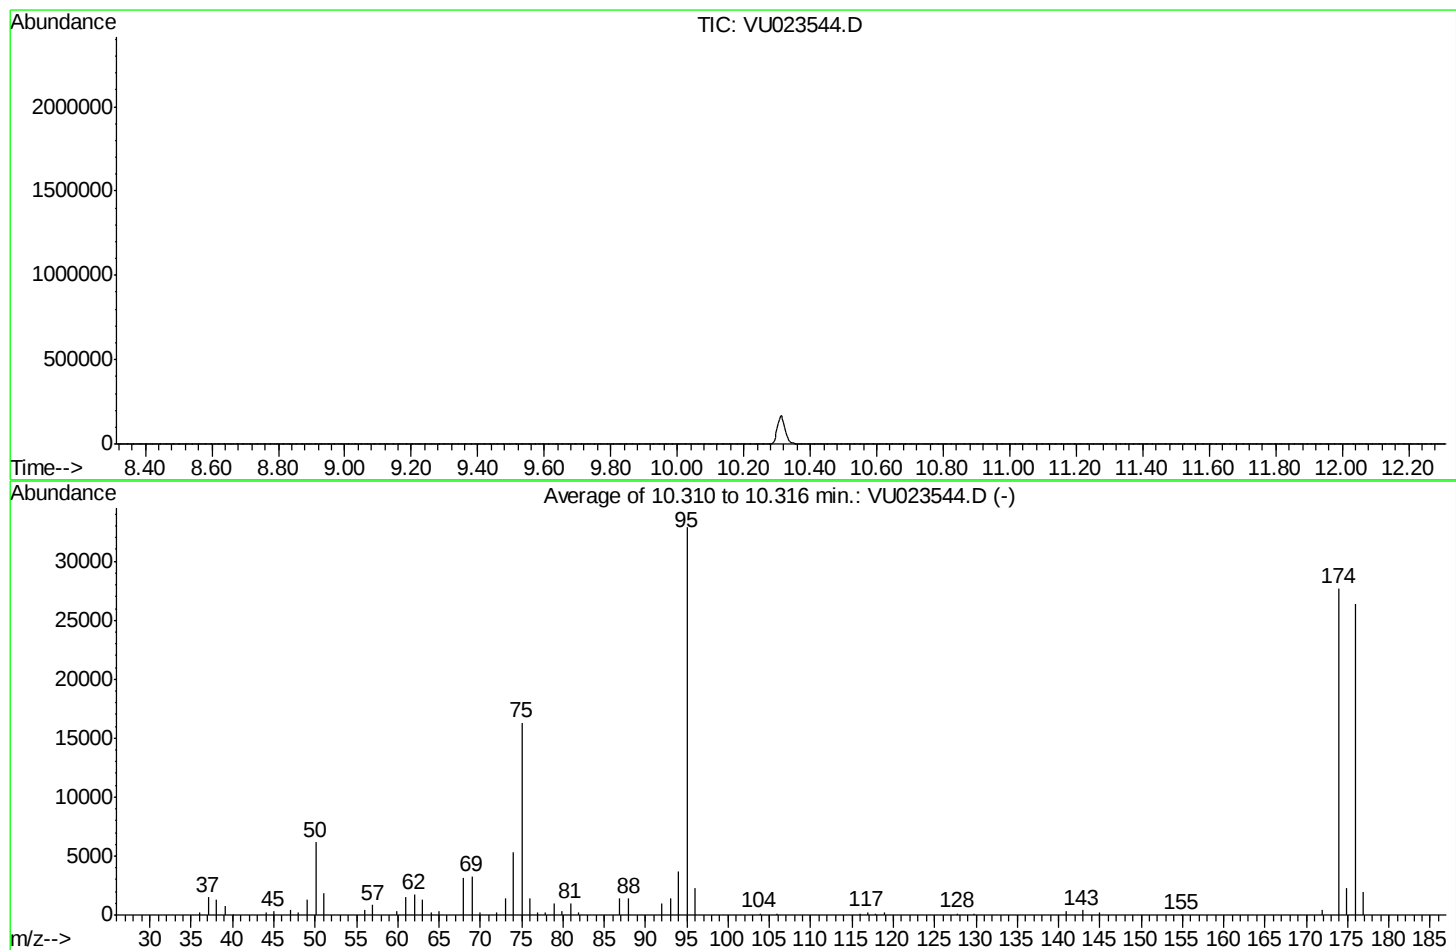

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	6172	PASS
75	95	30	80	49.6	16298	PASS
95	95	100	100	100.0	32877	PASS
96	95	5	9	6.9	2255	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	27648	PASS
175	174	5	9	8.1	2238	PASS
176	174	95	101	95.3	26357	PASS
177	176	5	9	7.5	1984	PASS

Scan 3011 (10.271 min): VU023544.D
BFB45

m/z	Abundance
40.00	111.0
44.00	401.0

Scan 3023 (10.310 min): VU023544.D
BFB45

m/z	Abundance
35.90	272.0
37.00	1497.0
38.00	1406.0
39.00	799.0
40.10	158.0
44.00	554.0
45.00	293.0
47.00	439.0
48.00	231.0
49.10	1399.0
50.00	6460.0
51.10	1828.0
56.00	542.0
57.00	887.0
60.00	355.0
61.00	1551.0
62.00	1727.0
63.00	1338.0
64.00	264.0
65.00	396.0
68.00	3377.0
69.00	3305.0
69.90	237.0
72.00	183.0
73.00	1467.0
74.00	5627.0
75.00	16760.0
76.00	1463.0
76.90	205.0
77.80	190.0
78.90	995.0
79.80	372.0
80.90	939.0
82.00	194.0
86.90	1503.0
88.00	1399.0
91.90	984.0
93.00	1489.0
94.00	3793.0
95.00	33528.0
96.00	2304.0
103.80	161.0
105.80	159.0
115.90	107.0
116.80	246.0
117.80	124.0
118.90	222.0
127.80	114.0
140.90	294.0
142.90	416.0
144.90	232.0
154.90	108.0
171.90	487.0
173.90	27416.0
174.90	2263.0
175.90	26528.0
176.90	1978.0

m/z	Abundance
35.90	258.0
37.00	1561.0
38.00	1352.0
39.00	792.0
40.10	160.0
44.00	606.0
45.00	323.0
47.00	465.0
48.00	225.0
49.00	1363.0
50.00	6365.0
51.10	1893.0
56.00	482.0
57.00	857.0
60.00	364.0
61.00	1563.0
62.00	1768.0
63.00	1367.0
64.00	262.0
65.00	380.0
68.00	3299.0
69.00	3322.0
70.00	250.0
72.00	190.0
73.00	1482.0
74.00	5487.0
75.00	16792.0
76.00	1453.0
76.90	170.0
77.90	168.0
78.90	992.0
79.90	347.0
80.90	993.0
81.90	207.0
86.90	1454.0
88.00	1486.0
91.90	964.0
93.00	1466.0
94.00	3854.0
95.00	33880.0
96.00	2360.0
103.90	168.0
105.80	133.0
115.90	105.0
116.90	263.0
117.80	109.0
118.90	220.0
127.80	115.0
129.80	123.0
140.90	318.0
142.90	419.0
144.90	241.0
171.90	492.0
174.00	28432.0
174.90	2330.0
175.90	27312.0
177.00	2048.0

Scan 3025 (10.316 min): VU023544.D
BFB45

m/z	Abundance
36.00	237.0
37.10	1431.0
38.00	1214.0
39.10	663.0
40.10	168.0
44.00	632.0
45.00	299.0
47.00	390.0
47.90	195.0
49.00	1204.0
50.10	5691.0
51.10	1720.0
56.00	407.0
57.00	738.0
59.90	341.0
61.00	1418.0
62.00	1595.0
63.00	1316.0
64.00	222.0
65.00	325.0
68.00	2889.0
69.00	3114.0
70.00	225.0
72.00	155.0
73.00	1361.0
74.00	4961.0
75.00	15344.0
76.00	1312.0
76.90	151.0
77.90	147.0
78.90	924.0
79.90	280.0
80.90	930.0
81.90	200.0
86.90	1260.0
87.90	1348.0
92.00	840.0
93.00	1309.0
94.00	3534.0
95.00	31224.0
96.10	2101.0
103.90	157.0
105.90	106.0
116.90	260.0
118.80	195.0
127.80	102.0
129.80	148.0
140.90	320.0
142.90	410.0
144.90	208.0
171.90	437.0
174.00	27096.0
174.90	2123.0
175.90	25232.0
177.00	1928.0