

Data File : VU031675.D
Acq On : 01 May 2019 11:37
Operator : JC/SP
Sample : K2604-12 5X
Misc : 5.09g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAJ86

Quant Time: May 02 02:26:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 02:23:23 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	1049490	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	1002501	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	473012	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	347575	39.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.14%
7) Chloroethane-d5	1.68	69	272027	40.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.16%
11) 1,1-Dichloroethene-d2	2.26	63	532743	30.46	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.92%
21) 2-Butanone-d5	4.18	46	764246	96.03	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.03%
24) Chloroform-d	4.64	84	632720	39.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.66%
26) 1,2-Dichloroethane-d4	5.30	65	426761	40.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.22%
32) Benzene-d6	5.33	84	1301297	42.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.54%
36) 1,2-Dichloropropane-d6	6.32	67	464301	42.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.74%
41) Toluene-d8	7.56	98	1141765	42.58	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.16%
43) trans-1,3-Dichloropropene-	7.85	79	200687	43.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.34%
47) 2-Hexanone-d5	8.31	63	508751	108.53	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.53%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	621539	42.76	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.52%
64) 1,2-Dichlorobenzene-d4	11.86	152	427043	42.93	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.86%

Target Compounds


					Qvalue
42) Toluene	7.63	91	266119	7.248 ug/L	98
44) trans-1,3-Dichloropropene	7.85	75	8367	0.667 ug/L #	71
48) 2-Hexanone	8.31	43	66526	5.109 ug/L #	70
52) Ethylbenzene	9.25	91	7632006	200.393 ug/L	100
53) m,p-Xylene	9.37	106	1237155	93.234 ug/L	97
54) o-xylene	9.77	106	1360435	103.414 ug/L	96
55) Styrene	9.79	104	688574	30.637 ug/L	87
56) Isopropylbenzene	10.16	105	69293	2.003 ug/L	98
70) 1,2,3-Trichlorobenzene	13.94	180	7760	0.734 ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU031675.D
Acq On : 01 May 2019 11:37
Operator : JC/SP
Sample : K2604-12 5X
Misc : 5.09g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAJ86

Quant Time: May 02 02:26:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 02:23:23 2019
Response via : Initial Calibration

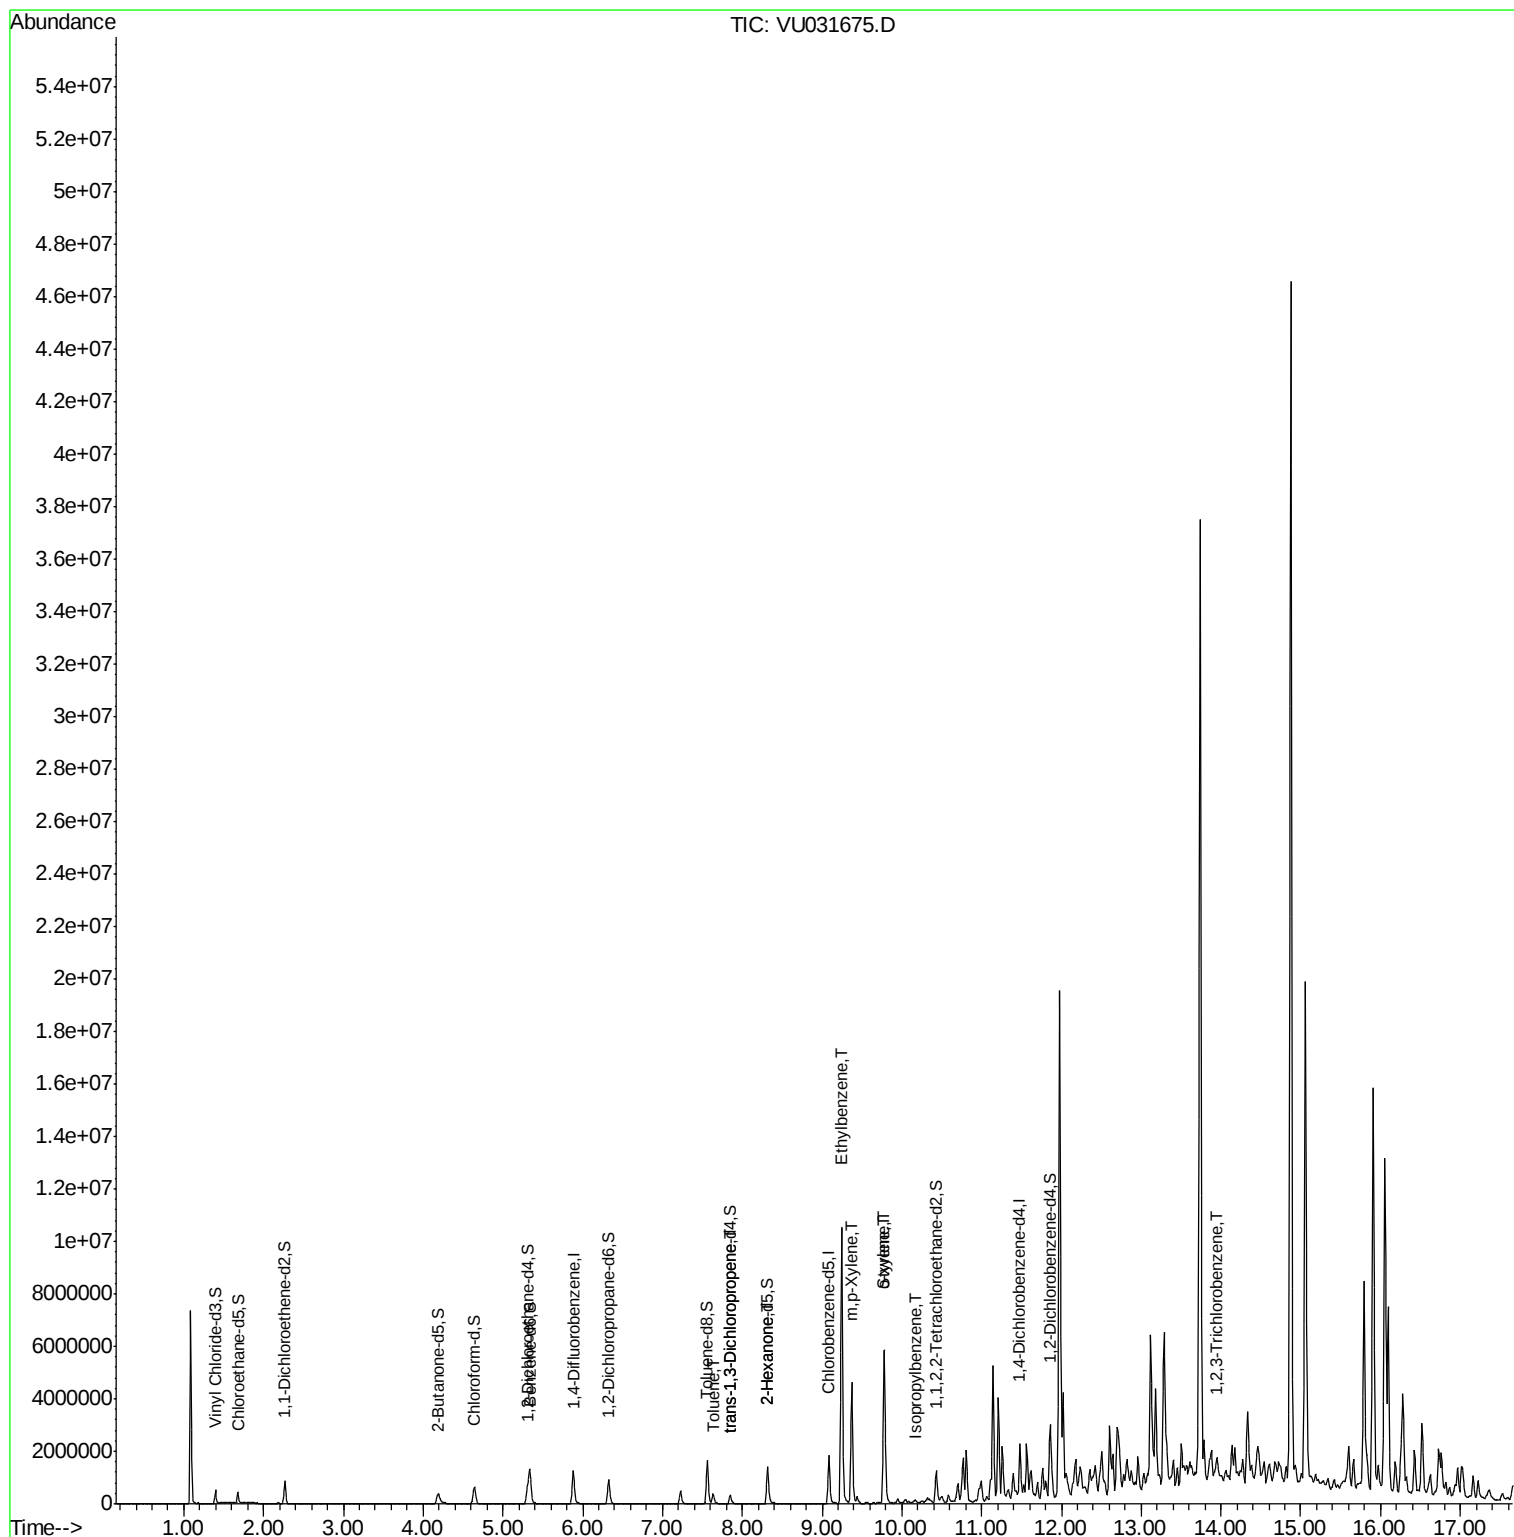

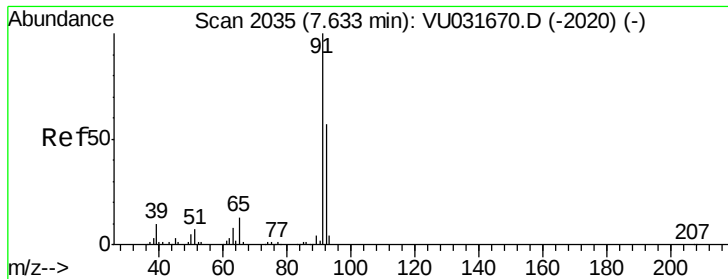

#42

Toluene

Concen: 7.248 ug/L

RT: 7.63 min Scan# 2328

Delta R.T. -0.00 min

Lab File: VU031675.D

Acq: 01 May 2019 11:37

Instrument :

MSVOA_U

ClientSampleId :


GAJ86

Tgt Ion: 91 Resp: 266119

Ion Ratio Lower Upper

91 100

92 54.2 39.0 72.4

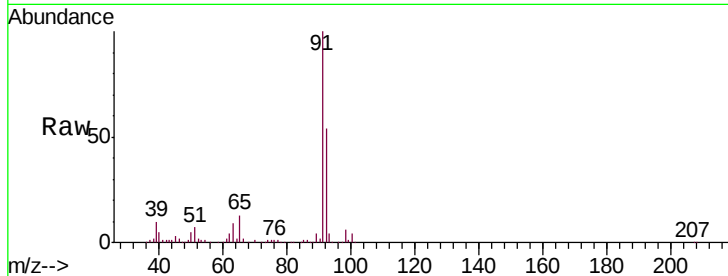

Abundance Ion 91.00 (90.70 to 91.70): VU031675.D (-2235) (-)

Ion 92.00 (91.70 to 92.70): VU031675.D (-2235) (-)

7.63

150000



100000

50000

0

7.55 7.60 7.65 7.70 7.75

Time-->

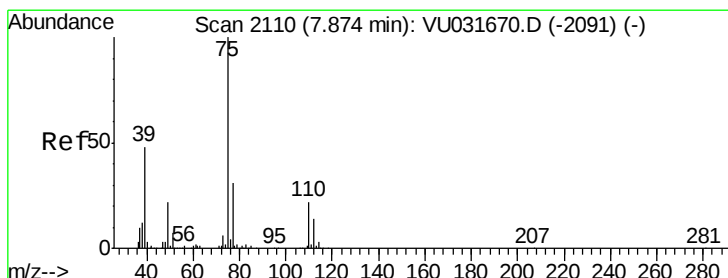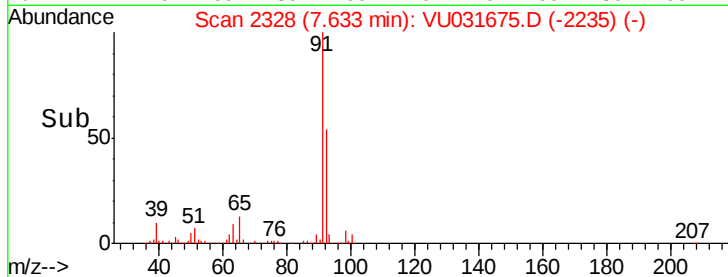

#44

trans-1,3-Dichloropropene

Concen: 0.667 ug/L

RT: 7.85 min Scan# 2396

Delta R.T. -0.02 min

Lab File: VU031675.D


Acq: 01 May 2019 11:37

Tgt Ion: 75 Resp: 8367

Ion Ratio Lower Upper

75 100

77 47.9 22.1 41.1#

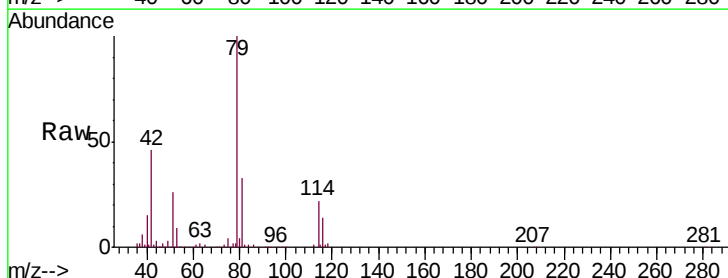

Abundance Ion 75.00 (74.70 to 75.70): VU031675.D (-2310) (-)

Ion 77.00 (76.70 to 77.70): VU031675.D (-2310) (-)

7.85

5000

4000

3000


2000


1000

0

7.80 7.85 7.90

Time-->




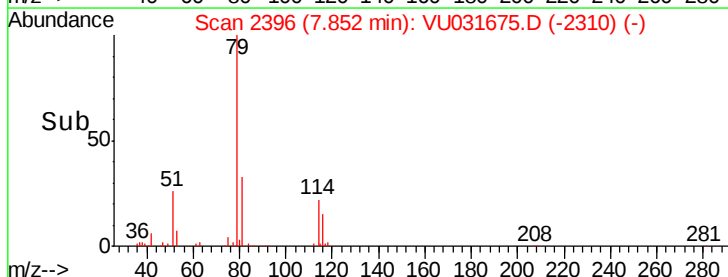


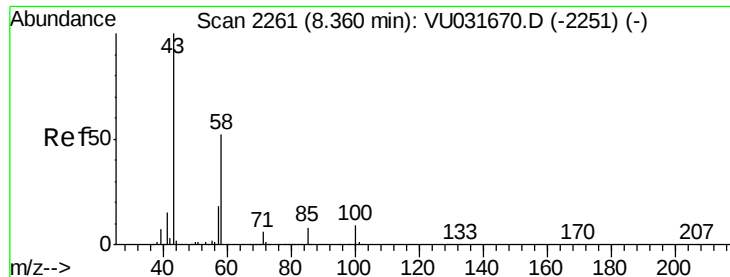

#48
2-Hexanone
Concen: 5.109 ug/L
RT: 8.31 min Scan# 2540
Delta R.T. -0.05 min
Lab File: VU031675.D
Acq: 01 May 2019 11:37




Instrument :
MSVOA_U
ClientSampleId :
GAJ86


Tgt Ion: 43 Resp: 66526
Ion Ratio Lower Upper
43 100
58 26.9 42.1 63.1#
57 23.9 14.6 22.0#
100 0.2 7.2 10.8#

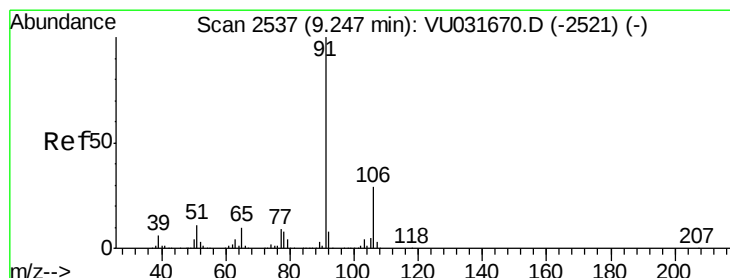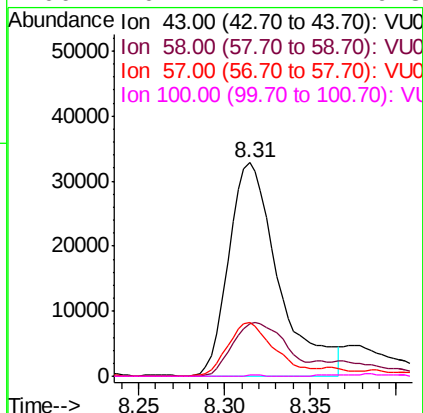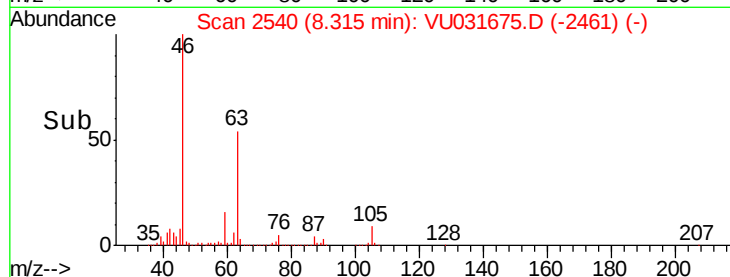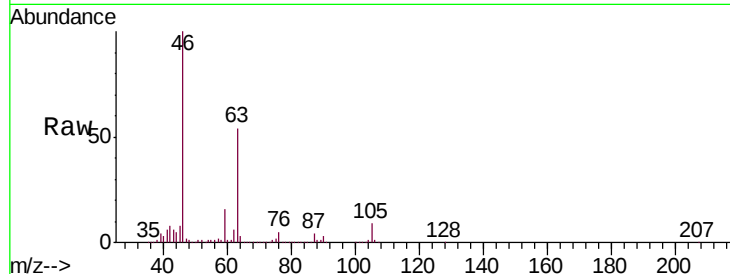

#52
Ethylbenzene
Concen: 200.393 ug/L
RT: 9.25 min Scan# 2830
Delta R.T. -0.00 min
Lab File: VU031675.D
Acq: 01 May 2019 11:37

Tgt Ion: 91 Resp: 7632006
Ion Ratio Lower Upper
91 100
106 29.0 20.4 37.8

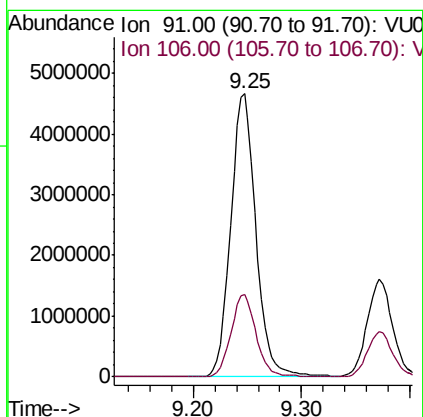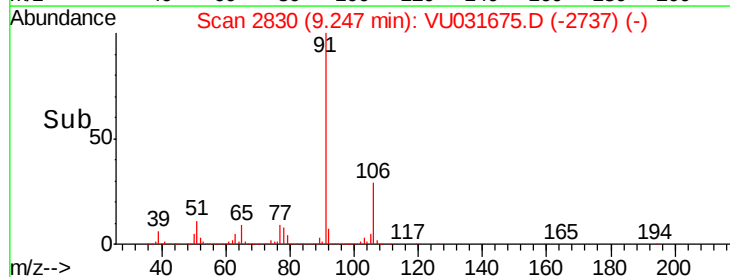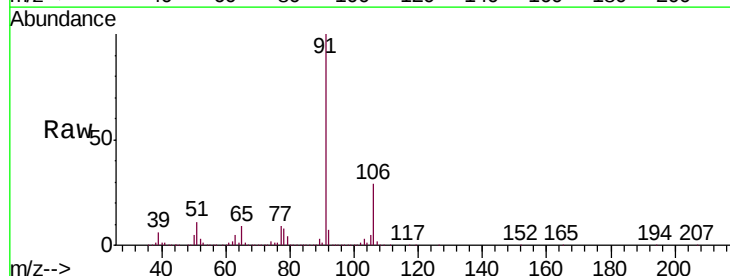

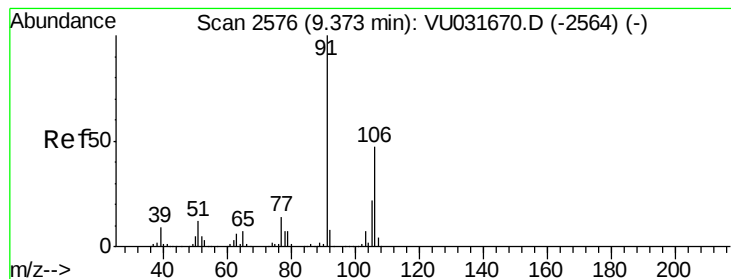

#53

m,p-Xylene

Concen: 93.234 ug/L

RT: 9.37 min Scan# 2869

Delta R.T. -0.00 min

Lab File: VU031675.D

Acq: 01 May 2019 11:37

Instrument :

MSVOA_U

ClientSampleId :


GAJ86

Tgt Ion:106 Resp: 1237155

Ion Ratio Lower Upper




106 100

91 212.7 152.2 282.6

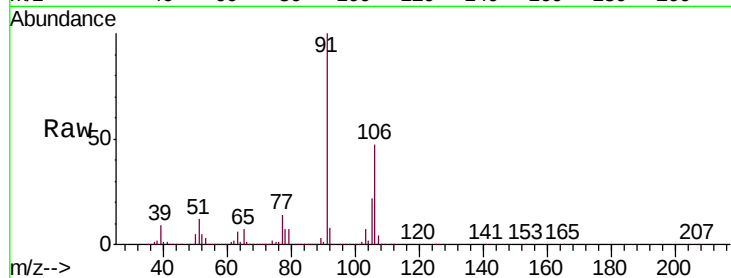

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

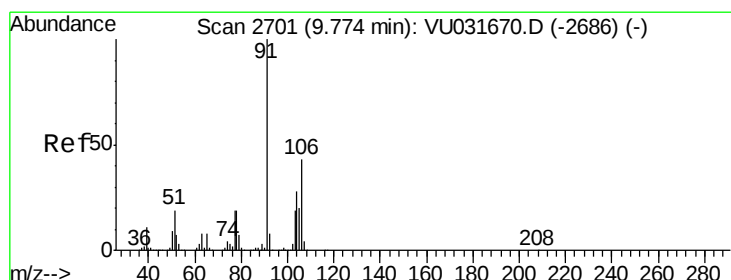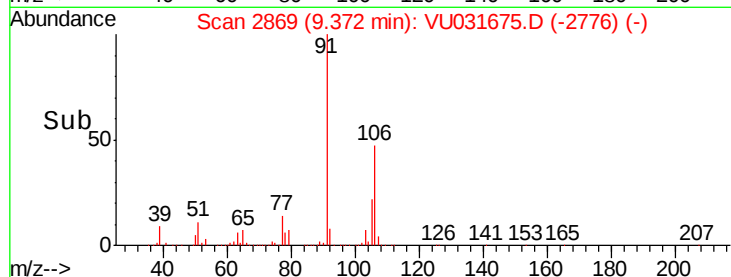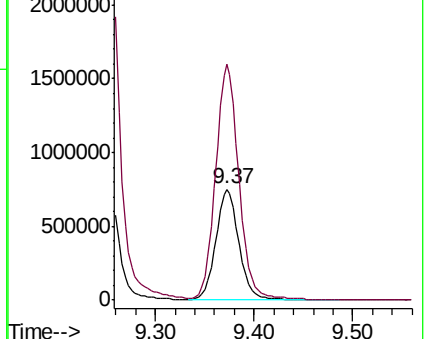

#54

o-xylene

Concen: 103.414 ug/L

RT: 9.77 min Scan# 2994

Delta R.T. -0.00 min

Lab File: VU031675.D


Acq: 01 May 2019 11:37

Tgt Ion:106 Resp: 1360435

Ion Ratio Lower Upper



106 100


91 225.8 163.2 303.2

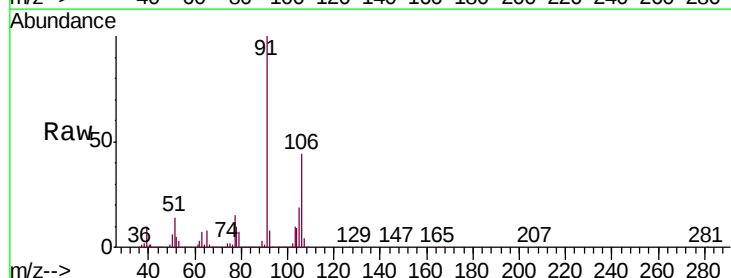

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

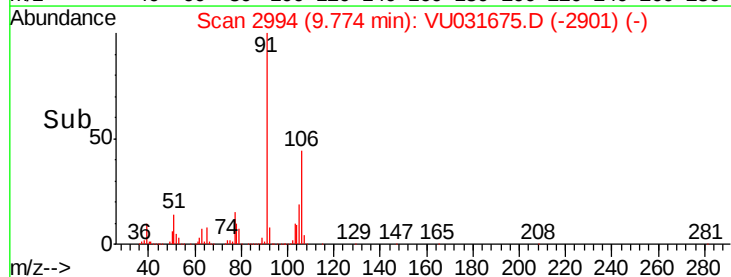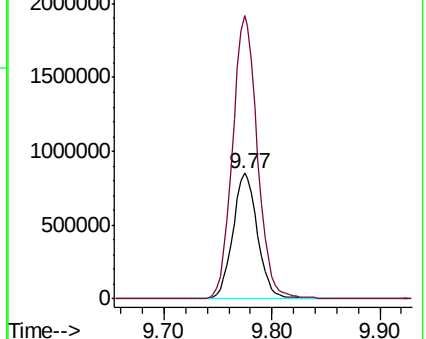

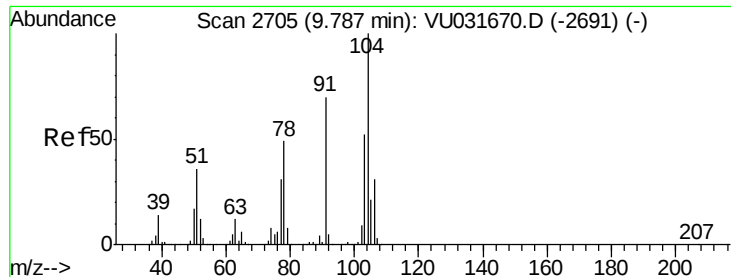

#55

Styrene

Concen: 30.637 ug/L

RT: 9.79 min Scan# 2998

Delta R.T. -0.00 min

Lab File: VU031675.D

Acq: 01 May 2019 11:37

Instrument :

MSVOA_U

ClientSampleId :


GAJ86

Tgt Ion:104 Resp: 688574

Ion Ratio Lower Upper




104 100

78 59.8 35.4 65.7

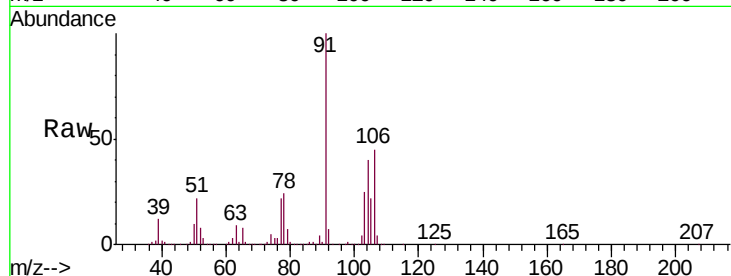

Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VU0

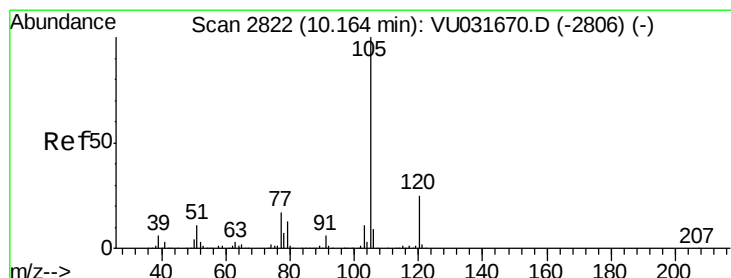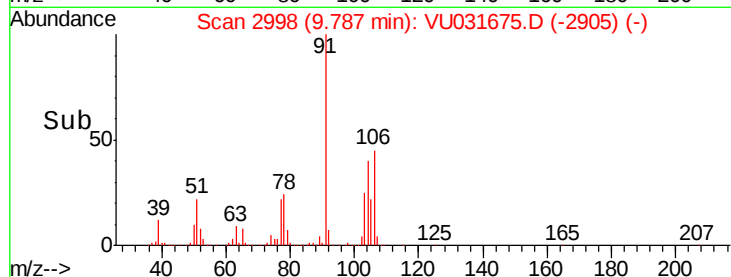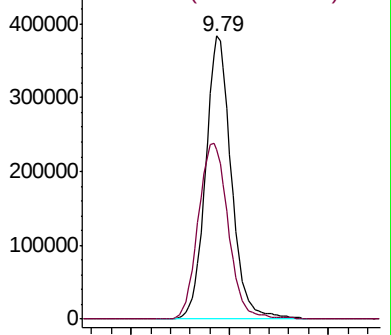

#56

Isopropylbenzene

Concen: 2.003 ug/L

RT: 10.16 min Scan# 3115

Delta R.T. -0.00 min

Lab File: VU031675.D

Acq: 01 May 2019 11:37


Tgt Ion:105 Resp: 69293

Ion Ratio Lower Upper

105 100

120 26.7 20.1 30.1



77 17.8 13.8 20.6

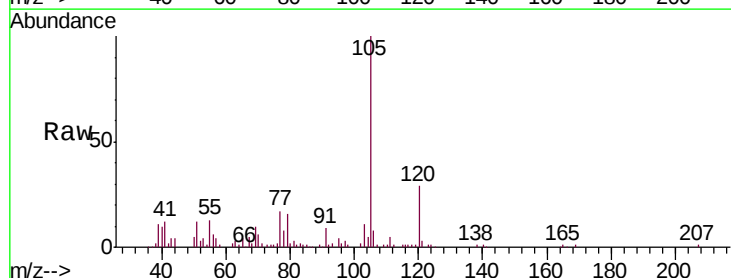


Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VU0

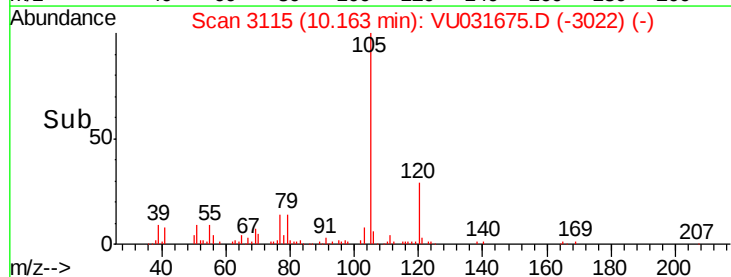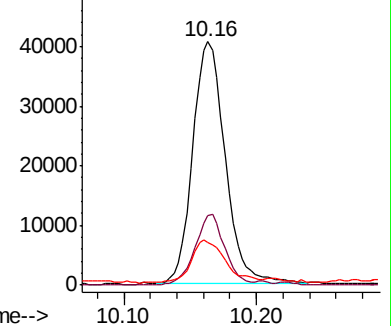


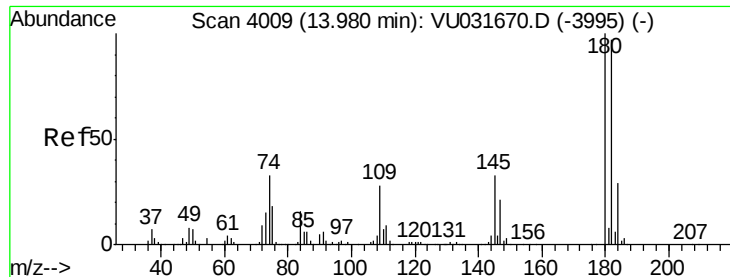

#70
 1,2,3-Trichlorobenzene
 Concen: 0.734 ug/L
 RT: 13.94 min Scan# 4291
 Delta R.T. -0.04 min
 Lab File: VU031675.D
 Acq: 01 May 2019 11:37

Instrument :
 MSVOA_U
 ClientSampleId :
 GAJ86

Tgt Ion:180 Resp: 7760
 Ion Ratio Lower Upper
 180 100
 182 55.0 76.1 114.1#
 145 1884.9 26.0 39.0#

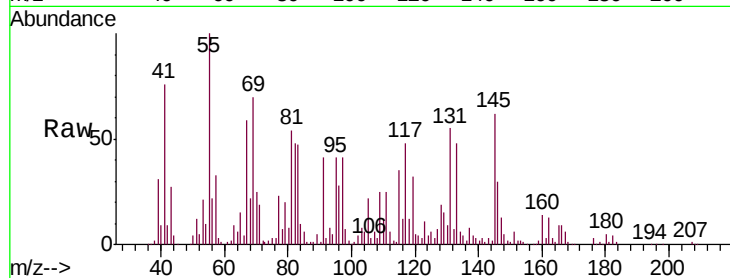

Abundance Ion 180.00 (179.70 to 180.70): V
 Ion 182.00 (181.70 to 182.70): V
 Ion 145.00 (144.70 to 145.70): V

