

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Quantitation Report (QT Reviewed)


Data File : VU031683.D
Acq On : 01 May 2019 14:43
Operator : JC/SP
Sample : K2593-17DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9DL

Manual Integrations
APPROVED

MMDadoda
5/2/2019 9:29:53 AM

Quant Time: May 02 04:56:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 02:23:23 2019
Response via : Initial Calibration

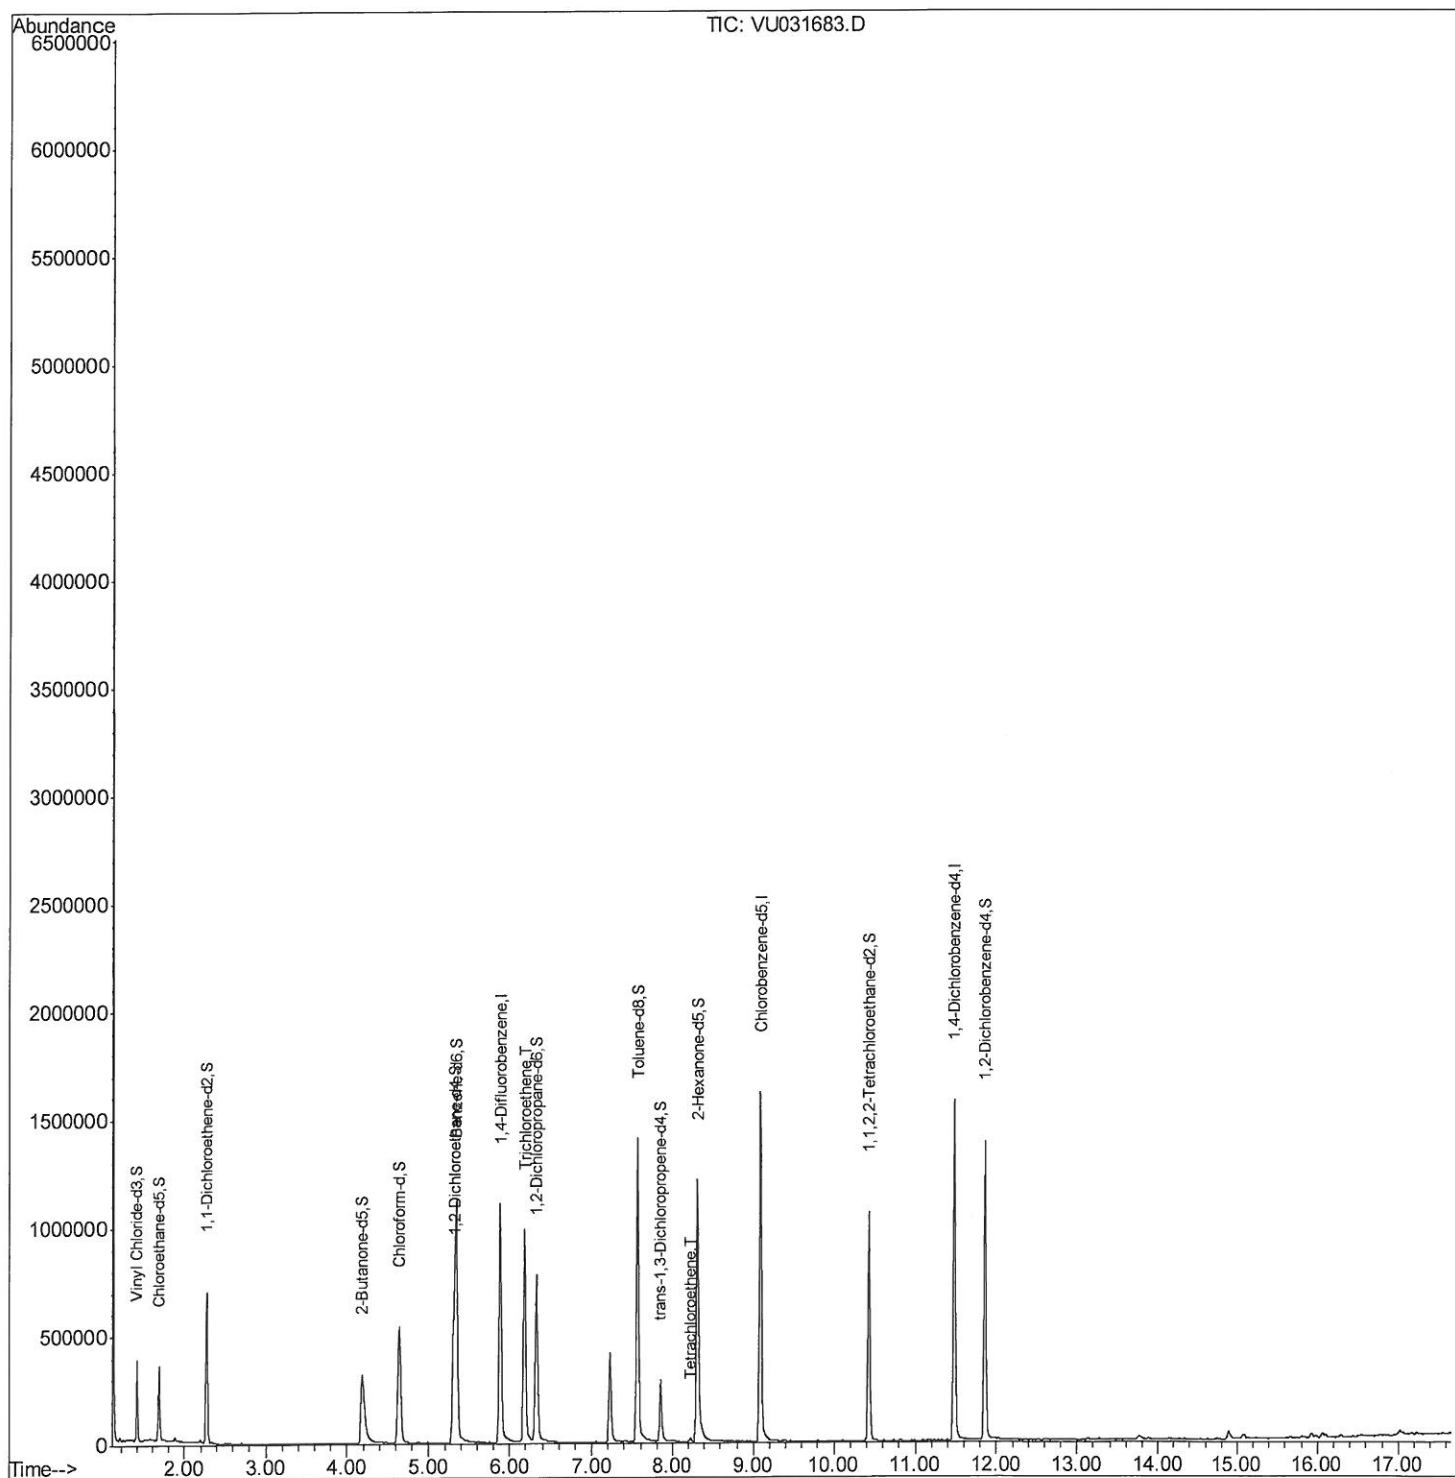

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Quantitation Report (Qedit)




Data File : VU031683.D
Acq On : 01 May 2019 14:43
Operator : JC/SP
Sample : K2593-17DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9DL

Manual Integrations
APPROVED

MMDadoda
5/2/2019 9:29:53 AM

Quant Time: May 02 02:27:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 02:23:23 2019
Response via : Initial Calibration

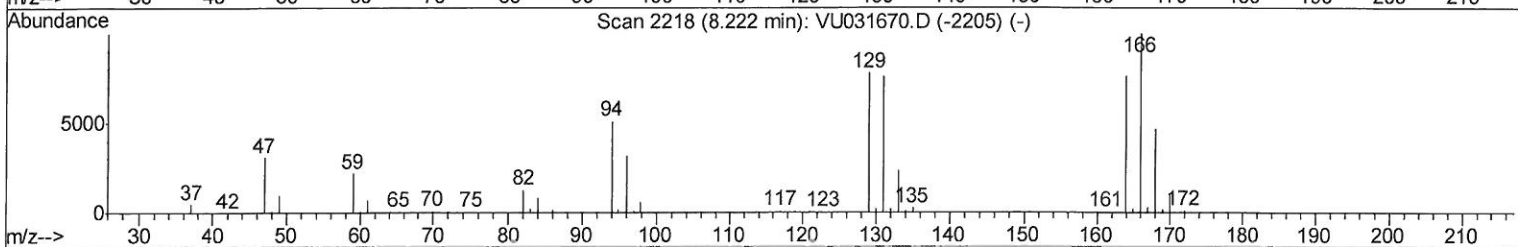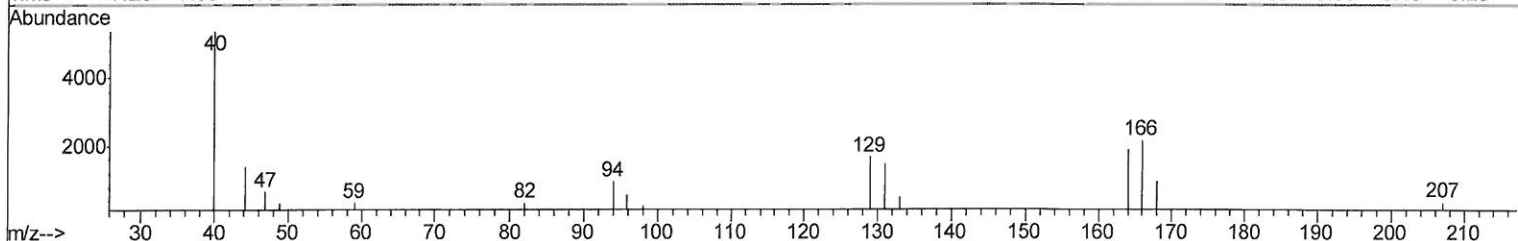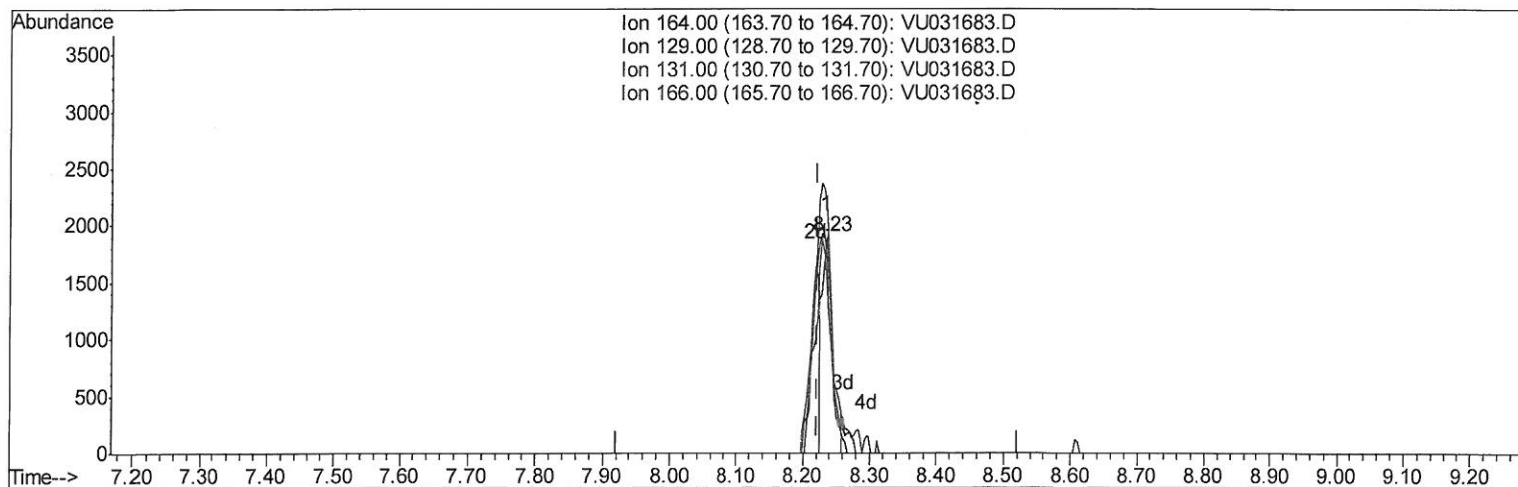

TIC: VU031683.D

(46) Tetrachloroethene (T)
8.234min (+0.013) 0.36ug/L
response 1963

Ion	Exp%	Act%
164.00	100	100
129.00	102.20	88.41
131.00	98.60	77.09
166.00	133.80	114.06

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Quantitation Report (Qedit)




Data File : VU031683.D
Acq On : 01 May 2019 14:43
Operator : JC/SP
Sample : K2593-17DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9DL

Manual Integrations
APPROVED

MMDadoda
5/2/2019 9:29:53 AM

Quant Time: May 02 02:27:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 02:23:23 2019
Response via : Initial Calibration

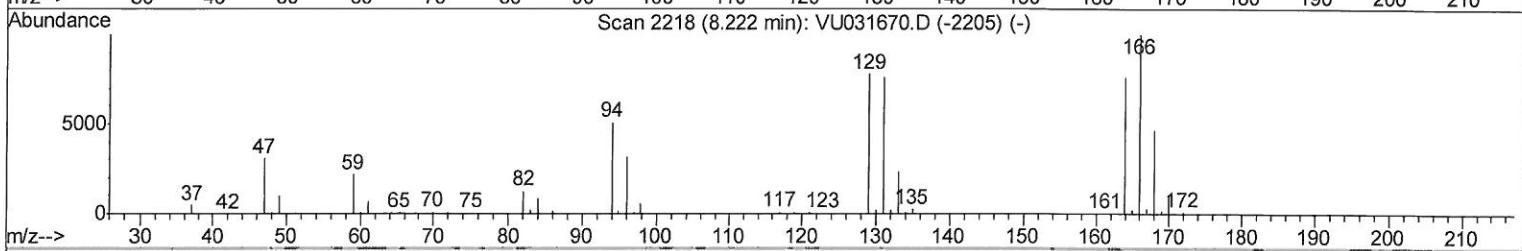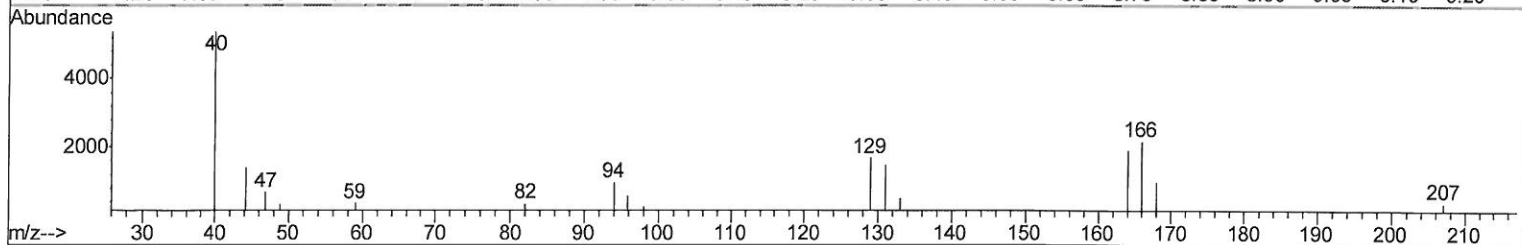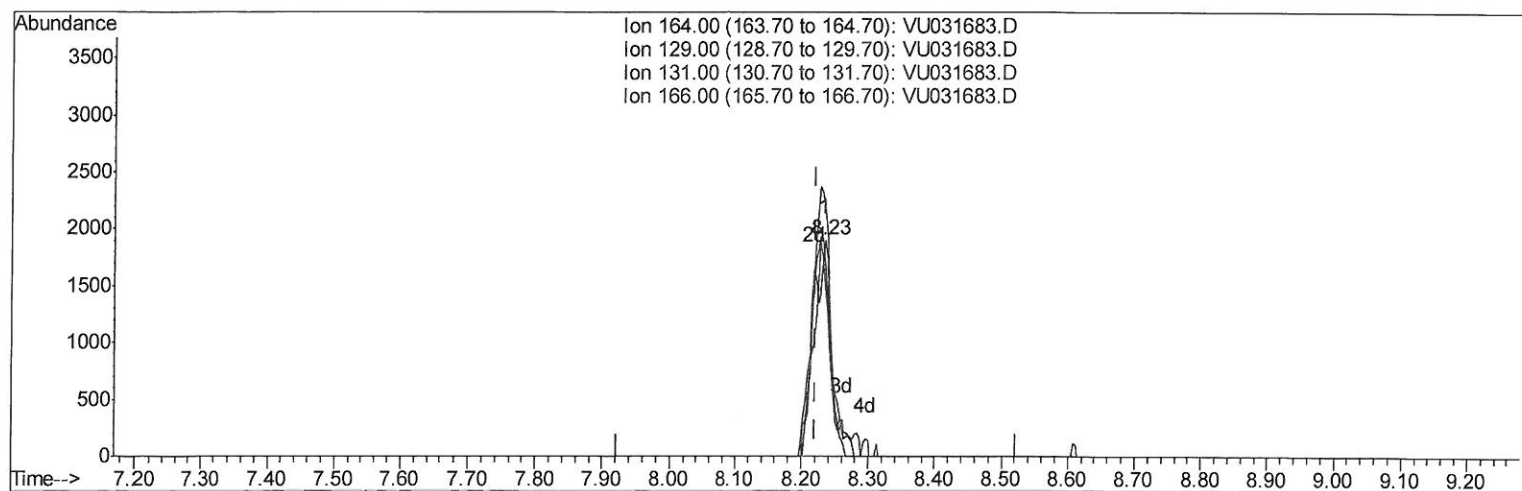

TIC: VU031683.D

(46) Tetrachloroethene (T)

8.234min (+0.013) 0.66ug/L m

response 3618

Ion	Exp%	Act%
164.00	100	100
129.00	102.20	88.41
131.00	98.60	77.09
166.00	133.80	114.06

MMD
5/2/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Quantitation Report (QT Reviewed)

Data File : VU031683.D
Acq On : 01 May 2019 14:43
Operator : JC/SP
Sample : K2593-17DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD9DL

Manual Integrations
APPROVED

MMDadoda
5/2/2019 9:29:53 AM

Quant Time: May 02 04:56:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 02:23:23 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	938518	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	896067	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	403666	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	252246	32.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	64.22%
7) Chloroethane-d5	1.68	69	231950	38.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	76.42%
11) 1,1-Dichloroethene-d2	2.27	63	419677	26.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	53.66%#
21) 2-Butanone-d5	4.19	46	685686	96.35	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.35%
24) Chloroform-d	4.64	84	542939	37.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.48%
26) 1,2-Dichloroethane-d4	5.31	65	380141	40.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.90%
32) Benzene-d6	5.34	84	1124040	40.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.70%
36) 1,2-Dichloropropane-d6	6.32	67	400326	41.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.70%
41) Toluene-d8	7.56	98	980884	40.93	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.86%
43) trans-1,3-Dichloropropene-	7.85	79	174959	42.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.20%
47) 2-Hexanone-d5	8.31	63	442166	105.53	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.53%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	553710	42.62	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.24%
64) 1,2-Dichlorobenzene-d4	11.85	152	365696	43.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.16%

Target Compounds

				Qvalue	
34) Trichloroethene	6.18	95	373476	46.767	ug/L 98
46) Tetrachloroethene	8.23	164	3618m	0.665	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
5/2/19