

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050119\
 Data File : VU031682.D
 Acq On : 01 May 2019 14:20
 Operator : JC/SP
 Sample : K2593-16DL 4000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	37	rVB3	17332	16319	0.47%	0.054%
2	1.396	88	95	109	rVB	384521	412230	11.77%	1.369%
3	1.682	176	184	198	rVB	332887	427134	12.20%	1.419%
4	2.270	356	367	381	rVB	704645	1068124	30.50%	3.548%
5	2.399	405	407	411	rVB4	2150	1319	0.04%	0.004%
6	2.624	474	477	479	rBV4	1632	1183	0.03%	0.004%
7	2.701	491	501	505	rBV9	3430	6044	0.17%	0.020%
8	2.797	527	531	535	rBV4	1286	1322	0.04%	0.004%
9	2.839	541	544	547	rVB2	1560	1072	0.03%	0.004%
10	2.859	547	550	553	rVB4	2061	1132	0.03%	0.004%
11	2.878	553	556	560	rBV3	1404	1021	0.03%	0.003%
12	2.900	560	563	566	rBV2	1134	800	0.02%	0.003%
13	2.929	566	572	577	rVB5	2204	3086	0.09%	0.010%
14	2.961	577	582	585	rBV3	1795	1676	0.05%	0.006%
15	3.019	595	600	604	rBV3	1798	2043	0.06%	0.007%
16	3.177	645	649	652	rVB2	1016	767	0.02%	0.003%
17	3.199	652	656	660	rBV3	1344	1458	0.04%	0.005%
18	3.338	697	699	702	rVB2	1269	746	0.02%	0.002%
19	3.360	702	706	709	rBV4	1594	1708	0.05%	0.006%
20	3.412	718	722	725	rVB4	1079	889	0.03%	0.003%
21	3.489	743	746	751	rVB	1444	1460	0.04%	0.005%
22	3.521	751	756	759	rBV3	935	1056	0.03%	0.004%
23	3.637	787	792	795	rBV3	1600	1336	0.04%	0.004%
24	3.704	811	813	816	rBV2	1077	828	0.02%	0.003%
25	3.868	859	864	869	rVB3	1149	988	0.03%	0.003%
26	3.945	884	888	894	rVB3	1197	1056	0.03%	0.004%
27	4.064	920	925	929	rBV3	1266	1149	0.03%	0.004%
28	4.100	932	936	938	rBV3	1566	1260	0.04%	0.004%
29	4.183	948	962	1010	rBV	363695	1125936	32.15%	3.740%
30	4.463	1047	1049	1053	rBV3	1959	1687	0.05%	0.006%
31	4.514	1062	1065	1067	rBV3	1379	847	0.02%	0.003%
32	4.643	1088	1105	1134	rBV	545776	1334707	38.11%	4.433%
33	4.862	1169	1173	1174	rBV3	1303	948	0.03%	0.003%
34	4.984	1208	1211	1214	rBV3	2297	1780	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050119\
 Data File : VU031682.D
 Acq On : 01 May 2019 14:20
 Operator : JC/SP
 Sample : K2593-16DL 4000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1296	1320	1359	rBV2	1139538	3502453	100.00%	11.633%
36	5.601	1401	1403	1406	rVB2	1961	1097	0.03%	0.004%
37	5.675	1423	1426	1430	rBV5	1869	1563	0.04%	0.005%
38	5.720	1438	1440	1443	rBV3	1396	893	0.03%	0.003%
39	5.881	1476	1490	1524	rBV	1113510	2329648	66.51%	7.738%
40	6.183	1569	1584	1614	rBV	907062	1848895	52.79%	6.141%
41	6.328	1616	1629	1655	rVB	770088	1592345	45.46%	5.289%
42	6.592	1708	1711	1714	rVB3	2540	1740	0.05%	0.006%
43	6.698	1741	1744	1747	rBV2	1306	1007	0.03%	0.003%
44	6.884	1799	1802	1805	rBV4	1325	982	0.03%	0.003%
45	6.948	1818	1822	1826	rBV6	1208	1231	0.04%	0.004%
46	6.977	1829	1831	1835	rVV2	1421	1042	0.03%	0.003%
47	7.000	1835	1838	1840	rVV4	976	768	0.02%	0.003%
48	7.026	1844	1846	1851	rVV3	1509	1135	0.03%	0.004%
49	7.083	1863	1864	1868	rVB2	1686	816	0.02%	0.003%
50	7.225	1896	1908	1934	rBV	425784	809292	23.11%	2.688%
51	7.498	1990	1993	1997	rVB4	1940	1344	0.04%	0.004%
52	7.563	2000	2013	2034	rBV	1427195	2619233	74.78%	8.699%
53	7.849	2091	2102	2129	rBV	282092	528623	15.09%	1.756%
54	8.112	2180	2184	2188	rBV3	1939	1980	0.06%	0.007%
55	8.183	2203	2206	2208	rBV2	1415	746	0.02%	0.002%
56	8.231	2213	2221	2229	rVB6	8636	13450	0.38%	0.045%
57	8.309	2233	2245	2290	rBV	1253514	2467492	70.45%	8.195%
58	8.698	2364	2366	2370	rVB4	1564	881	0.03%	0.003%
59	8.942	2436	2442	2444	rBV3	1541	1410	0.04%	0.005%
60	8.968	2447	2450	2453	rBV3	1661	1186	0.03%	0.004%
61	9.087	2474	2487	2531	rBV	1641560	2892871	82.60%	9.608%
62	9.302	2551	2554	2558	rVB3	2608	2114	0.06%	0.007%
63	9.379	2574	2578	2580	rBV2	2767	2037	0.06%	0.007%
64	9.421	2589	2591	2594	rBV3	1760	874	0.02%	0.003%
65	9.511	2613	2619	2622	rBV6	2023	2397	0.07%	0.008%
66	9.598	2644	2646	2652	rVB3	1696	1495	0.04%	0.005%
67	9.653	2660	2663	2667	rBV2	1357	1277	0.04%	0.004%
68	9.768	2695	2699	2703	rBV4	2033	2061	0.06%	0.007%
69	9.862	2726	2728	2732	rVB3	1663	1014	0.03%	0.003%
70	9.881	2732	2734	2738	rBV2	1643	1355	0.04%	0.005%
71	10.019	2775	2777	2782	rVB3	1395	833	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050119\
 Data File : VU031682.D
 Acq On : 01 May 2019 14:20
 Operator : JC/SP
 Sample : K2593-16DL 4000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.048	2783	2786	2788	rVV3	1000	780	0.02%	0.003%
73	10.074	2792	2794	2799	rBV3	942	907	0.03%	0.003%
74	10.193	2827	2831	2834	rBV2	2130	1676	0.05%	0.006%
75	10.215	2834	2838	2842	rBV5	1281	1270	0.04%	0.004%
76	10.299	2860	2864	2866	rVV3	1172	927	0.03%	0.003%
77	10.315	2866	2869	2872	rBV2	1041	761	0.02%	0.003%
78	10.427	2891	2904	2925	rBV	1075834	1762191	50.31%	5.853%
79	10.739	2999	3001	3004	rVB2	2105	1159	0.03%	0.004%
80	10.810	3020	3023	3025	rBV3	1902	1533	0.04%	0.005%
81	10.935	3059	3062	3065	rBV3	1457	874	0.02%	0.003%
82	10.987	3074	3078	3080	rBV3	1167	813	0.02%	0.003%
83	11.045	3093	3096	3100	rBV3	1552	1225	0.03%	0.004%
84	11.080	3105	3107	3111	rVB3	1634	1068	0.03%	0.004%
85	11.112	3114	3117	3121	rVV3	1960	1744	0.05%	0.006%
86	11.238	3154	3156	3160	rVB3	1650	1084	0.03%	0.004%
87	11.312	3176	3179	3181	rBV3	1571	1172	0.03%	0.004%
88	11.389	3200	3203	3208	rBV4	2190	2282	0.07%	0.008%
89	11.424	3211	3214	3217	rBV2	2115	1523	0.04%	0.005%
90	11.479	3219	3231	3257	rBV	1615949	2659844	75.94%	8.834%
91	11.855	3336	3348	3381	rBV	1412745	2392020	68.30%	7.945%
92	12.173	3442	3447	3449	rBV6	2860	2772	0.08%	0.009%
93	12.463	3533	3537	3538	rBV5	2056	1524	0.04%	0.005%
94	12.601	3577	3580	3581	rBV3	2404	1397	0.04%	0.005%
95	12.681	3602	3605	3607	rBV3	2022	1505	0.04%	0.005%
96	13.006	3703	3706	3710	rVB4	2612	1788	0.05%	0.006%
97	13.138	3737	3747	3752	rBV4	9346	17307	0.49%	0.057%
98	13.549	3872	3875	3878	rBV3	2305	1689	0.05%	0.006%
99	14.893	4283	4293	4315	rBV3	47707	127105	3.63%	0.422%
100	15.926	4606	4614	4626	rBV4	29766	53332	1.52%	0.177%


Sum of corrected areas: 30107963

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050119\
Data File : VU031682.D
Acq On : 01 May 2019 14:20
Operator : JC/SP
Sample : K2593-16DL 4000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

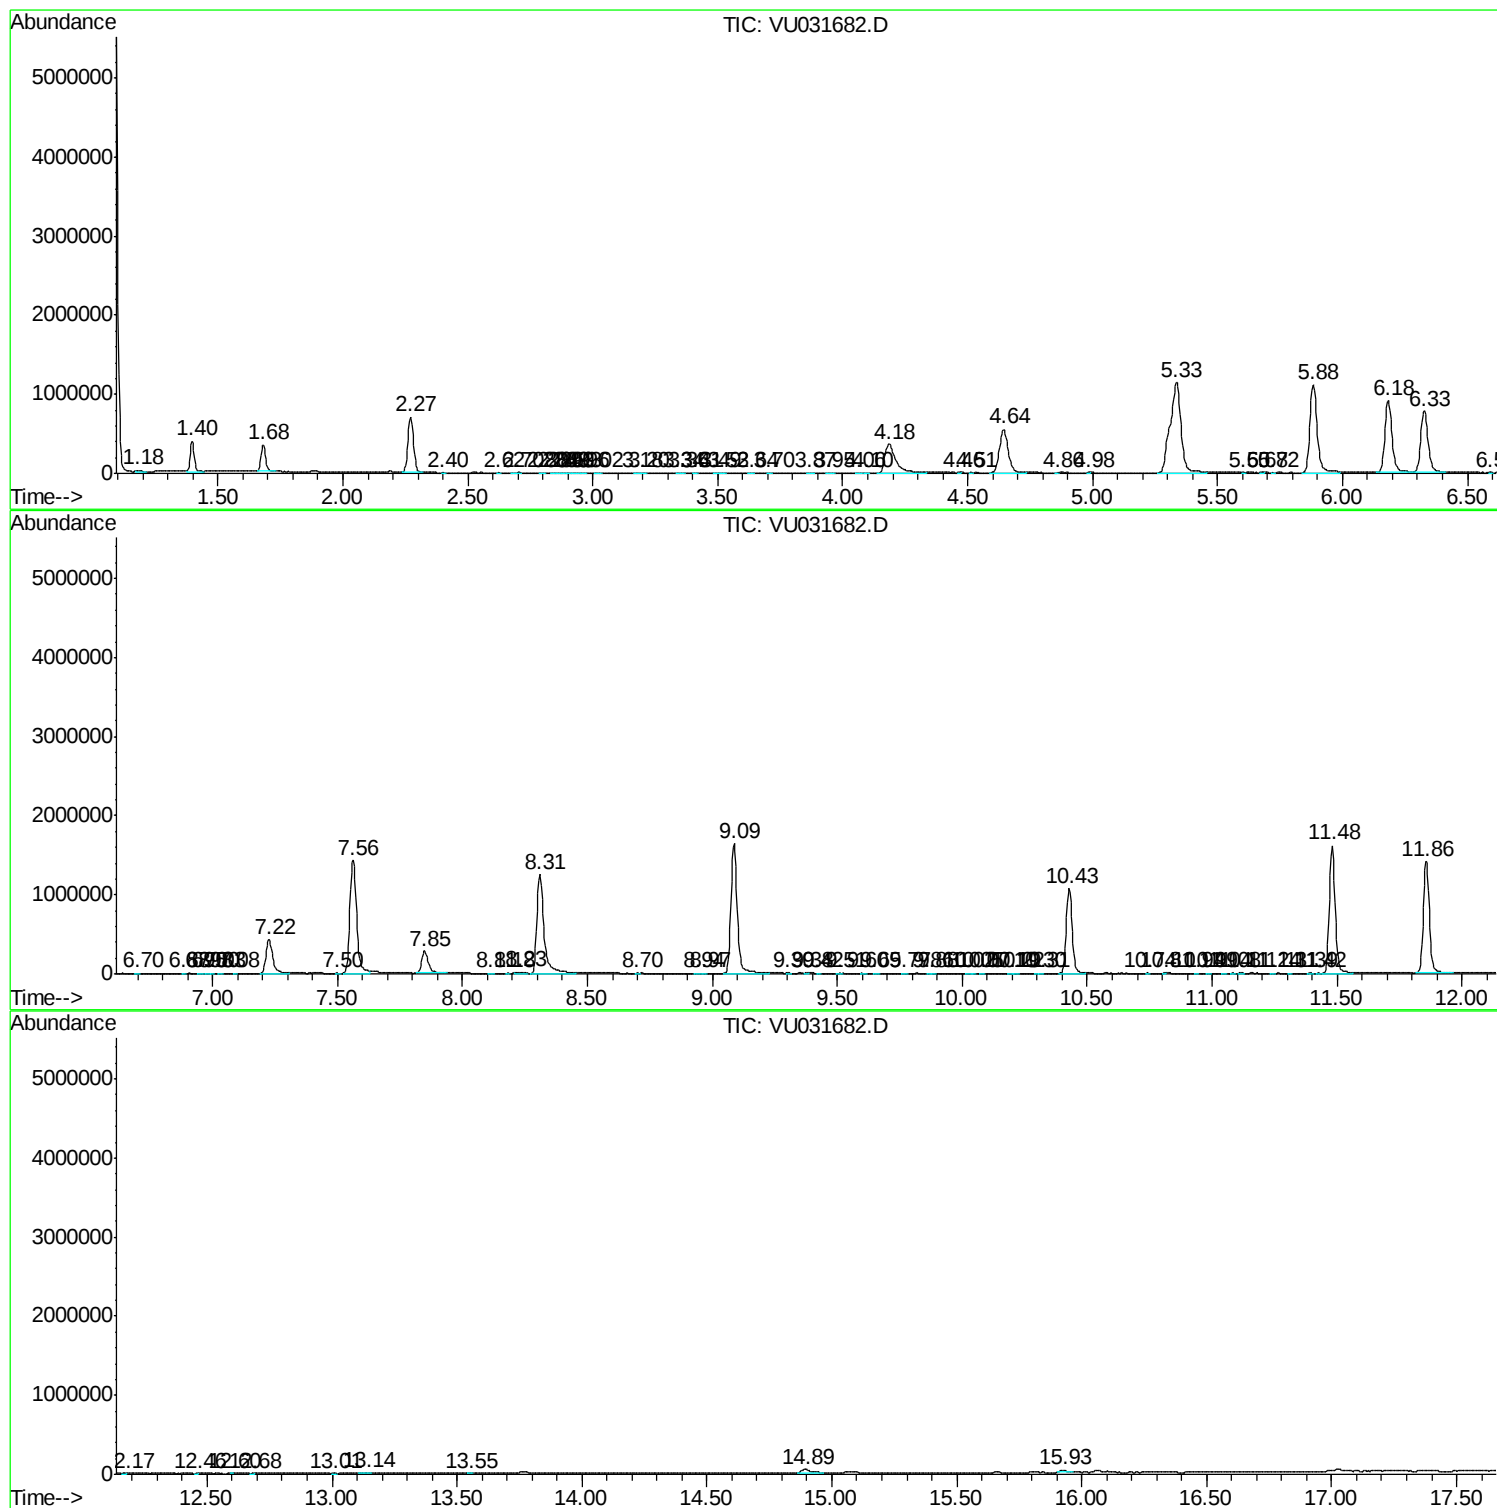

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Data File : VU031682.D
Acq On : 01 May 2019 14:20
Operator : JC/SP
Sample : K2593-16DL 4000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Data File : VU031682.D
Acq On : 01 May 2019 14:20
Operator : JC/SP
Sample : K2593-16DL 4000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc