

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050119\
 Data File : VU031685.D
 Acq On : 01 May 2019 15:29
 Operator : JC/SP
 Sample : K2593-19DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	89	95	112	rVB	375311	407326	11.88%	1.347%
2	1.682	176	184	203	rVB	341689	425038	12.40%	1.406%
3	2.270	357	367	381	rVB	691764	1062213	30.98%	3.513%
4	2.421	411	414	419	rBV6	1069	809	0.02%	0.003%
5	2.482	426	433	437	rBV6	2262	2733	0.08%	0.009%
6	2.530	446	448	453	rBV4	1729	1581	0.05%	0.005%
7	2.624	473	477	482	rBV4	1674	2038	0.06%	0.007%
8	2.698	494	500	509	rVB7	3301	5220	0.15%	0.017%
9	2.797	528	531	534	rBV	1820	1195	0.03%	0.004%
10	2.961	577	582	585	rBV3	1171	1444	0.04%	0.005%
11	3.083	617	620	626	rVB2	1286	1076	0.03%	0.004%
12	3.116	626	630	635	rVB4	2464	2245	0.07%	0.007%
13	3.157	638	643	646	rBV5	1427	1482	0.04%	0.005%
14	3.186	650	652	657	rVB3	1059	892	0.03%	0.003%
15	3.212	657	660	663	rBV2	1070	847	0.02%	0.003%
16	3.231	663	666	671	rVB3	1036	1043	0.03%	0.003%
17	3.283	678	682	686	rBV3	1297	1166	0.03%	0.004%
18	3.302	686	688	692	rVB5	1412	882	0.03%	0.003%
19	3.431	724	728	731	rBV2	1392	936	0.03%	0.003%
20	3.482	741	744	750	rVB3	1426	1040	0.03%	0.003%
21	3.514	750	754	756	rBV2	914	645	0.02%	0.002%
22	3.592	774	778	781	rBV2	1064	921	0.03%	0.003%
23	3.624	784	788	791	rBV2	1228	1091	0.03%	0.004%
24	3.656	795	798	801	rVB2	1129	771	0.02%	0.003%
25	3.688	801	808	812	rBV2	1720	1856	0.05%	0.006%
26	3.714	813	816	819	rVB3	1862	1125	0.03%	0.004%
27	3.739	819	824	827	rBV3	1437	1591	0.05%	0.005%
28	3.817	846	848	851	rVB	1140	637	0.02%	0.002%
29	3.846	851	857	861	rBV4	1990	1781	0.05%	0.006%
30	3.919	874	880	882	rBV3	753	691	0.02%	0.002%
31	4.006	902	907	909	rBV3	762	665	0.02%	0.002%
32	4.058	920	923	927	rVB2	1302	961	0.03%	0.003%
33	4.125	941	944	946	rBV	1182	825	0.02%	0.003%
34	4.186	950	963	994	rBV2	346534	1078999	31.47%	3.568%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050119\
 Data File : VU031685.D
 Acq On : 01 May 2019 15:29
 Operator : JC/SP
 Sample : K2593-19DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.518	1063	1066	1068	rBV2	1196	844	0.02%	0.003%
36	4.643	1088	1105	1134	rBV	539434	1324621	38.64%	4.381%
37	4.961	1201	1204	1205	rBV2	1315	706	0.02%	0.002%
38	5.064	1233	1236	1242	rBV5	1341	1142	0.03%	0.004%
39	5.125	1251	1255	1263	rVB4	2412	3274	0.10%	0.011%
40	5.337	1297	1321	1350	rBV2	1139873	3428481	100.00%	11.338%
41	5.736	1442	1445	1447	rBV3	1626	921	0.03%	0.003%
42	5.884	1477	1491	1514	rBV	1112541	2256207	65.81%	7.461%
43	6.183	1570	1584	1616	rBV	1165665	2354887	68.69%	7.788%
44	6.328	1616	1629	1663	rVB	773932	1607598	46.89%	5.316%
45	6.595	1710	1712	1715	rVB2	1553	729	0.02%	0.002%
46	6.704	1743	1746	1750	rBV3	2158	1514	0.04%	0.005%
47	6.726	1750	1753	1758	rVB4	1106	733	0.02%	0.002%
48	6.788	1769	1772	1774	rVV3	1215	666	0.02%	0.002%
49	6.878	1796	1800	1802	rBV2	1752	1257	0.04%	0.004%
50	6.900	1804	1807	1810	rVB3	944	791	0.02%	0.003%
51	6.935	1815	1818	1821	rVV5	992	780	0.02%	0.003%
52	7.038	1846	1850	1851	rBV3	1131	639	0.02%	0.002%
53	7.115	1870	1874	1876	rBV2	1560	1232	0.04%	0.004%
54	7.132	1876	1879	1882	rVV2	1217	850	0.02%	0.003%
55	7.225	1895	1908	1939	rBV	415768	809716	23.62%	2.678%
56	7.562	1999	2013	2059	rBV	1433374	2707269	78.96%	8.953%
57	7.849	2091	2102	2130	rBV	278698	525945	15.34%	1.739%
58	8.138	2188	2192	2195	rBV4	1495	1366	0.04%	0.005%
59	8.157	2195	2198	2200	rBV2	2136	1400	0.04%	0.005%
60	8.231	2211	2221	2233	rBV3	19748	36429	1.06%	0.120%
61	8.308	2235	2245	2281	rBV	1249836	2410499	70.31%	7.972%
62	8.620	2339	2342	2347	rVB5	2131	2017	0.06%	0.007%
63	8.752	2381	2383	2386	rBV2	1043	907	0.03%	0.003%
64	8.852	2411	2414	2419	rBV6	1117	1261	0.04%	0.004%
65	8.971	2447	2451	2455	rBV6	1726	1660	0.05%	0.005%
66	9.032	2468	2470	2474	rVB3	1526	859	0.03%	0.003%
67	9.086	2474	2487	2528	rBV	1623568	2868064	83.65%	9.485%
68	9.328	2556	2562	2565	rBV7	1728	2348	0.07%	0.008%
69	9.366	2571	2574	2576	rBV3	1298	951	0.03%	0.003%
70	9.501	2614	2616	2622	rVB7	1372	960	0.03%	0.003%
71	9.530	2622	2625	2628	rBV5	1206	973	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050119\
 Data File : VU031685.D
 Acq On : 01 May 2019 15:29
 Operator : JC/SP
 Sample : K2593-19DL 5000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.566	2633	2636	2638	rBV3	970	714	0.02%	0.002%
73	9.611	2648	2650	2658	rVB4	1131	1445	0.04%	0.005%
74	9.749	2688	2693	2697	rBV4	1256	1356	0.04%	0.004%
75	9.791	2701	2706	2711	rBV4	2353	2199	0.06%	0.007%
76	9.887	2734	2736	2739	rVB3	1334	721	0.02%	0.002%
77	10.012	2772	2775	2779	rBV3	1126	1127	0.03%	0.004%
78	10.109	2802	2805	2808	rVB3	1212	834	0.02%	0.003%
79	10.128	2808	2811	2814	rBV3	1164	927	0.03%	0.003%
80	10.157	2818	2820	2823	rBV2	1186	771	0.02%	0.003%
81	10.283	2857	2859	2864	rVB4	1062	767	0.02%	0.003%
82	10.312	2864	2868	2873	rBV4	1429	1756	0.05%	0.006%
83	10.334	2873	2875	2879	rVV3	1224	932	0.03%	0.003%
84	10.427	2891	2904	2933	rBV	1093217	1774443	51.76%	5.868%
85	10.829	3026	3029	3031	rBV4	1136	773	0.02%	0.003%
86	10.951	3063	3067	3071	rBV4	2054	1945	0.06%	0.006%
87	10.990	3076	3079	3082	rVB3	1674	968	0.03%	0.003%
88	11.012	3082	3086	3091	rBV6	1602	1806	0.05%	0.006%
89	11.083	3104	3108	3111	rBV3	1600	1292	0.04%	0.004%
90	11.228	3150	3153	3156	rBV2	1248	1155	0.03%	0.004%
91	11.270	3164	3166	3168	rBV2	1055	659	0.02%	0.002%
92	11.389	3200	3203	3205	rBV2	1055	662	0.02%	0.002%
93	11.479	3219	3231	3252	rBV	1595479	2612840	76.21%	8.641%
94	11.855	3335	3348	3380	rBV	1424700	2396366	69.90%	7.925%
95	12.694	3607	3609	3611	rBV3	1875	1136	0.03%	0.004%
96	12.832	3647	3652	3657	rBV5	2393	2949	0.09%	0.010%
97	13.128	3741	3744	3745	rBV3	3049	1939	0.06%	0.006%
98	13.257	3781	3784	3785	rBV2	1780	1097	0.03%	0.004%
99	13.581	3882	3885	3890	rBV5	1847	2098	0.06%	0.007%
100	14.903	4287	4296	4309	rBV3	20607	48715	1.42%	0.161%


Sum of corrected areas: 30238653

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050119\
Data File : VU031685.D
Acq On : 01 May 2019 15:29
Operator : JC/SP
Sample : K2593-19DL 5000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

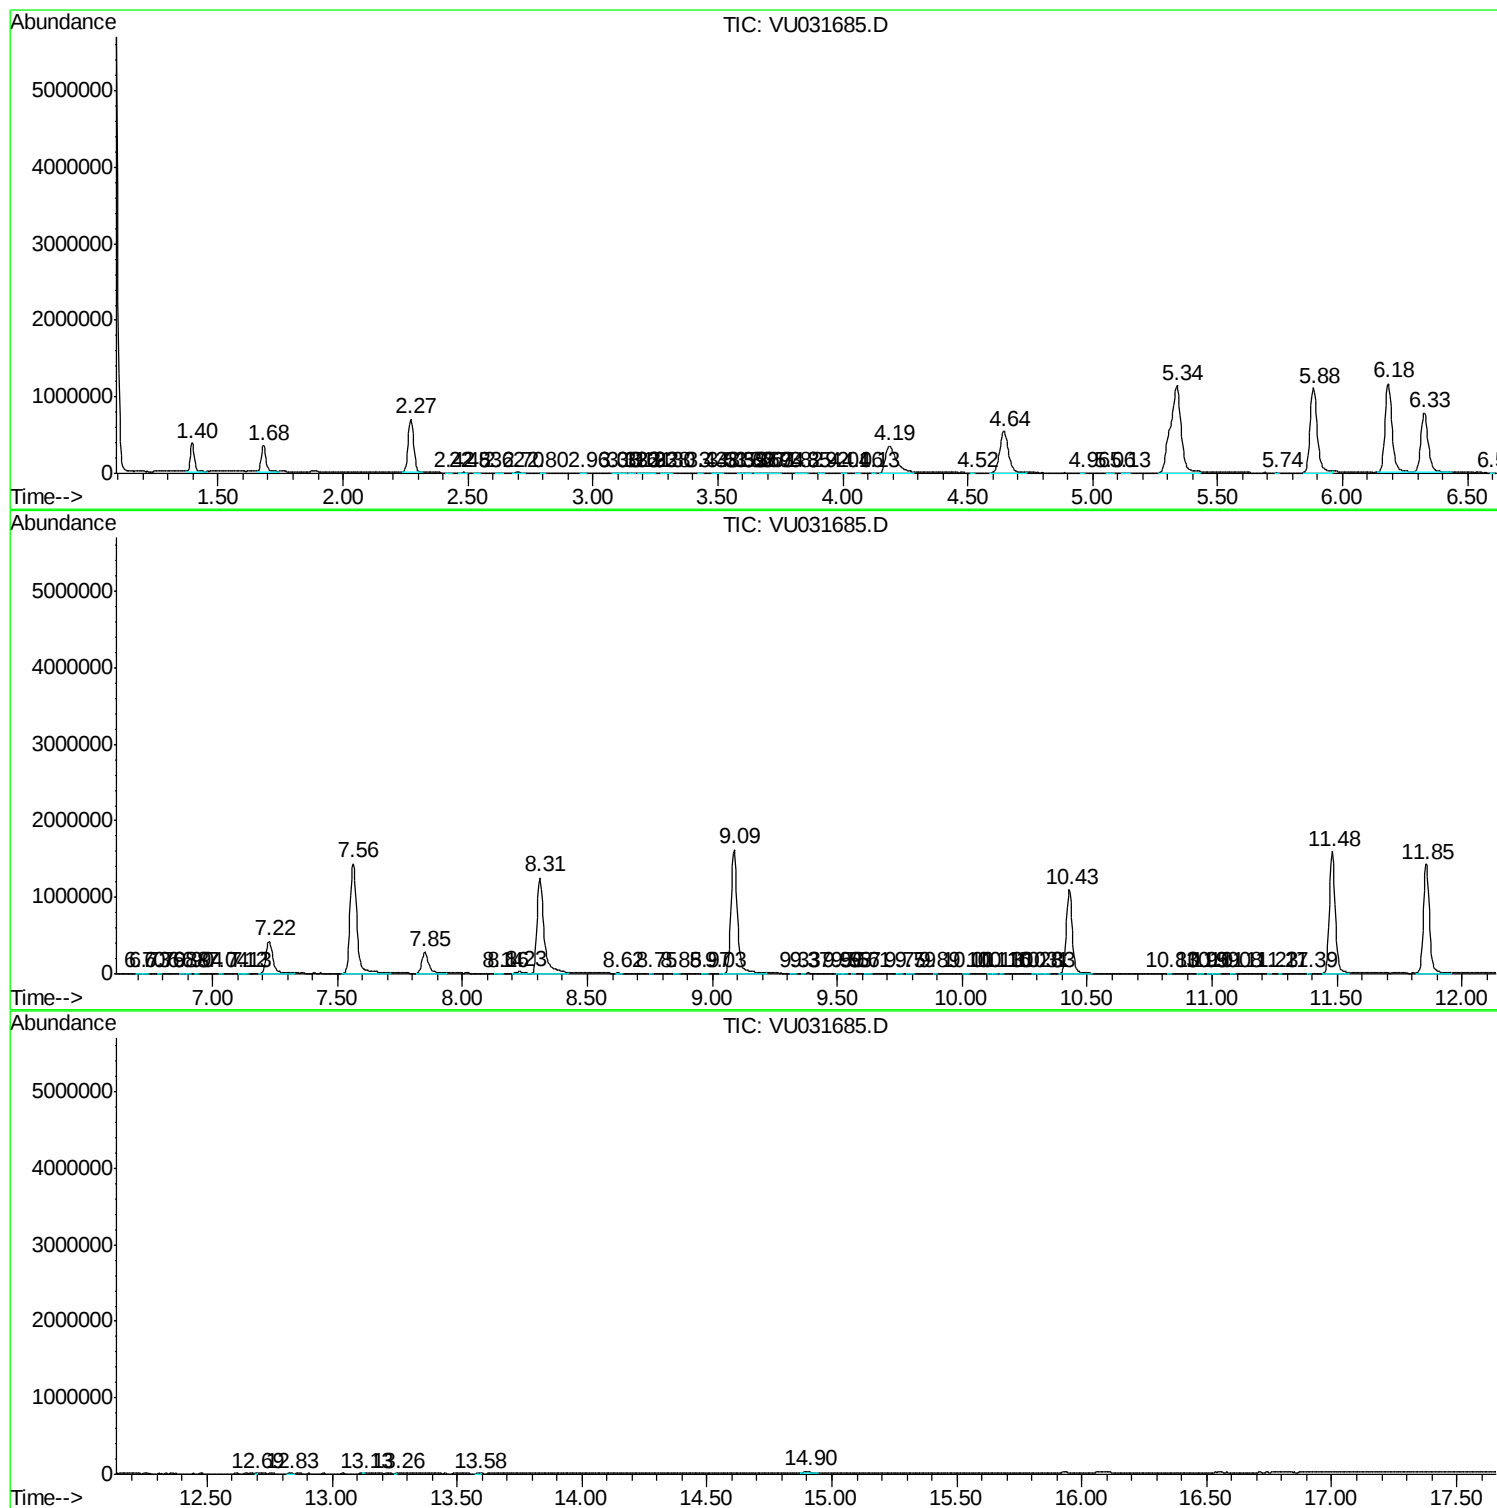

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050119\
Data File : VU031685.D
Acq On : 01 May 2019 15:29
Operator : JC/SP
Sample : K2593-19DL 5000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU050119\
Data File : VU031685.D
Acq On : 01 May 2019 15:29
Operator : JC/SP
Sample : K2593-19DL 5000X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0XG5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc