


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050119\
 Data File : VU031669.D
 Acq On : 01 May 2019 09:08
 Operator : JC/SP
 Sample : BFB35
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB35

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Thu May 02 02:23:23 2019

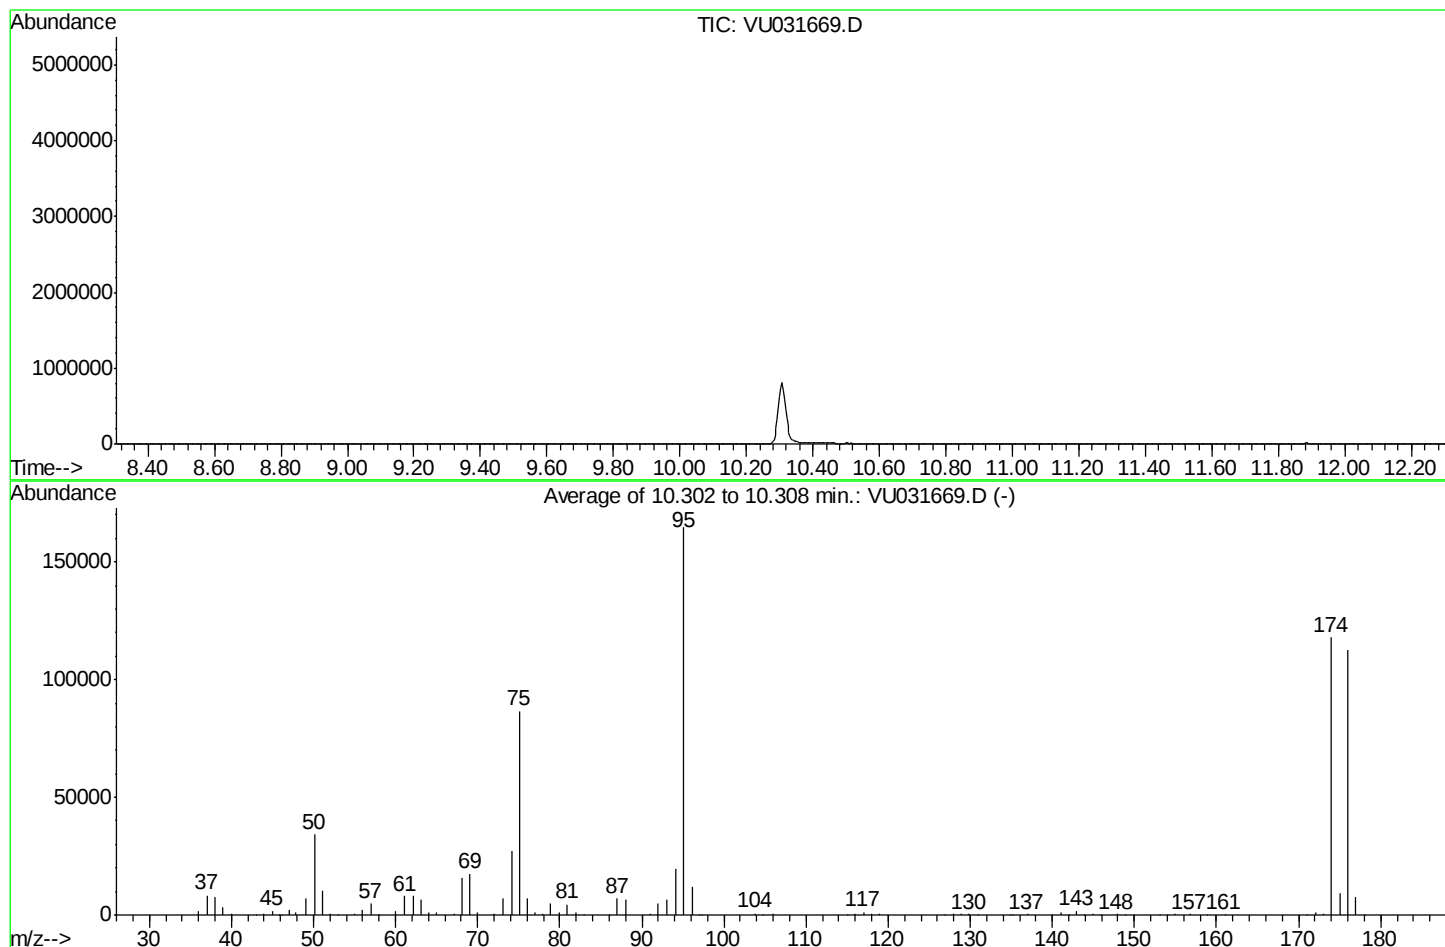

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	34122	PASS
75	95	30	80	52.5	86512	PASS
95	95	100	100	100.0	164672	PASS
96	95	5	9	7.3	11950	PASS
173	174	0.00	2	0.4	457	PASS
174	95	50	120	71.5	117781	PASS
175	174	5	9	7.8	9222	PASS
176	174	95	101	95.4	112333	PASS
177	176	5	9	6.7	7534	PASS

m/z	Abundance
36.00	1784.0
37.00	8041.0
38.10	7769.0
39.00	2980.0
40.00	5154.0
43.00	112.0
44.10	2217.0
45.00	1610.0
45.80	161.0
47.00	2098.0
47.90	1218.0
49.00	6959.0
50.10	33272.0
51.10	10066.0
52.00	641.0
53.00	261.0
55.00	585.0
56.00	2674.0
57.00	4649.0
58.00	137.0
60.10	1556.0
61.10	7489.0
62.10	7760.0
63.00	6300.0
64.10	995.0
65.10	1028.0
67.20	421.0
68.10	15665.0
69.10	17584.0
70.00	1064.0
72.00	800.0
73.00	6702.0
74.10	26224.0
75.10	85256.0
76.00	7256.0
77.00	1198.0
77.90	1004.0
78.90	4910.0
80.00	1238.0
81.00	4421.0
82.00	856.0
82.90	127.0
86.00	266.0
87.00	6729.0
88.00	6143.0
91.00	641.0
92.00	4481.0
93.10	6386.0
94.10	19320.0
95.10	155648.0
96.10	11949.0
97.00	240.0
103.90	580.0
104.80	296.0
106.00	541.0
115.00	143.0
115.90	440.0
117.10	1063.0
117.90	392.0
118.90	696.0
126.80	122.0
128.00	421.0
128.90	283.0
129.90	317.0
130.90	208.0
134.80	245.0
136.90	213.0
140.00	148.0
141.00	1236.0
142.00	179.0
143.00	1838.0
144.90	438.0
146.00	229.0
147.90	455.0
148.90	206.0
150.00	104.0
154.00	189.0
154.80	364.0
156.80	350.0
161.00	275.0
171.00	224.0
172.10	1049.0
173.00	1372.0
174.00	109400.0
175.00	9287.0
176.00	104920.0
177.00	7536.0
178.00	116.0
207.40	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	2040.0
37.00	8655.0
38.00	8039.0
39.00	3452.0
40.00	4896.0
42.90	114.0
44.10	2232.0
45.00	1684.0
46.20	191.0
47.00	2467.0
47.90	1214.0
49.00	7228.0
50.10	35440.0
51.10	10685.0
52.00	637.0
53.00	237.0
55.10	735.0
56.00	2582.0
57.00	4953.0
58.00	143.0
60.00	1512.0
61.10	8331.0
62.10	8349.0
63.10	7045.0
64.10	1140.0
65.00	958.0
67.10	469.0
68.10	16325.0
69.10	17968.0
70.00	1153.0
72.00	857.0
73.10	7666.0
74.10	28432.0
75.10	89336.0
76.00	7366.0
77.00	1098.0
78.00	915.0
78.90	5128.0
80.00	1209.0
81.00	4503.0
82.00	945.0
82.90	139.0
86.00	189.0
87.00	7516.0
88.00	6729.0
91.00	592.0
92.00	4960.0
93.10	6614.0
94.10	20560.0
95.10	169984.0
96.10	12424.0
97.20	254.0
103.90	636.0
104.70	331.0
106.00	625.0
115.00	126.0
116.00	408.0
117.00	1258.0
118.00	537.0
119.00	767.0
128.00	440.0
128.80	304.0
129.90	436.0
130.90	186.0
134.70	273.0
135.10	239.0
136.90	363.0
140.00	214.0
141.00	1347.0
142.00	170.0
142.90	1877.0
143.80	103.0
144.90	434.0
146.00	278.0
147.90	521.0
148.80	215.0
153.00	105.0
154.00	208.0
154.90	370.0
156.80	444.0
158.80	182.0
161.00	300.0
171.00	228.0
172.10	1079.0
174.00	121848.0
175.00	9414.0
176.00	115456.0
177.00	7868.0
207.40	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	1825.0
37.00	8575.0
38.00	7857.0
39.00	3393.0
40.00	4910.0
42.90	123.0
44.00	2204.0
45.00	1643.0
46.10	213.0
47.00	2365.0
47.90	1089.0
49.00	6727.0
50.10	33656.0
51.00	10679.0
52.00	500.0
53.00	175.0
55.10	707.0
56.00	2108.0
57.00	4554.0
58.00	223.0
60.00	1356.0
61.10	8304.0
62.10	7982.0
63.10	6810.0
64.10	1109.0
65.00	894.0
67.10	492.0
68.10	15359.0
69.10	17080.0
70.00	1156.0
72.00	826.0
73.00	8060.0
74.10	27504.0
75.10	84944.0
76.10	6807.0
77.10	933.0
78.00	596.0
78.90	4863.0
80.00	1166.0
80.90	4468.0
82.00	849.0
82.80	104.0
85.80	158.0
87.00	6857.0
88.00	6473.0
91.00	482.0
92.00	4783.0
93.00	6333.0
94.10	19536.0
95.10	168384.0
96.10	11477.0
97.30	219.0
103.80	703.0
104.70	242.0
106.00	575.0
115.00	106.0
116.10	479.0
116.90	1270.0
118.00	654.0
119.00	752.0
128.00	395.0
128.90	332.0
129.90	605.0
130.90	183.0
134.80	234.0
135.10	301.0
137.00	394.0
140.00	212.0
141.00	1431.0
141.90	114.0
142.90	1717.0
144.90	461.0
145.90	253.0
147.90	516.0
148.80	156.0
153.00	179.0
154.00	120.0
155.00	334.0
156.80	479.0
158.80	255.0
161.00	211.0
171.00	158.0
172.10	1077.0
174.00	122096.0
175.00	8965.0
176.00	116624.0
177.00	7199.0
207.30	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

Scan 2853 (10.263 min): VU031669.D
BFB35

m/z	Abundance
40.00	4305.0
41.20	148.0
44.00	1616.0
73.10	203.0
207.20	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35