

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054015.D
 Acq On : 01 May 2023 10:33
 Operator : JC/MD
 Sample : VU0501MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK083

Quant Time: May 02 05:30:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 02 05:29:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	259655	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	239734	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	116771	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	93346	47.533	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	95.060%		
7) Chloroethane-d5	1.912	69	60684	47.076	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.160%		
11) 1,1-Dichloroethene-d2	2.562	63	128600	36.921	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.840%		
21) 2-Butanone-d5	4.623	46	117507	104.914	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	104.910%		
24) Chloroform-d	5.057	84	169744	47.063	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.120%		
26) 1,2-Dichloroethane-d4	5.693	65	113251	48.905	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.800%		
32) Benzene-d6	5.722	84	342671	48.560	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.120%		
36) 1,2-Dichloropropane-d6	6.684	67	110549	49.625	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.240%		
41) Toluene-d8	7.893	98	304353	47.773	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.540%		
43) trans-1,3-Dichloroprop...	8.172	79	46792	42.444	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.880%		
47) 2-Hexanone-d5	8.629	63	79083	99.114	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.110%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	144828	49.356	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.720%		
66) 1,2-Dichlorobenzene-d4	12.188	152	121506	53.265	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.520%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.565	101	1151	0.662	ug/L	# 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054015.D
Acq On : 01 May 2023 10:33
Operator : JC/MD
Sample : VU0501MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK083

Quant Time: May 02 05:30:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 02 05:29:54 2023
Response via : Initial Calibration

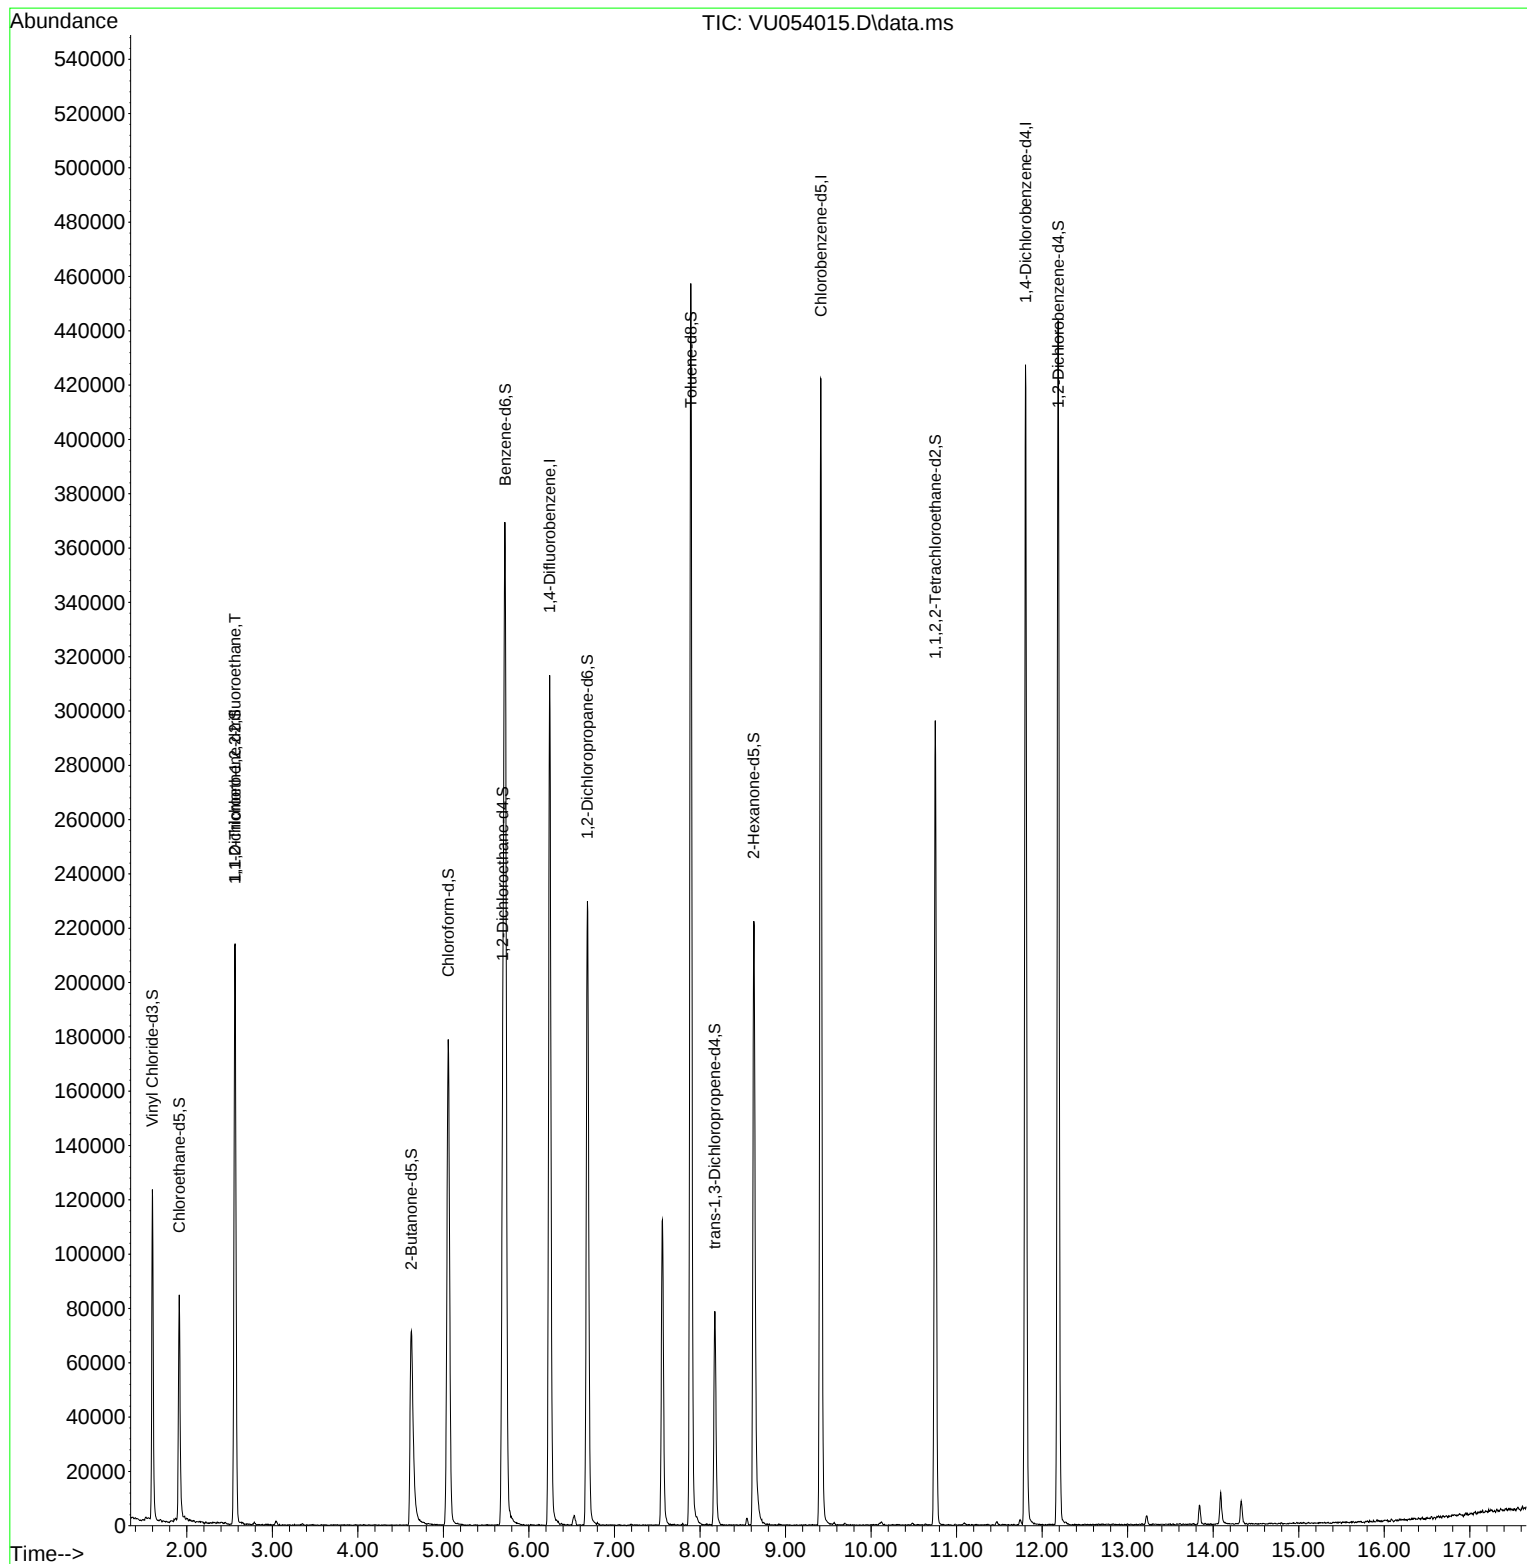

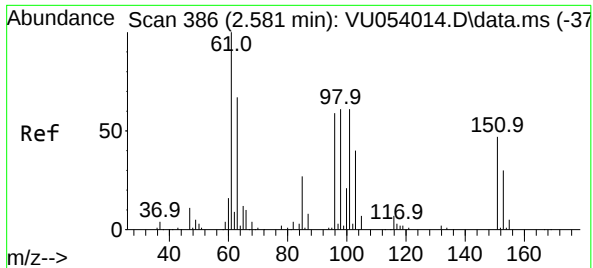

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.662 ug/L
 RT: 2.565 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VU054015.D
 Acq: 01 May 2023 10:33

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK083

Tgt Ion:101 Resp: 1151
 Ion Ratio Lower Upper
 101 100
 85 0.0 34.3 51.5#
 151 0.0 60.3 90.5#

