

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054038.D
 Acq On : 01 May 2023 20:02
 Operator : JC/MD
 Sample : 02548-31ME
 Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCR1ME

Quant Time: May 02 05:35:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 02 05:29:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	252157	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.410	117	244099	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	120457	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	77926	40.861	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.720%		
7) Chloroethane-d5	1.906	69	60652	48.450	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.900%		
11) 1,1-Dichloroethene-d2	2.562	63	111908	33.084	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.160%		
21) 2-Butanone-d5	4.616	46	107981	99.276	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.280%		
24) Chloroform-d	5.057	84	159450	45.523	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.040%		
26) 1,2-Dichloroethane-d4	5.694	65	107694	47.888	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.780%		
32) Benzene-d6	5.719	84	322481	44.882	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.760%		
36) 1,2-Dichloropropane-d6	6.684	67	102435	45.160	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.320%		
41) Toluene-d8	7.893	98	284445	43.849	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.700%		
43) trans-1,3-Dichloroprop...	8.173	79	47694	42.489	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.980%		
47) 2-Hexanone-d5	8.629	63	74321	91.480	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.480%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	140530	47.035	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.080%		
66) 1,2-Dichlorobenzene-d4	12.188	152	116391	49.461	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.920%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	6.684	63	11134	5.539	ug/L #	87
60) 1,2,3-Trichloropropane	11.806	75	13328	5.957	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054038.D
Acq On : 01 May 2023 20:02
Operator : JC/MD
Sample : 02548-31ME
Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCR1ME

Quant Time: May 02 05:35:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 02 05:29:54 2023
Response via : Initial Calibration

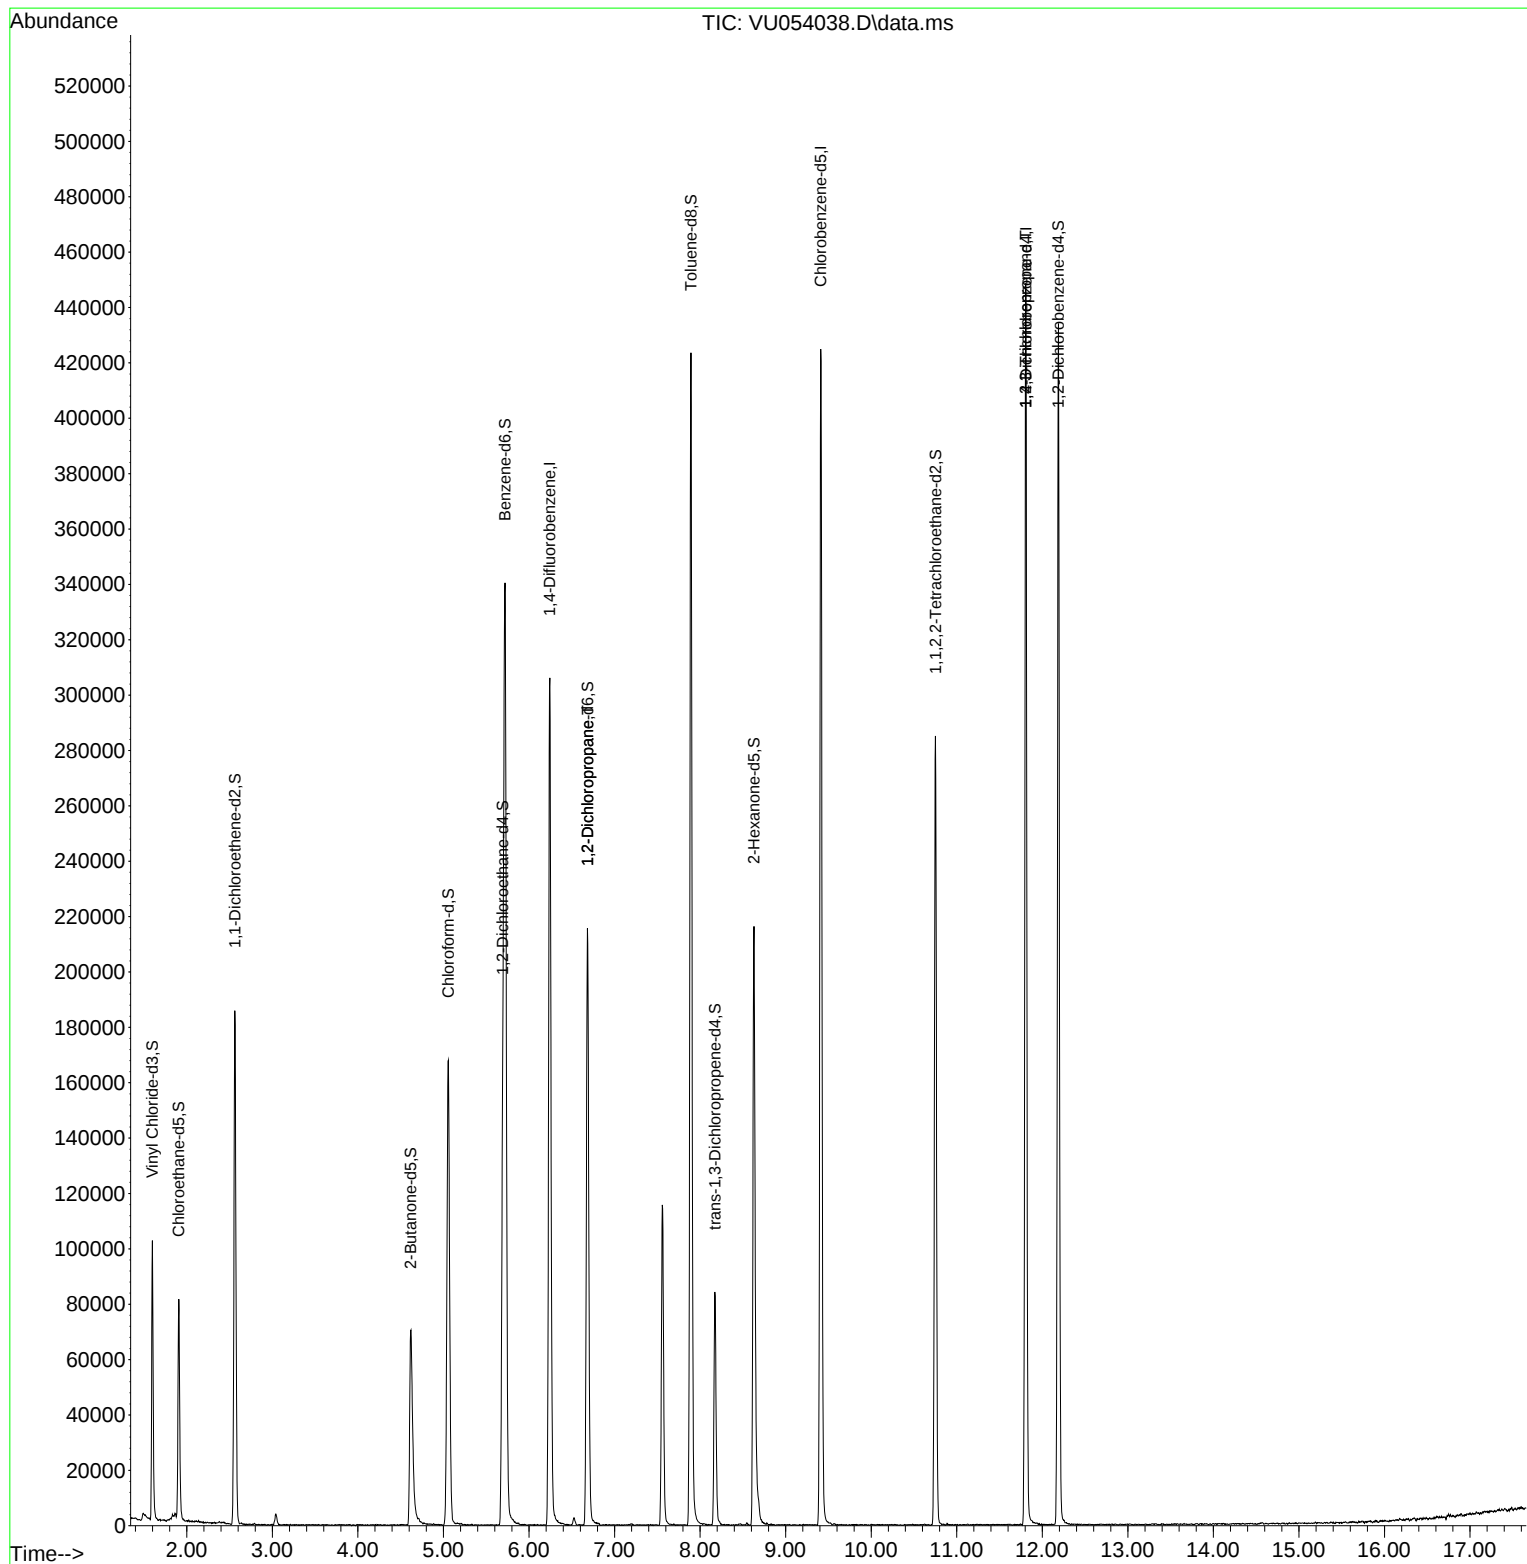

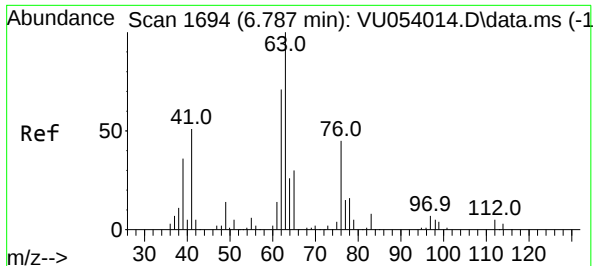

#37

1,2-Dichloropropane

Concen: 5.539 ug/L

RT: 6.684 min Scan# 1

Delta R.T. -0.103 min

Lab File: VU054038.D

Acq: 01 May 2023 20:02

Instrument :

MSVOA_U

ClientSampleId :





DCCR1ME

Tgt Ion: 63 Resp: 11134

Ion Ratio Lower Upper

63 100

112 0.0 3.4 5.0#

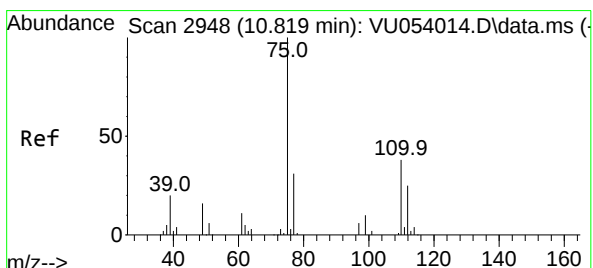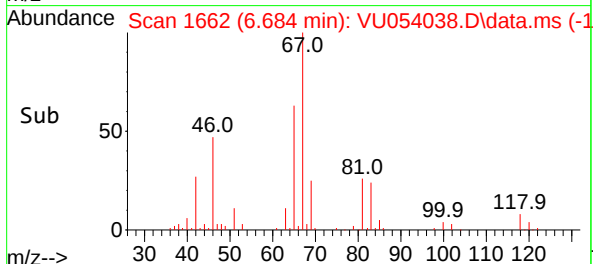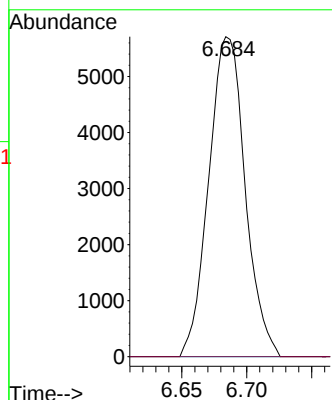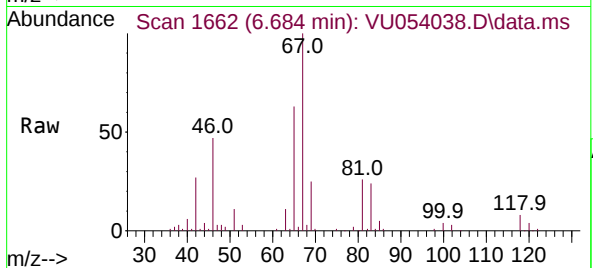

#60

1,2,3-Trichloropropane

Concen: 5.957 ug/L

RT: 11.806 min Scan# 3255

Delta R.T. 0.987 min

Lab File: VU054038.D

Acq: 01 May 2023 20:02

Tgt Ion: 75 Resp: 13328

Ion Ratio Lower Upper

75 100

77 32.1 26.0 39.0

110 2.7 31.8 47.8#

